

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV042420\
 Data File : VV015668.D
 Acq On : 24 Apr 2020 10:43
 Operator : SY/MD
 Sample : VV0424WBL01
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK44

Quant Time: Apr 25 00:35:33 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR042220WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Apr 25 00:15:39 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	132113	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	127536	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	62484	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.31	65	30897	4.48	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	89.60%
7) Chloroethane-d5	1.57	69	30799	4.63	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	92.60%
11) 1,1-Dichloroethene-d2	2.12	63	48615	3.22	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	64.40%
20) 2-Butanone-d5	3.94	46	113170	51.05	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	102.10%
24) Chloroform-d	4.38	84	75238	4.68	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.60%
26) 1,2-Dichloroethane-d4	5.06	65	44482	4.94	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	98.80%
32) Benzene-d6	5.07	84	144065	4.73	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.60%
36) 1,2-Dichloropropane-d6	6.09	67	46050	4.73	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	94.60%
41) Toluene-d8	7.34	98	133406	4.61	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.20%
43) trans-1,3-Dichloropropene-	7.64	79	15503	4.12	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	82.40%
46) 2-Hexanone-d5	8.11	63	84968	46.32	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	92.64%
57) 1,1,2,2-Tetrachloroethane-	10.24	84	33464	4.62	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	92.40%
64) 1,2-Dichlorobenzene-d4	11.65	152	51605	4.86	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	97.20%


Target Compounds					Ovalue
25) Chloroform	4.40	83	3810	0.212 ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV042420\
Data File : VV015668.D
Acq On : 24 Apr 2020 10:43
Operator : SY/MD
Sample : VV0424WBL01
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK44

Quant Time: Apr 25 00:35:33 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR042220WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Apr 25 00:15:39 2020
Response via : Initial Calibration

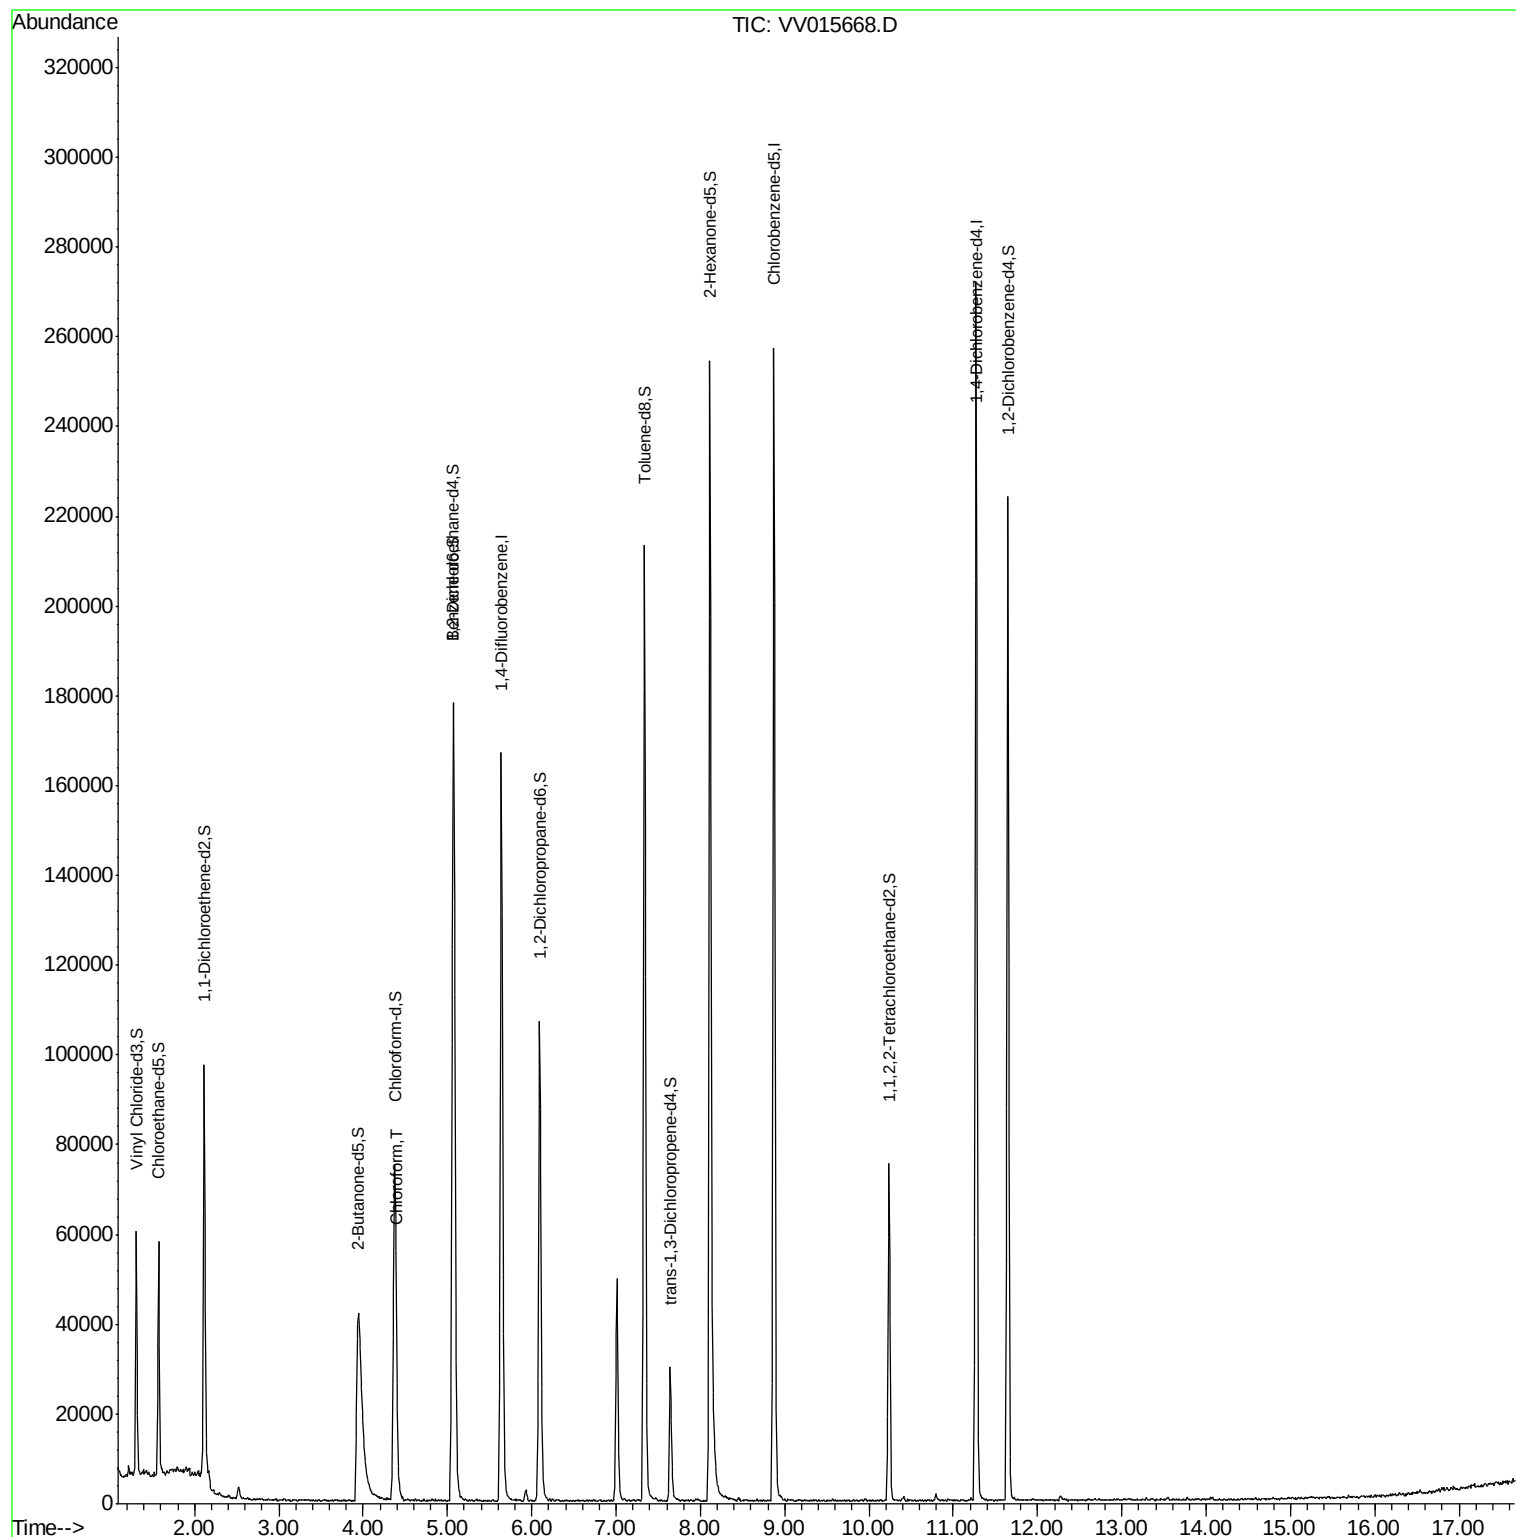

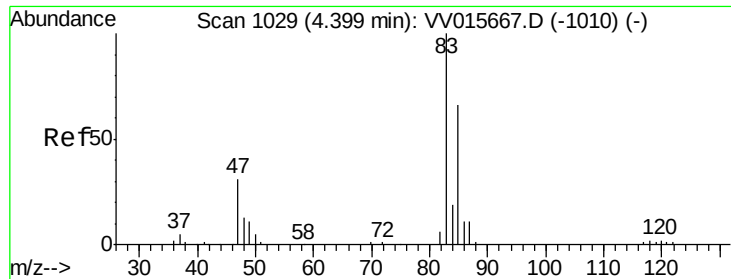

#25
 Chloroform
 Concen: 0.212 ug/L
 RT: 4.40 min Scan# 1030
 Delta R.T. 0.00 min
 Lab File: VV015668.D
 Acq: 24 Apr 2020 10:43

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK44

Tot Ion: 83 Resp: 3810
 Ion Ratio Lower Upper
 83 100
 85 71.6 46.1 85.5

