


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV042420\
 Data File : VV015666.D
 Acq On : 24 Apr 2020 09:09
 Operator : SY/MD
 Sample : BFB42
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB42

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR042220WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Mon Apr 27 12:28:46 2020

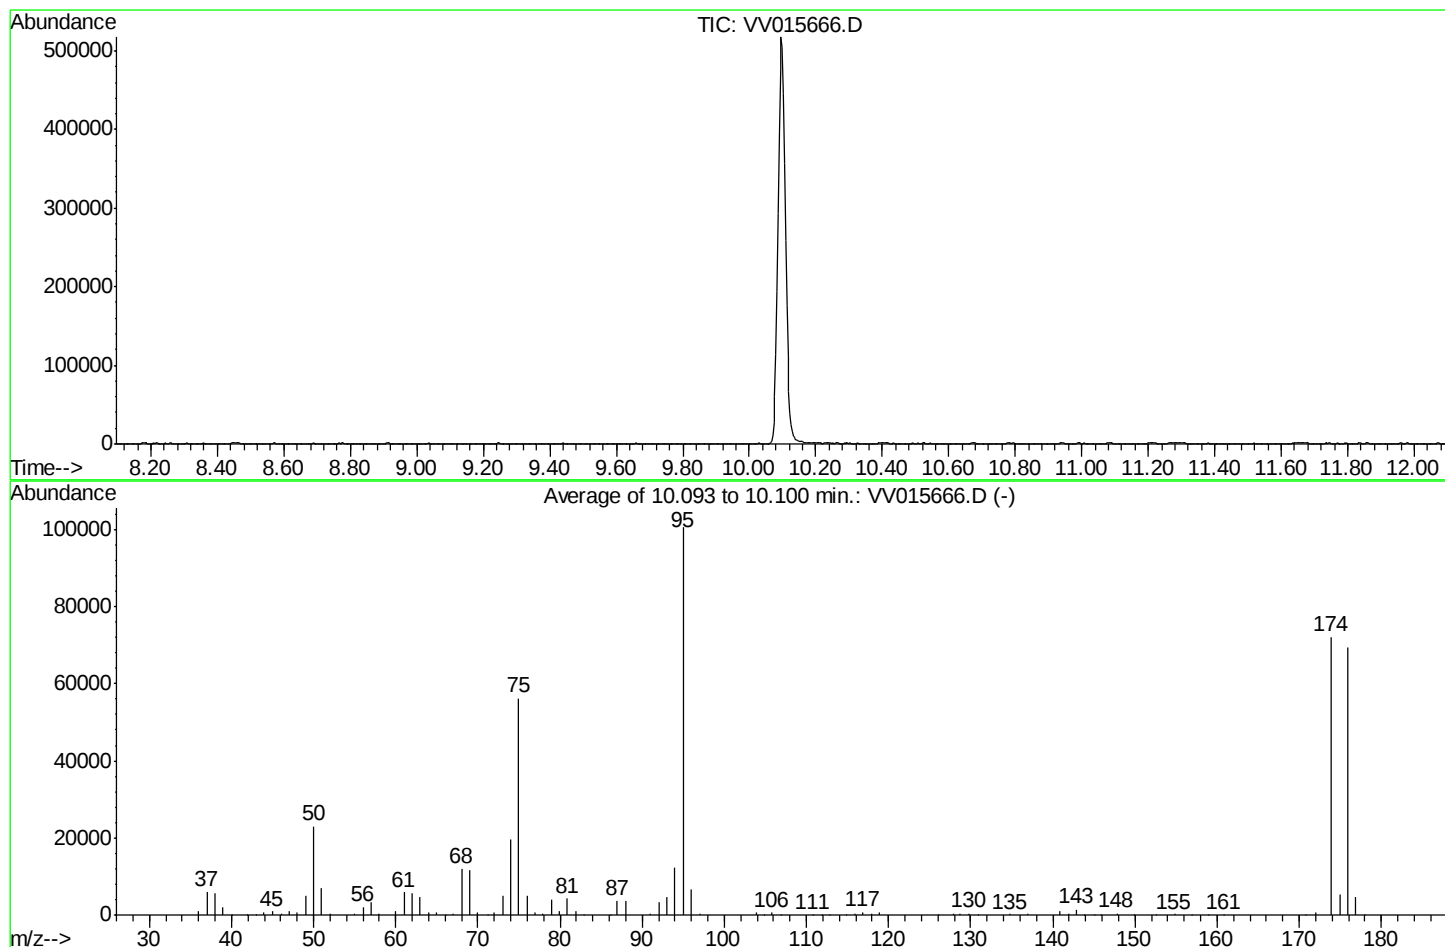

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2787

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.9	23074	PASS
75	95	30	80	55.9	56216	PASS
95	95	100	100	100.0	100576	PASS
96	95	5	9	6.7	6761	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	71.7	72141	PASS
175	174	5	9	7.5	5413	PASS
176	174	95	101	96.1	69296	PASS
177	176	5	9	6.9	4800	PASS

m/z	Abundance
36.00	1013.0
37.00	5907.0
38.00	5548.0
39.00	2073.0
40.00	329.0
41.90	103.0
43.00	127.0
44.00	1105.0
45.00	902.0
46.20	188.0
47.10	1065.0
48.00	784.0
49.00	4734.0
50.00	22640.0
51.00	6814.0
52.00	282.0
54.90	355.0
56.00	2057.0
57.00	3430.0
57.90	199.0
59.90	1084.0
61.00	5628.0
62.00	5291.0
63.00	4473.0
64.00	557.0
65.00	511.0
67.00	325.0
68.00	11712.0
69.00	11519.0
70.00	751.0
71.20	102.0
72.00	578.0
73.00	4898.0
74.00	18816.0
75.00	53920.0
76.00	4808.0
77.00	591.0
77.90	374.0
78.90	3936.0
79.90	1032.0
80.90	4190.0
81.90	908.0
86.10	128.0
86.90	3575.0
88.00	3419.0
90.90	464.0
92.00	3097.0
93.00	4629.0
94.00	11825.0
95.00	96472.0
96.00	6582.0
97.10	206.0
103.90	468.0
104.90	167.0
105.90	542.0
106.80	152.0
110.80	113.0
112.90	108.0
114.80	128.0
115.80	467.0
116.90	715.0
117.90	386.0
118.90	614.0
127.90	305.0
128.80	187.0
129.80	375.0
130.90	165.0
134.80	238.0
136.90	192.0
140.90	1087.0
141.80	200.0
142.90	1266.0
143.80	131.0
145.10	150.0
145.90	132.0
147.80	400.0
154.90	213.0
156.90	181.0
158.80	115.0
160.90	121.0
172.00	621.0
173.90	67472.0
174.90	5124.0
175.90	64608.0
176.90	4472.0
177.90	141.0

Instrument :
MSVOA_V
ClientSampleId :
BFB42

m/z	Abundance
36.00	1161.0
37.00	6259.0
38.00	5688.0
39.00	2230.0
40.00	317.0
41.90	102.0
43.00	140.0
44.00	1134.0
45.00	1018.0
46.20	195.0
47.10	1193.0
48.00	806.0
49.00	5112.0
50.00	23896.0
51.00	7357.0
52.00	287.0
55.00	390.0
56.00	2144.0
57.00	3565.0
57.90	214.0
60.00	1159.0
61.00	5993.0
62.00	5710.0
63.00	4856.0
64.00	583.0
65.00	553.0
67.10	309.0
68.00	12603.0
69.00	12117.0
70.00	832.0
72.00	660.0
73.00	5062.0
74.00	20192.0
75.00	58248.0
76.00	5221.0
77.00	620.0
77.90	386.0
78.90	4129.0
79.90	1134.0
80.90	4413.0
81.90	945.0
82.90	105.0
86.10	102.0
87.00	3781.0
88.00	3674.0
90.90	520.0
92.00	3354.0
93.00	5001.0
94.00	12833.0
95.00	104072.0
96.00	7003.0
97.10	192.0
103.90	535.0
104.90	171.0
105.90	555.0
106.80	136.0
110.80	155.0
111.80	108.0
112.90	111.0
114.90	153.0
115.90	483.0
116.90	770.0
117.90	421.0
118.90	673.0
126.00	105.0
127.90	348.0
128.70	185.0
129.80	401.0
130.90	147.0
134.80	285.0
136.90	232.0
140.90	1125.0
141.90	205.0
142.90	1394.0
143.80	143.0
145.10	160.0
145.90	140.0
147.90	414.0
152.60	108.0
154.80	228.0
156.90	170.0
158.80	115.0
160.80	113.0
172.00	702.0
173.90	74688.0
174.90	5603.0
175.90	71760.0
176.90	5011.0
177.90	149.0

Instrument :
MSVOA_V
ClientSampleId :
BFB42

m/z	Abundance
36.00	1155.0
37.00	5899.0
38.00	5398.0
39.00	2074.0
40.00	328.0
41.90	105.0
43.00	144.0
44.00	1076.0
45.00	1049.0
46.10	177.0
47.10	1237.0
48.00	749.0
49.00	5102.0
50.00	22688.0
51.00	7071.0
52.00	313.0
55.00	376.0
56.00	2028.0
57.00	3265.0
57.90	204.0
60.00	1106.0
61.00	5860.0
62.00	5684.0
63.00	4727.0
64.00	572.0
65.00	547.0
66.10	103.0
66.90	277.0
68.00	12042.0
69.00	11659.0
70.00	890.0
72.00	682.0
73.00	4861.0
74.00	19600.0
75.00	56480.0
76.00	5033.0
77.00	645.0
78.00	367.0
78.90	3996.0
79.90	1162.0
80.90	4142.0
81.90	939.0
82.90	126.0
87.00	3773.0
88.00	3565.0
90.90	532.0
92.00	3206.0
93.00	4731.0
94.00	12577.0
95.00	101184.0
96.00	6700.0
97.00	166.0
103.90	580.0
104.90	173.0
105.80	494.0
106.80	119.0
110.80	151.0
111.80	114.0
112.80	104.0
114.80	161.0
115.80	443.0
116.90	739.0
117.90	436.0
118.90	730.0
127.90	354.0
128.70	186.0
129.90	352.0
130.90	144.0
134.80	264.0
136.90	228.0
140.80	1129.0
141.90	177.0
142.90	1339.0
143.80	129.0
145.00	150.0
145.90	127.0
147.90	346.0
149.90	105.0
154.80	225.0
156.80	154.0
158.90	116.0
160.70	116.0
170.80	103.0
171.90	686.0
173.90	74264.0
175.00	5512.0
175.90	71520.0
176.90	4918.0
177.90	151.0

Instrument :
MSVOA_V
ClientSampleId :
BFB42

Scan 2787 (10.051 min): VV015666.D
BFB42

m/z	Abundance
39.90	319.0
43.90	425.0

Instrument :
MSVOA_V
ClientSampleId :
BFB42