

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
 Data File : VV030782.D
 Acq On : 24 Apr 2023 10:51
 Operator : SY/MD
 Sample : VV0424MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK330

Quant Time: Apr 25 03:21:26 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Apr 22 00:43:23 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.542	114	245115	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.792	117	237591	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152	115850	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.281	65	65696	36.561	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	73.120%		
7) Chloroethane-d5	1.535	69	56890	37.781	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	75.560%		
11) 1,1-Dichloroethene-d2	2.063	65	34505	40.492	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	80.980%		
21) 2-Butanone-d5	3.799	46	93679	94.917	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	94.920%		
24) Chloroform-d	4.259	84	140573	43.169	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	86.340%		
26) 1,2-Dichloroethane-d4	4.950	65	97383	46.515	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	93.020%		
32) Benzene-d6	4.969	84	254052	45.227	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	90.460%		
36) 1,2-Dichloropropane-d6	5.995	67	78791	45.155	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	90.320%		
41) Toluene-d8	7.252	98	225130	42.686	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	85.380%		
43) trans-1,3-Dichloroprop...	7.561	79	37924	43.122	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	86.240%		
47) 2-Hexanone-d5	8.034	63	56298	81.902	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	81.900%		
56) 1,1,2,2-Tetrachloroeth...	10.162	84	110415	43.609	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	87.220%		
66) 1,2-Dichlorobenzene-d4	11.567	152	93020	50.516	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	101.040%		
Target Compounds					Qvalue	
71) Naphthalene	13.451	128	5613	0.884	ug/L #	86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
Data File : VV030782.D
Acq On : 24 Apr 2023 10:51
Operator : SY/MD
Sample : VV042424MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK330

Quant Time: Apr 25 03:21:26 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Apr 22 00:43:23 2023
Response via : Initial Calibration

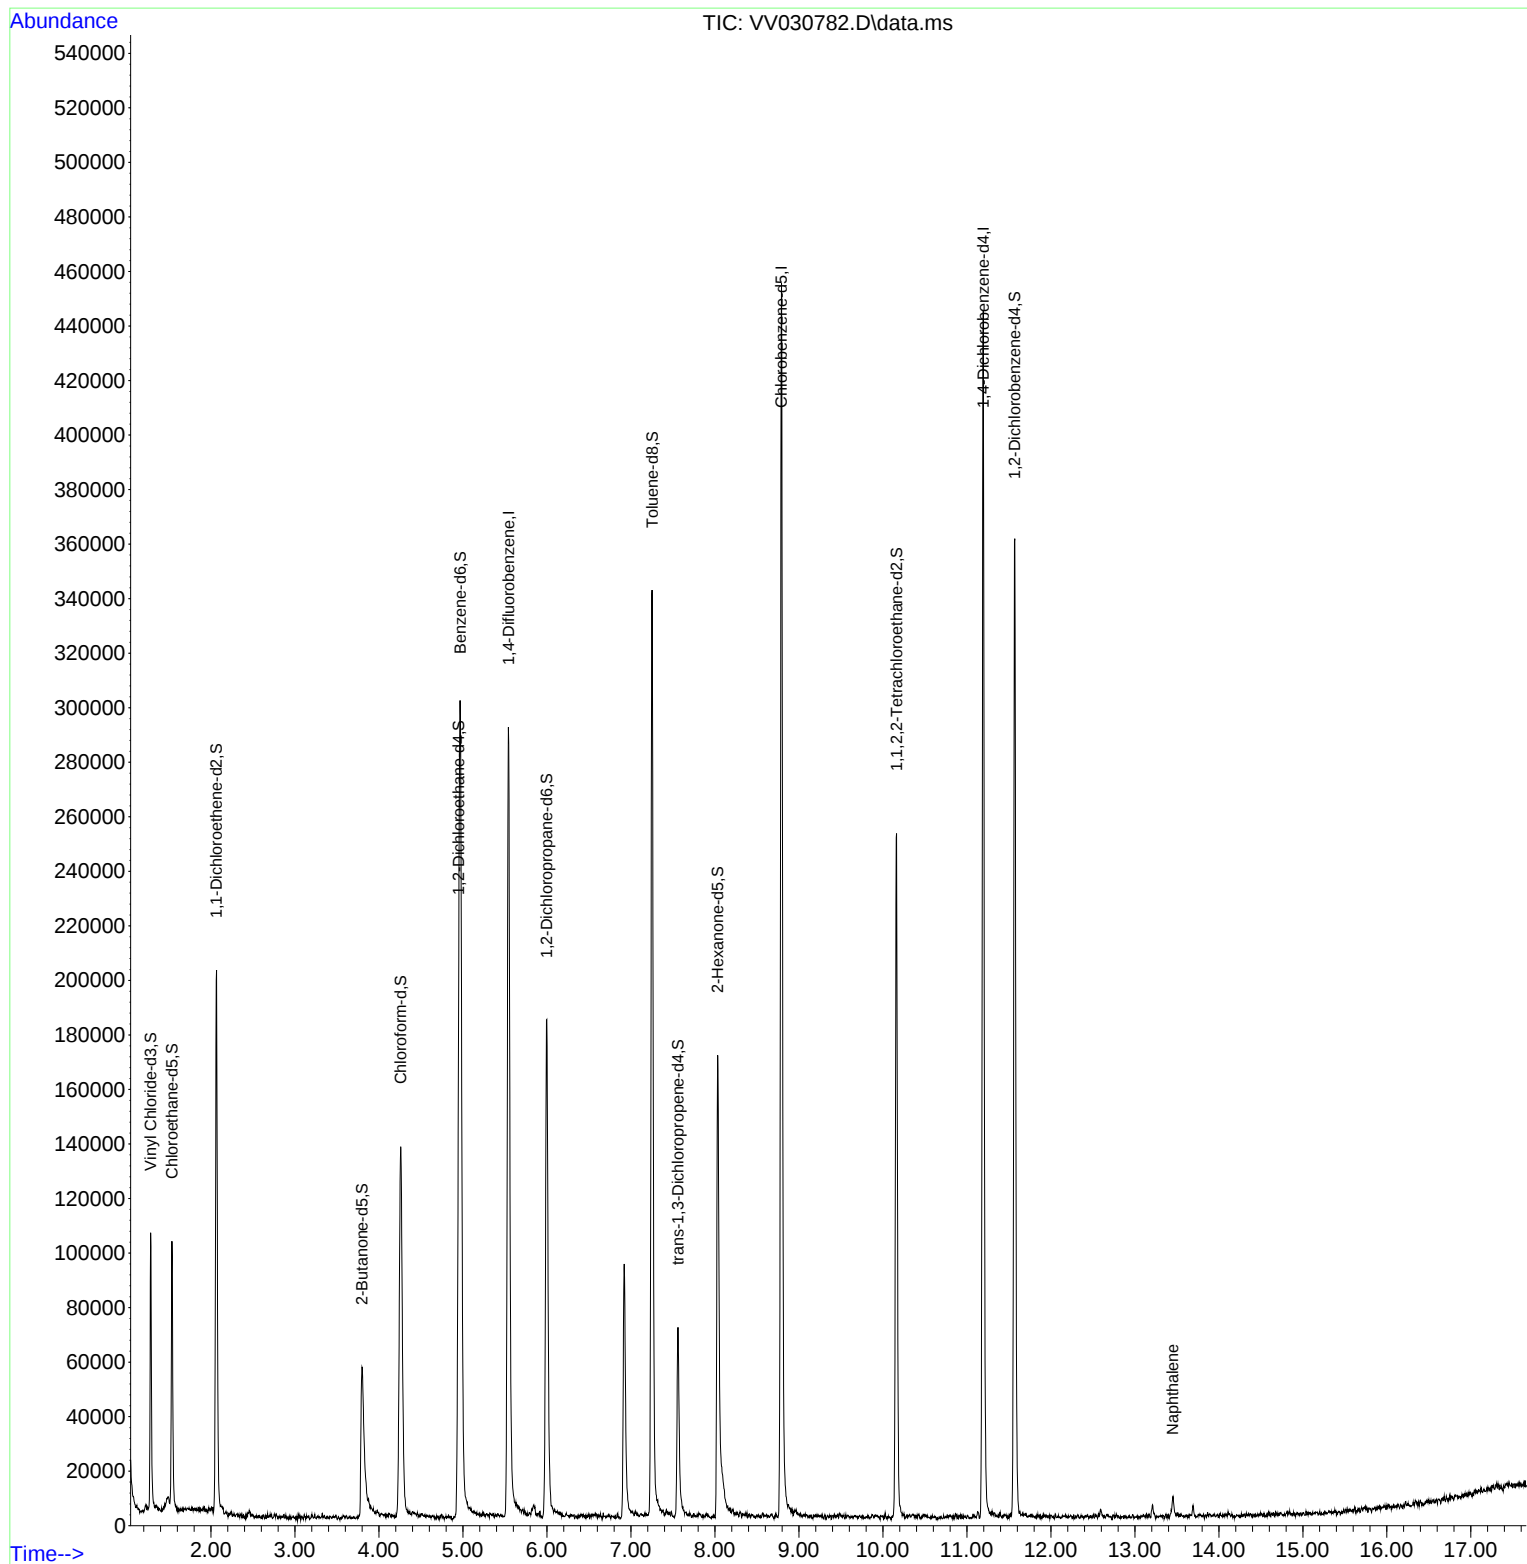

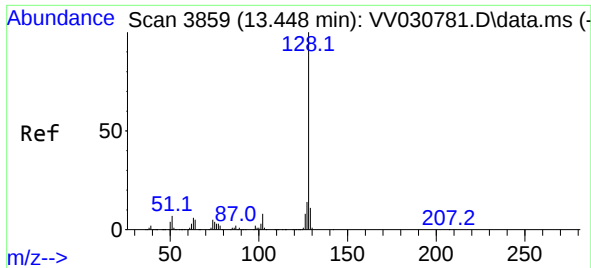

#71
Naphthalene
Concen: 0.884 ug/L
RT: 13.451 min Scan# 3860
Delta R.T. 0.003 min
Lab File: VV030782.D
Acq: 24 Apr 2023 10:51

Instrument :
MSVOA_V
ClientSampleId :
VBLK330

Tgt Ion	Ratio	Lower	Upper
128	100		
127	11.8	10.7	16.1
129	0.9	8.6	13.0#

