

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042423\
 Data File : VW030798.D
 Acq On : 24 Apr 2023 17:22
 Operator : SY/MD
 Sample : 02440-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMR3

Quant Time: Apr 25 03:23:29 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Apr 22 00:43:23 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.542	114	235661	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.792	117	234471	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152	112988	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.281	65	55596	32.181	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	64.360%		
7) Chloroethane-d5	1.539	69	52283	36.114	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	72.220%		
11) 1,1-Dichloroethene-d2	2.066	65	29632	36.169	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	72.340%		
21) 2-Butanone-d5	3.809	46	90647	95.530	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	95.530%		
24) Chloroform-d	4.259	84	128019	40.890	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	81.780%		
26) 1,2-Dichloroethane-d4	4.953	65	90829	45.125	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	90.240%		
32) Benzene-d6	4.969	84	230460	41.573	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	83.140%		
36) 1,2-Dichloropropane-d6	5.998	67	72684	42.210	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	84.420%		
41) Toluene-d8	7.252	98	205081	39.402	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	78.800%#		
43) trans-1,3-Dichloroprop...	7.561	79	32139	37.030	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	74.060%		
47) 2-Hexanone-d5	8.034	63	54947	81.001	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	81.000%		
56) 1,1,2,2-Tetrachloroeth...	10.159	84	105030	42.034	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	84.060%		
66) 1,2-Dichlorobenzene-d4	11.570	152	85398	47.552	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	95.100%		
Target Compounds						Qvalue
44) trans-1,3-Dichloropropene	7.561	75	2077	0.735	ug/L	# 71


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
Data File : VV030798.D
Acq On : 24 Apr 2023 17:22
Operator : SY/MD
Sample : 02440-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMR3

Quant Time: Apr 25 03:23:29 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Apr 22 00:43:23 2023
Response via : Initial Calibration

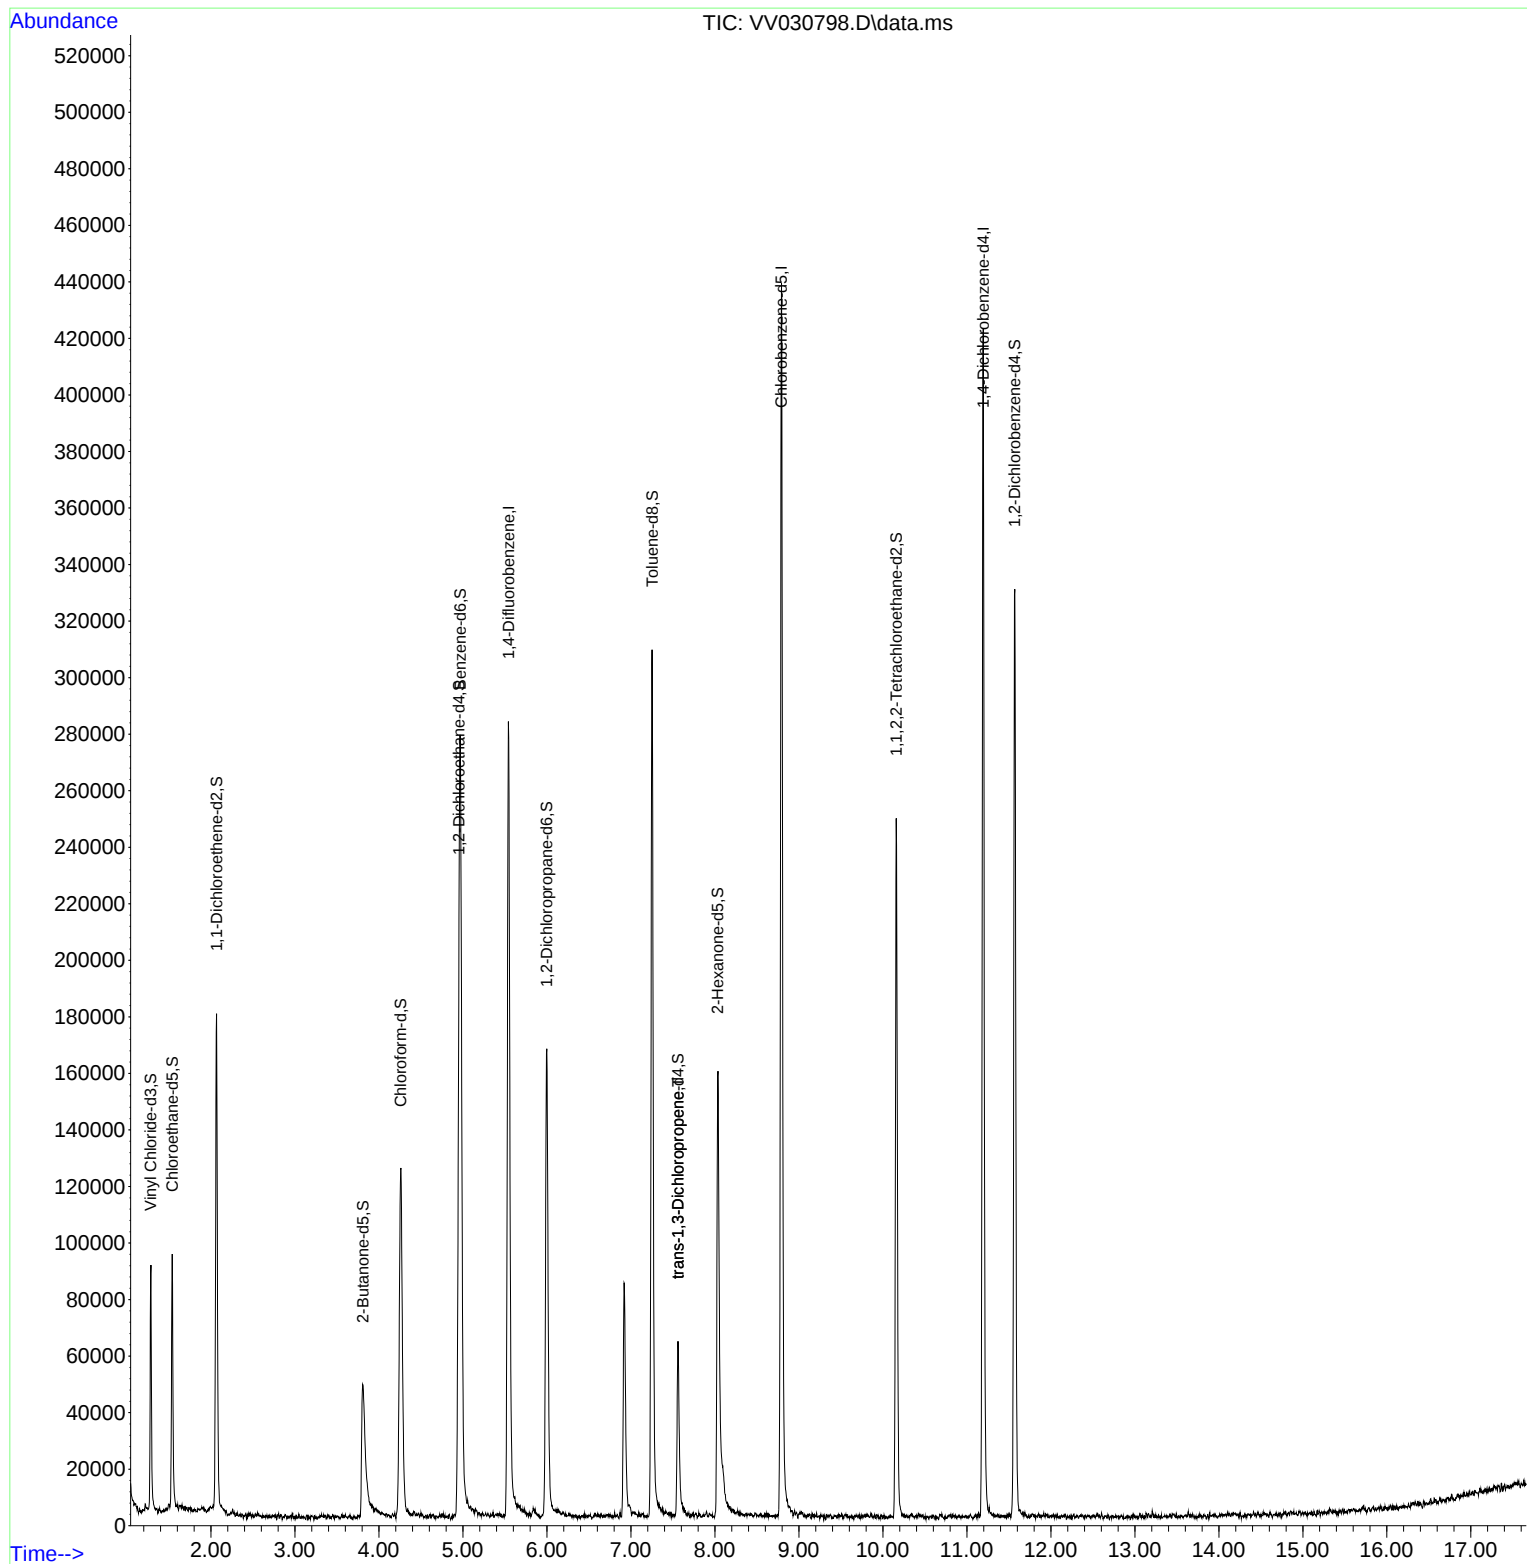

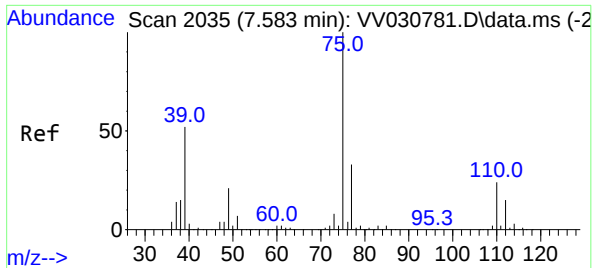

#44
 trans-1,3-Dichloropropene
 Concen: 0.735 ug/L
 RT: 7.561 min Scan# 20
 Delta R.T. -0.026 min
 Lab File: VV030798.D
 Acq: 24 Apr 2023 17:22

Instrument :
 MSVOA_V
 ClientSampleId :
 COMR3

Tgt Ion: 75 Resp: 2077
 Ion Ratio Lower Upper
 75 100
 77 47.7 22.1 41.1#

