




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
 Data File : VV030819.D
 Acq On : 25 Apr 2023 02:19
 Operator : SY/MD
 Sample : 02417-16ME
 Misc : 5.44g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW8Y2ME

Manual IntegrationsAPPROVED

Quant Time: Apr 25 05:32:04 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Apr 22 00:43:23 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 04/26/2023
 Supervised By :Mahesh Dadoda 04/26/2023

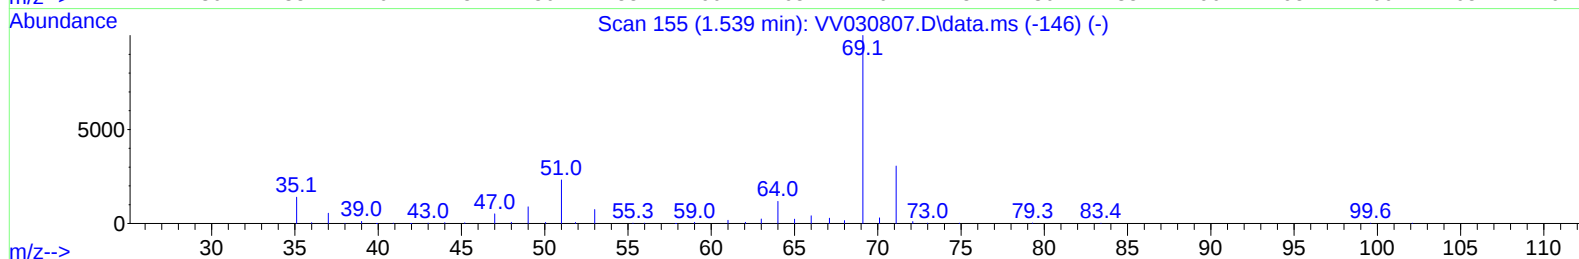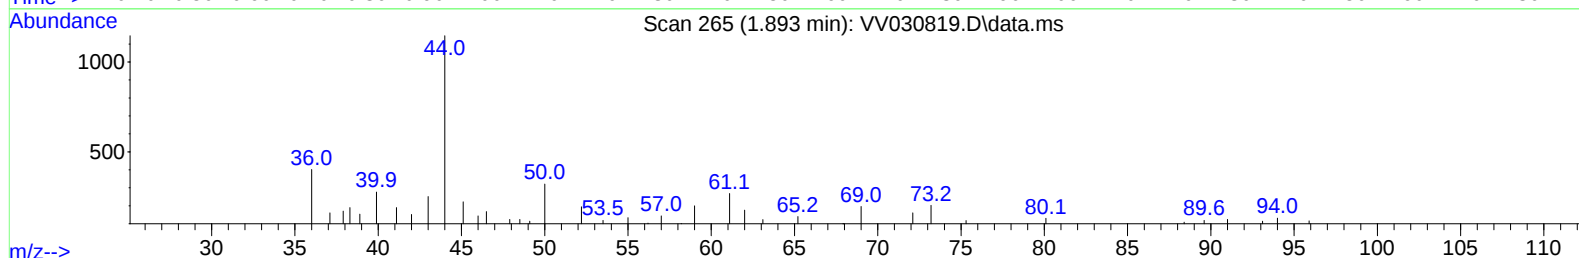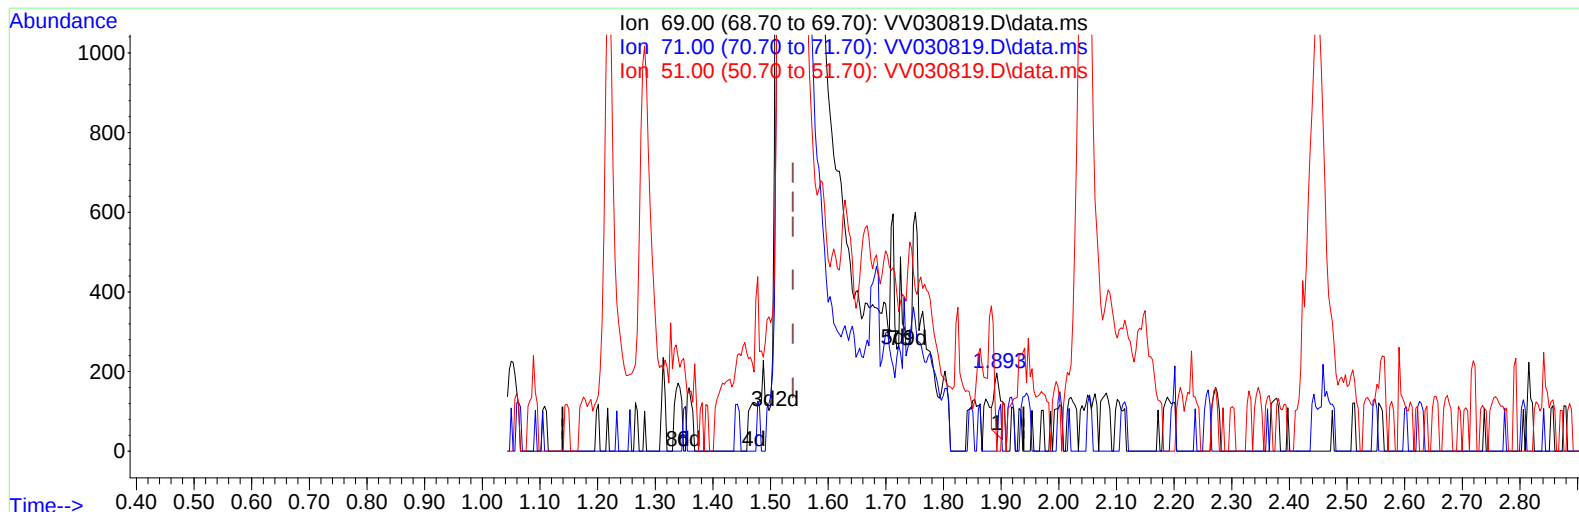

TIC: VV030819.D\data.ms

(7) Chloroethane-d5 (S)

1.893min (+ 0.354) 0.08 ug/L

response 126

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	32.00	33.33
51.00	30.70	35.71
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
 Data File : VV030819.D
 Acq On : 25 Apr 2023 02:19
 Operator : SY/MD
 Sample : 02417-16ME
 Misc : 5.44g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW8Y2ME

Manual IntegrationsAPPROVED

Quant Time: Apr 25 05:32:04 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Apr 22 00:43:23 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 04/26/2023
 Supervised By :Mahesh Dadoda 04/26/2023

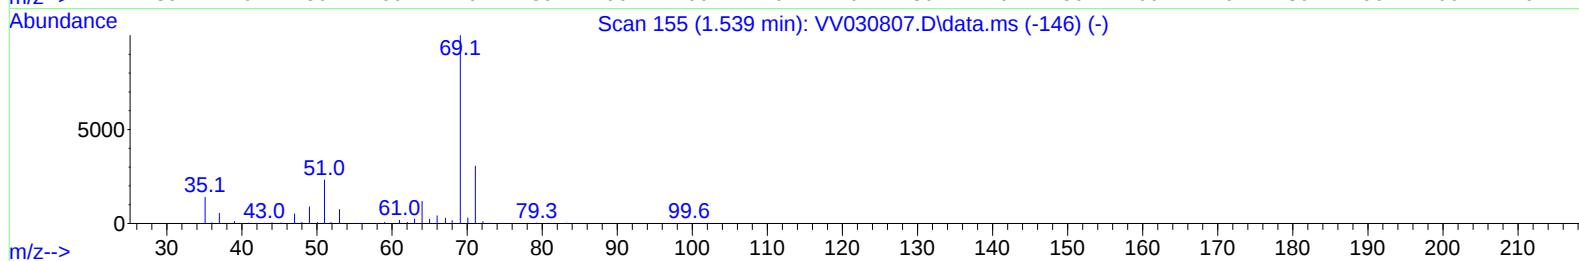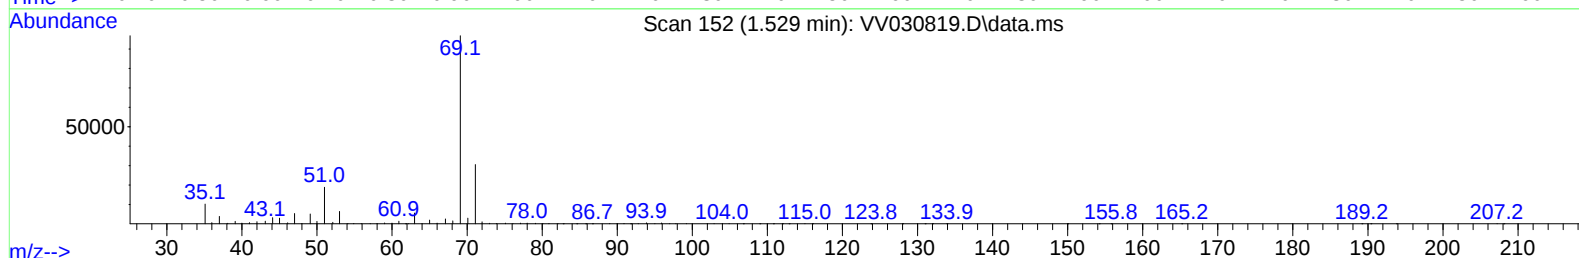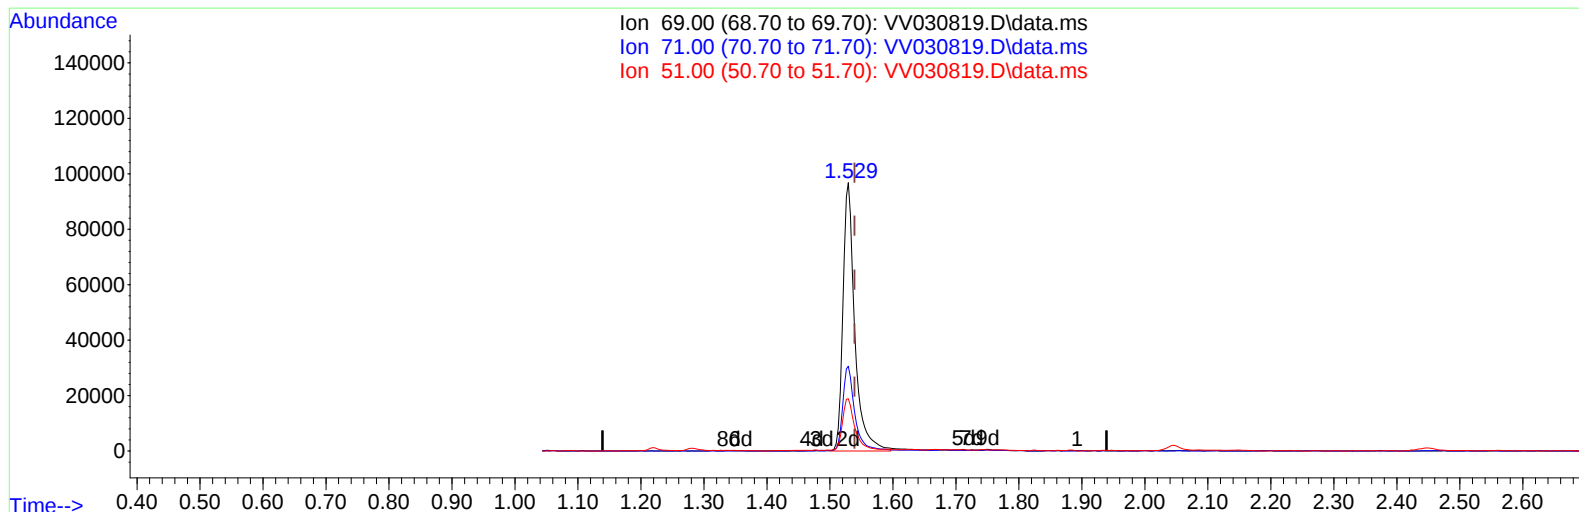

TIC: VV030819.D\data.ms

(7) Chloroethane-d5 (S)

1.529min (-0.010) 79.49 ug/L m

response 126628

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	32.00	0.03#
51.00	30.70	0.04#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
 Data File : VV030819.D
 Acq On : 25 Apr 2023 02:19
 Operator : SY/MD
 Sample : 02417-16ME
 Misc : 5.44g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW8Y2ME

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 04/26/2023
 Supervised By :Mahesh Dadoda 04/26/2023

Quant Time: Apr 25 05:32:04 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Apr 22 00:43:23 2023
 Response via : Initial Calibration

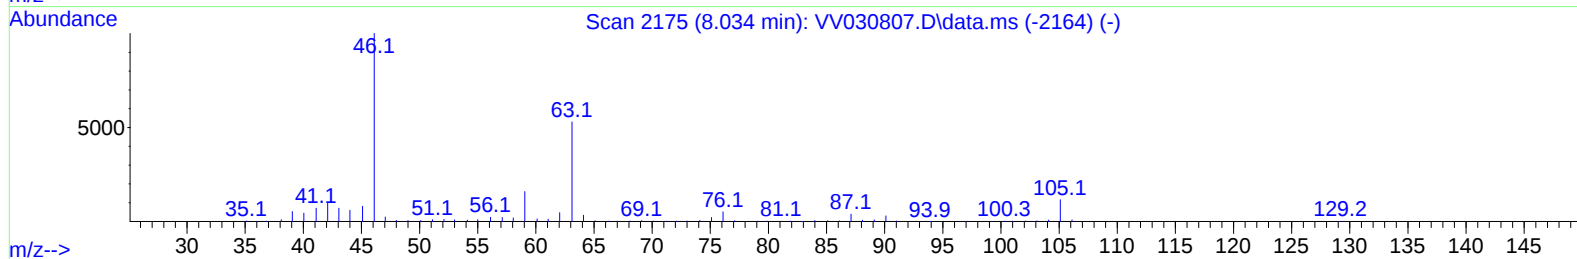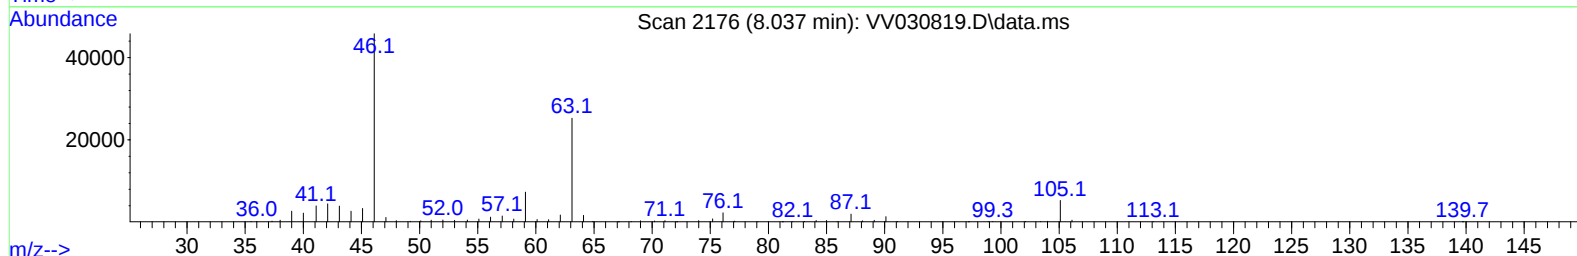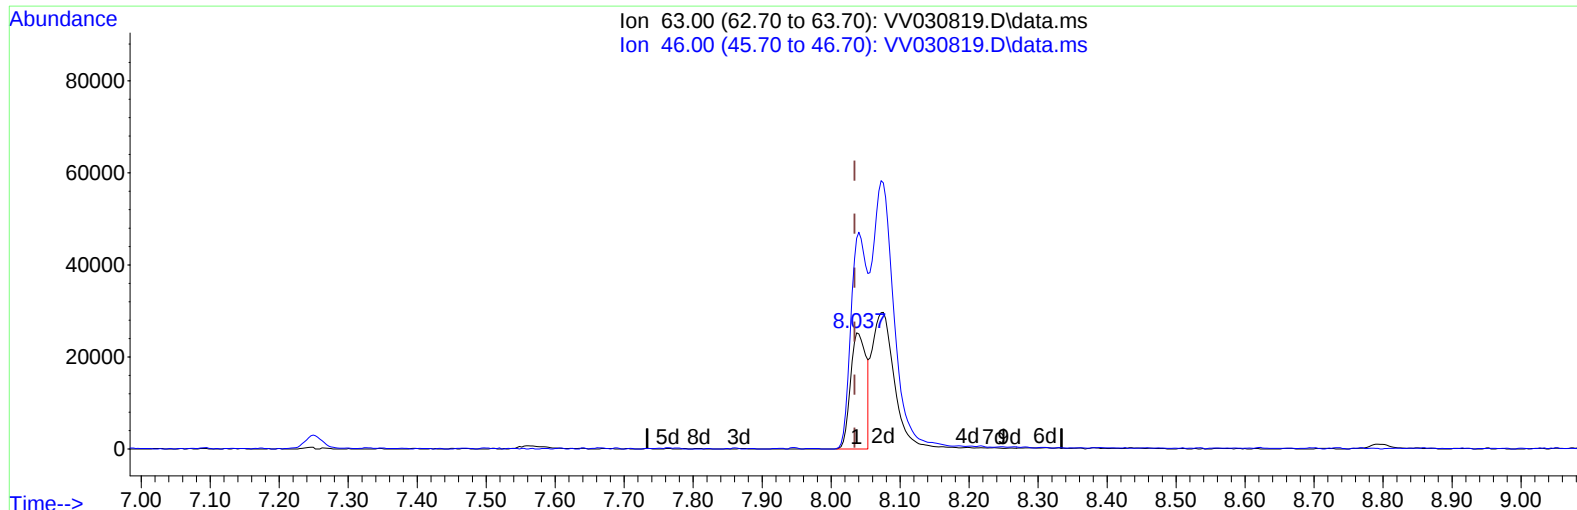

TIC: VV030819.D\data.ms

(47) 2-Hexanone-d5 (S)

8.037min (+ 0.003) 54.46 ug/L

response 39873

Ion	Exp%	Act%
63.00	100.00	100.00
46.00	190.80	187.46
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
 Data File : VV030819.D
 Acq On : 25 Apr 2023 02:19
 Operator : SY/MD
 Sample : 02417-16ME
 Misc : 5.44g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW8Y2ME

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 04/26/2023
 Supervised By :Mahesh Dadoda 04/26/2023

Quant Time: Apr 25 05:32:04 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Apr 22 00:43:23 2023
 Response via : Initial Calibration

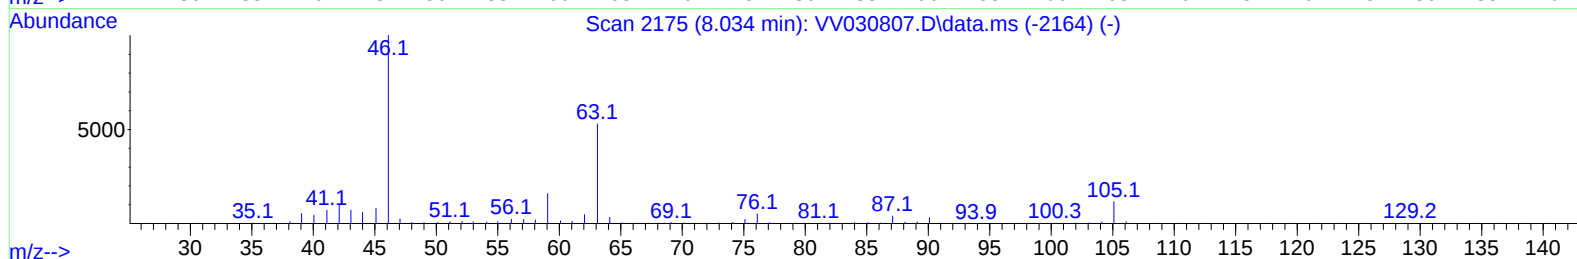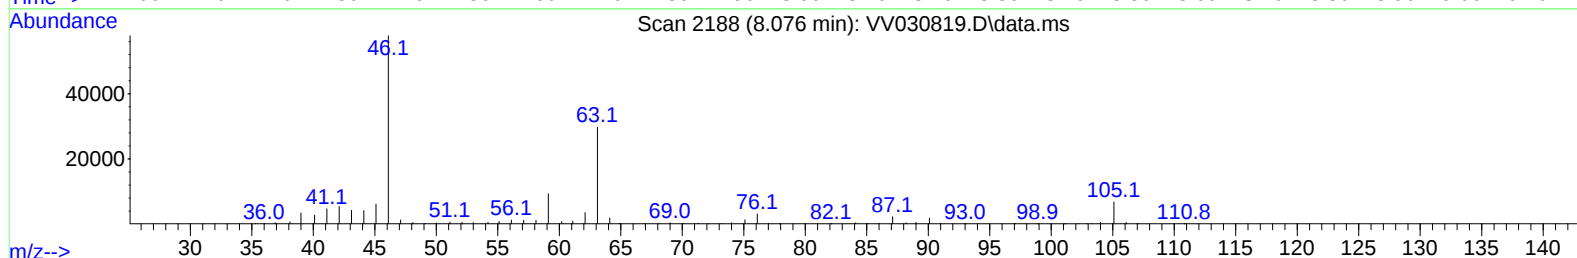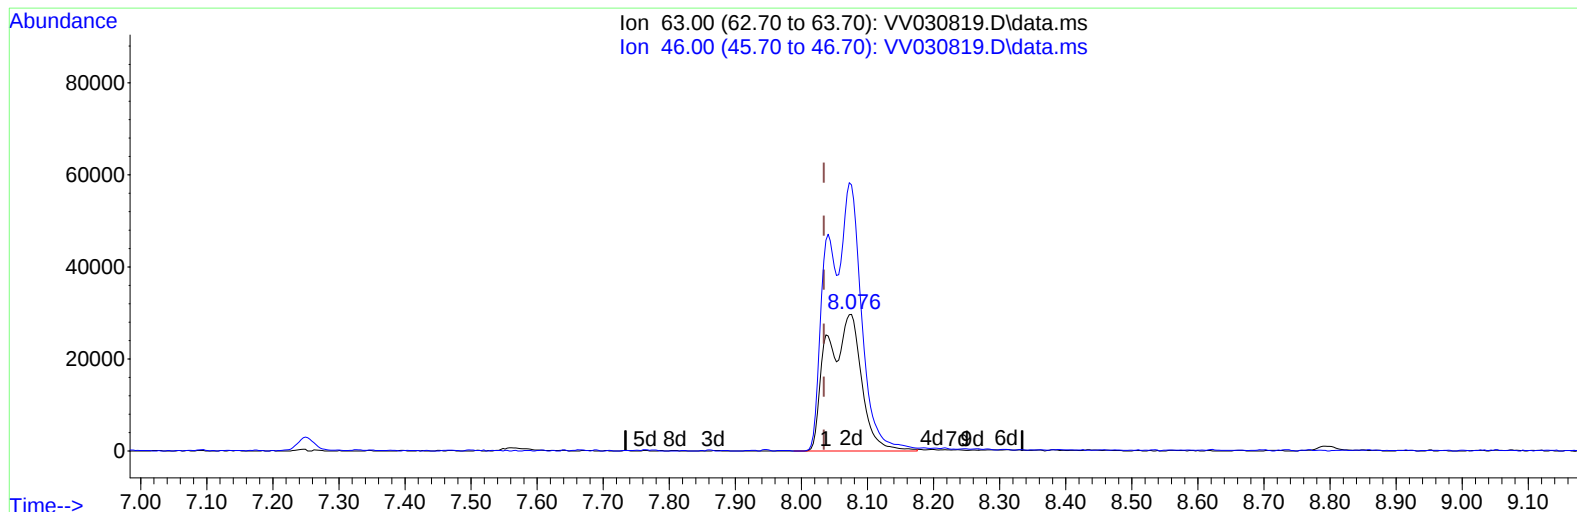

TIC: VV030819.D\data.ms

(47) 2-Hexanone-d5 (S)

8.076min (+ 0.042) 145.97 ug/L m

response 106871

Ion	Exp%	Act%
63.00	100.00	100.00
46.00	190.80	69.94#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042423\
 Data File : VW030819.D
 Acq On : 25 Apr 2023 02:19
 Operator : SY/MD
 Sample : 02417-16ME
 Misc : 5.44g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW8Y2ME

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 04/26/2023
 Supervised By :Mahesh Dadoda 04/26/2023

Quant Time: Apr 25 05:32:04 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Apr 22 00:43:23 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.542	114	259313	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.793	117	253064	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.198	152	138604	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.282	65	116443	61.255	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery = 122.500%			
7) Chloroethane-d5	1.529	69	126628m	79.490	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery = 158.980%#			
11) 1,1-Dichloroethene-d2	2.047	65	59429	65.922	ug/L	-0.02
Spiked Amount 50.000	Range 60 - 125		Recovery = 131.840%#			
21) 2-Butanone-d5	3.815	46	152042	145.617	ug/L	0.01
Spiked Amount 100.000	Range 40 - 130		Recovery = 145.620%#			
24) Chloroform-d	4.259	84	253118	73.474	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 146.940%#			
26) 1,2-Dichloroethane-d4	4.947	65	184225	83.177	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 166.360%#			
32) Benzene-d6	4.963	84	487170	81.424	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 162.840%#			
36) 1,2-Dichloropropane-d6	5.995	67	147465	79.345	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery = 158.700%#			
41) Toluene-d8	7.249	98	454318	80.874	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 161.740%#			
43) trans-1,3-Dichloroprop...	7.561	79	76714	81.896	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 163.800%#			
47) 2-Hexanone-d5	8.076	63	106871m	145.970	ug/L	0.04
Spiked Amount 100.000	Range 45 - 130		Recovery = 145.970%#			
56) 1,1,2,2-Tetrachloroeth...	10.172	84	200872	74.485	ug/L	0.01
Spiked Amount 50.000	Range 65 - 120		Recovery = 148.980%#			
66) 1,2-Dichlorobenzene-d4	11.574	152	197897	89.828	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 179.660%#			
Target Compounds						
3) Chloromethane	1.217	50	43193	14.769	ug/L	99
6) Bromomethane	1.491	94	14304	15.299	ug/L	95
16) Methylene chloride	2.452	84	5448	2.622	ug/L	99
46) Tetrachloroethene	7.915	164	1143	0.653	ug/L	85

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
Data File : VV030819.D
Acq On : 25 Apr 2023 02:19
Operator : SY/MD
Sample : 02417-16ME
Misc : 5.44g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW8Y2ME

Manual IntegrationsAPPROVED

Quant Time: Apr 25 05:32:04 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Apr 22 00:43:23 2023
Response via : Initial Calibration

Reviewed By :Krupa Patel 04/26/2023
Supervised By :Mahesh Dadoda 04/26/2023

