

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
 Data File : VV030783.D
 Acq On : 24 Apr 2023 11:22
 Operator : SY/MD
 Sample : VV0424WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK331

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030783.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	93	rVB	93158	105305	13.67%	1.689%
2	1.535	148	154	166	rVB	91263	108252	14.05%	1.736%
3	2.063	309	318	334	rBV	186683	268902	34.89%	4.313%
4	2.359	409	410	412	rBV3	760	321	0.04%	0.005%
5	2.388	416	419	421	rBV4	1702	1042	0.14%	0.017%
6	2.500	453	454	455	rBV	855	265	0.03%	0.004%
7	2.674	506	508	509	rVB2	1209	338	0.04%	0.005%
8	2.735	524	527	528	rBV3	902	421	0.05%	0.007%
9	2.793	543	545	546	rBV2	776	288	0.04%	0.005%
10	2.957	593	596	597	rBV3	1132	710	0.09%	0.011%
11	3.105	639	642	644	rBV4	1214	763	0.10%	0.012%
12	3.159	657	659	661	rBV3	900	448	0.06%	0.007%
13	3.307	703	705	708	rBV4	1527	687	0.09%	0.011%
14	3.587	791	792	796	rVB3	1012	497	0.06%	0.008%
15	3.616	800	801	803	rVB2	1729	519	0.07%	0.008%
16	3.722	832	834	836	rVB3	635	200	0.03%	0.003%
17	3.757	842	845	847	rBV3	1804	1072	0.14%	0.017%
18	3.799	849	858	888	rVV	54101	154817	20.09%	2.483%
19	4.259	987	1001	1021	rBV	127633	318575	41.34%	5.110%
20	4.667	1126	1128	1130	rBV3	1531	791	0.10%	0.013%
21	4.760	1154	1157	1159	rBV4	1453	1114	0.14%	0.018%
22	4.841	1180	1182	1184	rBV3	1415	623	0.08%	0.010%
23	4.895	1196	1199	1201	rBV4	2045	1419	0.18%	0.023%
24	4.963	1205	1220	1246	rVV2	285728	770606	100.00%	12.361%
25	5.400	1350	1356	1359	rBV6	2191	2578	0.33%	0.041%
26	5.490	1382	1384	1386	rBV3	1454	634	0.08%	0.010%
27	5.542	1388	1400	1425	rVV	270690	567736	73.67%	9.107%
28	5.838	1482	1492	1494	rBV8	4327	6525	0.85%	0.105%
29	5.995	1529	1541	1565	rBV	171915	357365	46.37%	5.732%
30	6.590	1724	1726	1731	rBV6	1403	922	0.12%	0.015%
31	6.680	1752	1754	1756	rBV2	1276	550	0.07%	0.009%
32	6.741	1771	1773	1777	rVB4	890	667	0.09%	0.011%
33	6.825	1797	1799	1803	rBV4	810	530	0.07%	0.009%
34	6.847	1803	1806	1809	rVV5	1305	1061	0.14%	0.017%
35	6.918	1817	1828	1846	rBV2	89094	172945	22.44%	2.774%
36	7.185	1908	1911	1912	rBV3	1066	652	0.08%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
 Data File : VV030783.D
 Acq On : 24 Apr 2023 11:22
 Operator : SY/MD
 Sample : VV0424WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK331

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	7.249	1919	1931	1950	rBV	320364	576112	74.76%	9.241%
38	7.561	2019	2028	2043	rBV2	64546	114301	14.83%	1.833%
39	8.034	2164	2175	2208	rBV	168272	350332	45.46%	5.619%
40	8.670	2370	2373	2375	rBV4	1352	865	0.11%	0.014%
41	8.792	2399	2411	2430	rBV	409654	701408	91.02%	11.251%
42	9.053	2490	2492	2497	rBV6	1128	798	0.10%	0.013%
43	9.079	2497	2500	2501	rBV3	1294	740	0.10%	0.012%
44	9.159	2524	2525	2526	rBV	836	298	0.04%	0.005%
45	9.191	2533	2535	2540	rVB6	1966	1039	0.13%	0.017%
46	9.271	2557	2560	2562	rBV4	1330	779	0.10%	0.012%
47	9.336	2577	2580	2582	rBV3	1183	659	0.09%	0.011%
48	9.358	2584	2587	2588	rBV3	1339	687	0.09%	0.011%
49	9.699	2690	2693	2696	rBV4	1435	1042	0.14%	0.017%
50	9.715	2696	2698	2700	rBV2	1385	853	0.11%	0.014%
51	9.963	2771	2775	2779	rVB6	1928	1540	0.20%	0.025%
52	10.159	2825	2836	2860	rVB	245572	396676	51.48%	6.363%
53	10.448	2924	2926	2928	rBV3	993	509	0.07%	0.008%
54	10.583	2967	2968	2969	rVB	959	185	0.02%	0.003%
55	10.603	2970	2974	2978	rBV6	1357	1183	0.15%	0.019%
56	10.641	2983	2986	2987	rBV3	1369	659	0.09%	0.011%
57	10.776	3026	3028	3030	rBV3	1083	436	0.06%	0.007%
58	10.914	3067	3071	3073	rBV4	1367	947	0.12%	0.015%
59	10.947	3079	3081	3084	rBV3	1218	682	0.09%	0.011%
60	10.985	3091	3093	3098	rVB6	1662	1159	0.15%	0.019%
61	11.008	3098	3100	3104	rVB5	1018	603	0.08%	0.010%
62	11.030	3104	3107	3110	rVB3	1473	884	0.11%	0.014%
63	11.050	3110	3113	3116	rBV6	697	598	0.08%	0.010%
64	11.066	3116	3118	3122	rBV4	1727	1295	0.17%	0.021%
65	11.136	3137	3140	3145	rVB7	2140	1581	0.21%	0.025%
66	11.194	3147	3158	3178	rBV	404037	653501	84.80%	10.482%
67	11.326	3195	3199	3206	rBV8	1452	1699	0.22%	0.027%
68	11.378	3213	3215	3216	rBV	1117	457	0.06%	0.007%
69	11.525	3257	3261	3262	rBV4	1911	1422	0.18%	0.023%
70	11.567	3264	3274	3294	rVB	334327	550520	71.44%	8.830%
71	11.795	3341	3345	3348	rBV4	1913	1693	0.22%	0.027%
72	11.995	3406	3407	3409	rBV2	1149	352	0.05%	0.006%
73	12.111	3441	3443	3444	rBV2	731	306	0.04%	0.005%
74	12.197	3466	3470	3471	rBV4	880	657	0.09%	0.011%
75	12.246	3483	3485	3490	rVB5	1563	928	0.12%	0.015%
76	12.297	3498	3501	3502	rBV3	1318	751	0.10%	0.012%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
 Data File : VV030783.D
 Acq On : 24 Apr 2023 11:22
 Operator : SY/MD
 Sample : VV0424WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK331

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	12.403	3532	3534	3535	rBV2	1373	423	0.05%	0.007%
78	12.442	3545	3546	3548	rBV2	824	281	0.04%	0.005%
79	12.458	3548	3551	3553	rVB3	1159	674	0.09%	0.011%
80	12.474	3553	3556	3560	rBV5	1491	1225	0.16%	0.020%
81	12.532	3572	3574	3575	rBV2	850	244	0.03%	0.004%
82	12.702	3622	3627	3630	rBV6	1752	1966	0.26%	0.032%
83	12.866	3673	3678	3679	rBV4	1565	1042	0.14%	0.017%
84	12.918	3691	3694	3697	rBV4	1040	606	0.08%	0.010%
85	13.133	3757	3761	3763	rBV4	1034	845	0.11%	0.014%
86	13.255	3795	3799	3803	rBV6	1451	1453	0.19%	0.023%
87	13.323	3816	3820	3825	rBV6	1700	1728	0.22%	0.028%
88	13.345	3825	3827	3828	rVB2	1167	328	0.04%	0.005%
89	13.509	3877	3878	3881	rBV3	866	487	0.06%	0.008%
90	13.721	3942	3944	3945	rBV2	1352	439	0.06%	0.007%
91	15.104	4372	4374	4378	rBV5	1858	1377	0.18%	0.022%




Sum of corrected areas: 6234394

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
Data File : VV030783.D
Acq On : 24 Apr 2023 11:22
Operator : SY/MD
Sample : VV0424WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK331

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

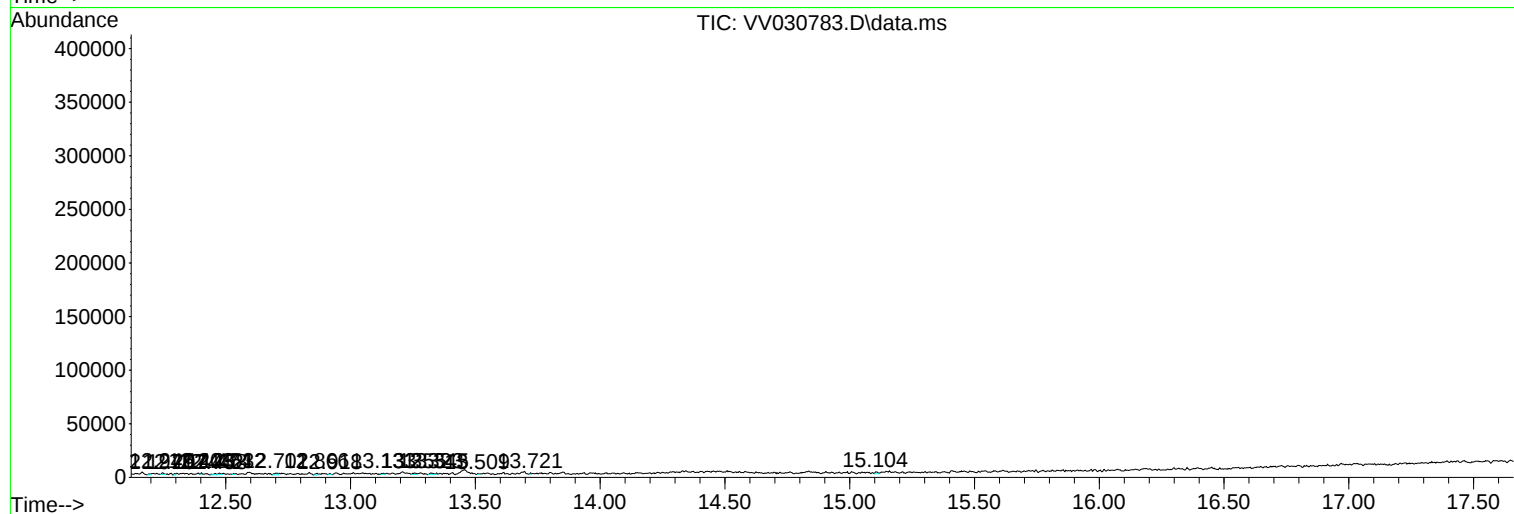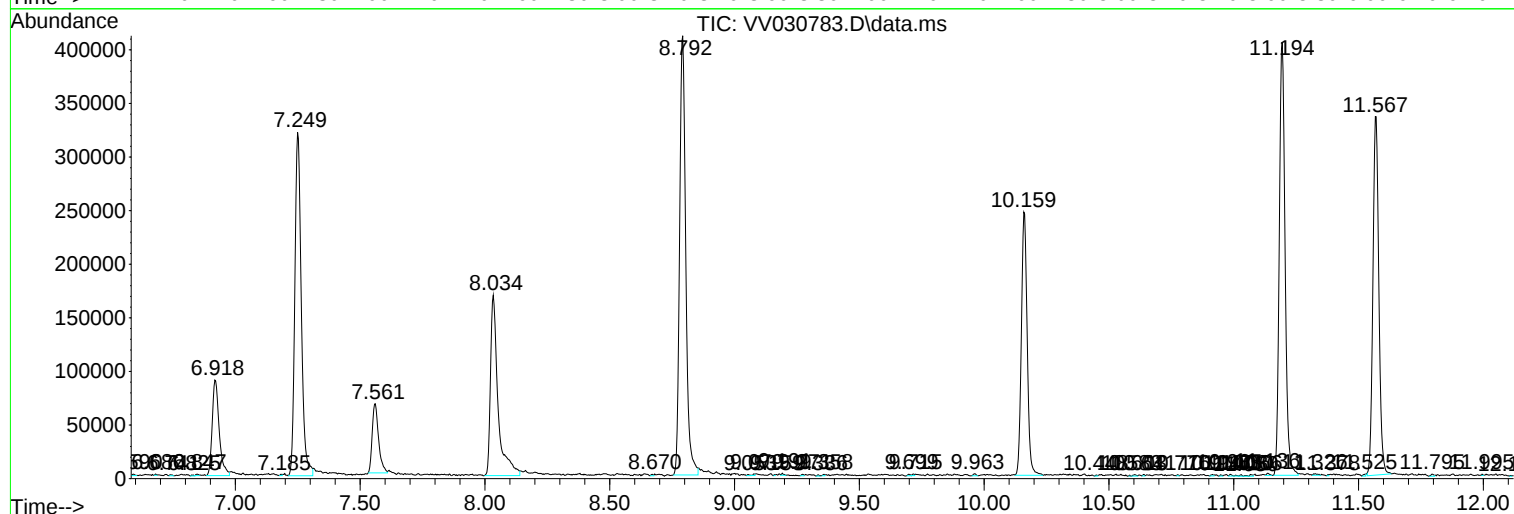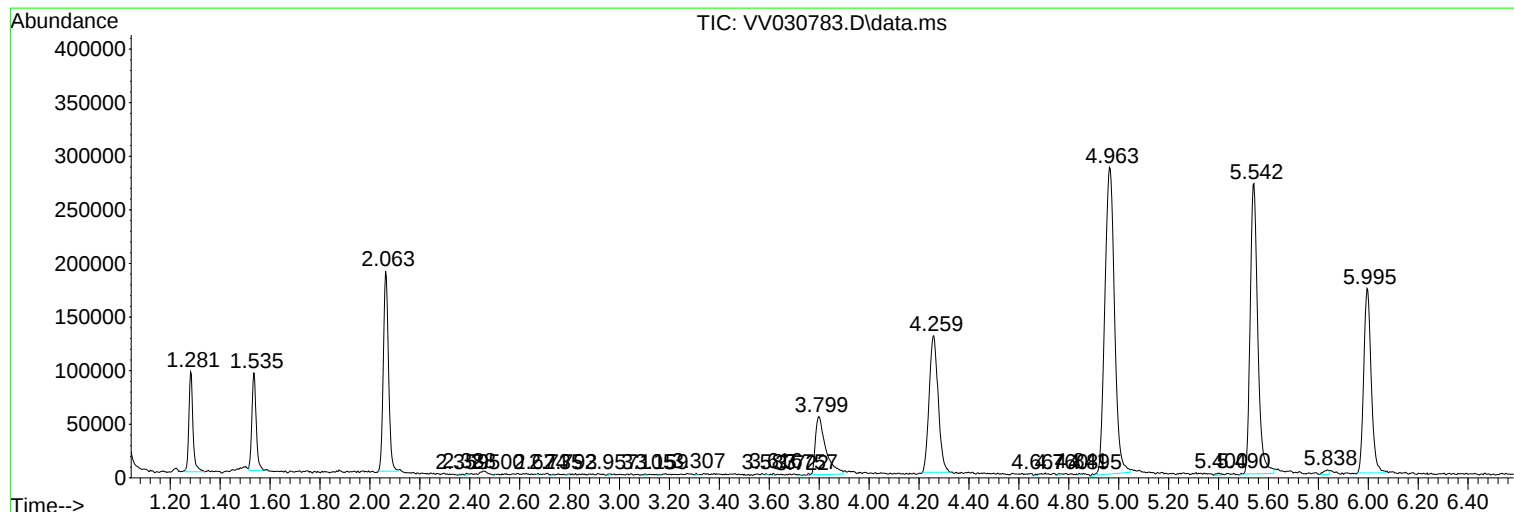

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
Data File : VV030783.D
Acq On : 24 Apr 2023 11:22
Operator : SY/MD
Sample : VV0424WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK331

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
Data File : VV030783.D
Acq On : 24 Apr 2023 11:22
Operator : SY/MD
Sample : VV0424WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK331

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------