

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
 Data File : VV030785.D
 Acq On : 24 Apr 2023 12:12
 Operator : SY/MD
 Sample : 02398-03DL 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMN2DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030785.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	88	rBV	89998	100000	3.04%	0.893%
2	1.539	148	155	169	rVB	92033	107239	3.26%	0.957%
3	2.066	310	319	334	rVB	185664	268734	8.18%	2.399%
4	2.416	426	428	431	rBV4	1089	694	0.02%	0.006%
5	2.503	453	455	457	rBV3	1148	424	0.01%	0.004%
6	2.613	487	489	491	rVB2	815	307	0.01%	0.003%
7	2.686	507	512	514	rBV5	1499	1254	0.04%	0.011%
8	2.780	539	541	543	rVB3	908	356	0.01%	0.003%
9	2.802	546	548	549	rVB2	1216	402	0.01%	0.004%
10	2.973	597	601	602	rBV4	1395	1122	0.03%	0.010%
11	3.005	609	611	614	rBV3	1520	596	0.02%	0.005%
12	3.050	623	625	626	rBV	528	168	0.01%	0.001%
13	3.085	632	636	637	rBV4	917	735	0.02%	0.007%
14	3.127	647	649	652	rBV3	1087	755	0.02%	0.007%
15	3.233	679	682	683	rBV3	890	493	0.02%	0.004%
16	3.262	687	691	694	rBV4	1360	1390	0.04%	0.012%
17	3.310	703	706	707	rBV4	957	522	0.02%	0.005%
18	3.323	708	710	711	rVV	1339	418	0.01%	0.004%
19	3.346	715	717	719	rBV2	781	356	0.01%	0.003%
20	3.368	722	724	726	rBV3	1219	518	0.02%	0.005%
21	3.410	735	737	739	rBV3	571	327	0.01%	0.003%
22	3.458	748	752	754	rBV4	1440	1218	0.04%	0.011%
23	3.584	788	791	795	rVB5	1767	1437	0.04%	0.013%
24	3.603	795	797	799	rBV3	1090	637	0.02%	0.006%
25	3.625	802	804	806	rBV3	594	323	0.01%	0.003%
26	3.658	812	814	815	rBV2	992	296	0.01%	0.003%
27	3.809	851	861	886	rBV	47636	149713	4.56%	1.336%
28	4.259	989	1001	1028	rVB2	125750	325957	9.92%	2.909%
29	4.510	1076	1079	1081	rBV4	1641	1164	0.04%	0.010%
30	4.651	1120	1123	1124	rBV3	848	548	0.02%	0.005%
31	4.966	1205	1221	1230	rBV2	293314	761697	23.19%	6.799%
32	5.542	1382	1400	1422	rBV	288961	607481	18.49%	5.422%
33	5.950	1522	1527	1529	rBV6	2023	1986	0.06%	0.018%
34	5.998	1529	1542	1565	rVV	172343	366821	11.17%	3.274%
35	6.374	1656	1659	1662	rBV4	1247	1204	0.04%	0.011%
36	6.751	1774	1776	1779	rVB4	1763	764	0.02%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042423\
 Data File : VW030785.D
 Acq On : 24 Apr 2023 12:12
 Operator : SY/MD
 Sample : 02398-03DL 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMN2DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	6.796	1786	1790	1792	rBV5	2295	1547	0.05%	0.014%
38	6.921	1817	1829	1846	rBV	90426	173009	5.27%	1.544%
39	7.165	1902	1905	1908	rBV4	1298	996	0.03%	0.009%
40	7.252	1920	1932	1956	rBV	323872	584661	17.80%	5.218%
41	7.419	1982	1984	1988	rVB5	2862	1691	0.05%	0.015%
42	7.561	2019	2028	2041	rBV	64527	112765	3.43%	1.007%
43	7.706	2070	2073	2075	rBV5	2235	1232	0.04%	0.011%
44	7.796	2099	2101	2103	rBV4	995	531	0.02%	0.005%
45	7.953	2148	2150	2154	rVB4	1026	412	0.01%	0.004%
46	8.034	2164	2175	2210	rBV	172786	373257	11.36%	3.332%
47	8.622	2356	2358	2360	rBV3	1001	485	0.01%	0.004%
48	8.673	2369	2374	2377	rBV6	1769	1543	0.05%	0.014%
49	8.686	2377	2378	2381	rBV3	883	391	0.01%	0.003%
50	8.796	2400	2412	2413	rBV	484984	597148	18.18%	5.330%
51	9.371	2589	2591	2594	rBV4	1042	679	0.02%	0.006%
52	9.706	2692	2695	2696	rBV2	997	575	0.02%	0.005%
53	9.799	2722	2724	2728	rBV5	1693	1217	0.04%	0.011%
54	9.866	2743	2745	2747	rBV2	1124	480	0.01%	0.004%
55	9.972	2775	2778	2781	rBV3	1236	849	0.03%	0.008%
56	10.088	2809	2814	2818	rBV7	1899	1926	0.06%	0.017%
57	10.162	2825	2837	2862	rBV	245038	400928	12.21%	3.579%
58	10.249	2862	2864	2867	rBV4	1117	817	0.02%	0.007%
59	10.371	2900	2902	2903	rBV2	822	260	0.01%	0.002%
60	10.381	2903	2905	2909	rVB4	1117	770	0.02%	0.007%
61	10.419	2915	2917	2918	rBV3	515	243	0.01%	0.002%
62	10.484	2933	2937	2938	rBV4	1243	886	0.03%	0.008%
63	10.535	2951	2953	2955	rBV2	1222	663	0.02%	0.006%
64	10.644	2985	2987	2993	rVB6	945	791	0.02%	0.007%
65	10.683	2993	2999	3001	rBV8	1638	1580	0.05%	0.014%
66	10.795	3031	3034	3038	rBV5	1222	876	0.03%	0.008%
67	10.918	3069	3072	3074	rBV4	1077	746	0.02%	0.007%
68	11.127	3126	3137	3147	rBV	113824	182158	5.55%	1.626%
69	11.217	3148	3165	3186	rVB2	1157478	2434960	74.12%	21.734%
70	11.586	3264	3280	3300	rBV3	1827206	3284941	100.00%	29.320%
71	11.905	3376	3379	3381	rBV4	1470	913	0.03%	0.008%
72	12.049	3422	3424	3425	rBV2	1399	587	0.02%	0.005%
73	12.397	3528	3532	3534	rBV4	1752	1360	0.04%	0.012%
74	12.699	3621	3626	3631	rBV9	1979	2113	0.06%	0.019%
75	12.757	3642	3644	3645	rBV2	1167	489	0.01%	0.004%
76	13.017	3723	3725	3726	rBV	839	292	0.01%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
 Data File : VV030785.D
 Acq On : 24 Apr 2023 12:12
 Operator : SY/MD
 Sample : 02398-03DL 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMN2DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M

Title : VOC Analysis

77	13.053	3734	3736	3739	rBV4	1097	877	0.03%	0.008%
78	13.078	3743	3744	3747	rBV4	803	336	0.01%	0.003%
79	13.094	3747	3749	3751	rBV3	1015	432	0.01%	0.004%
80	13.207	3770	3784	3804	rBV	154627	245258	7.47%	2.189%
81	13.689	3925	3934	3946	rVB3	46428	73791	2.25%	0.659%
82	13.982	4023	4025	4027	rBV3	1410	563	0.02%	0.005%
83	14.483	4179	4181	4184	rBV4	1559	935	0.03%	0.008%
84	14.590	4209	4214	4215	rBV5	1955	1646	0.05%	0.015%




Sum of corrected areas: 11203661

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
Data File : VV030785.D
Acq On : 24 Apr 2023 12:12
Operator : SY/MD
Sample : 02398-03DL 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMN2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

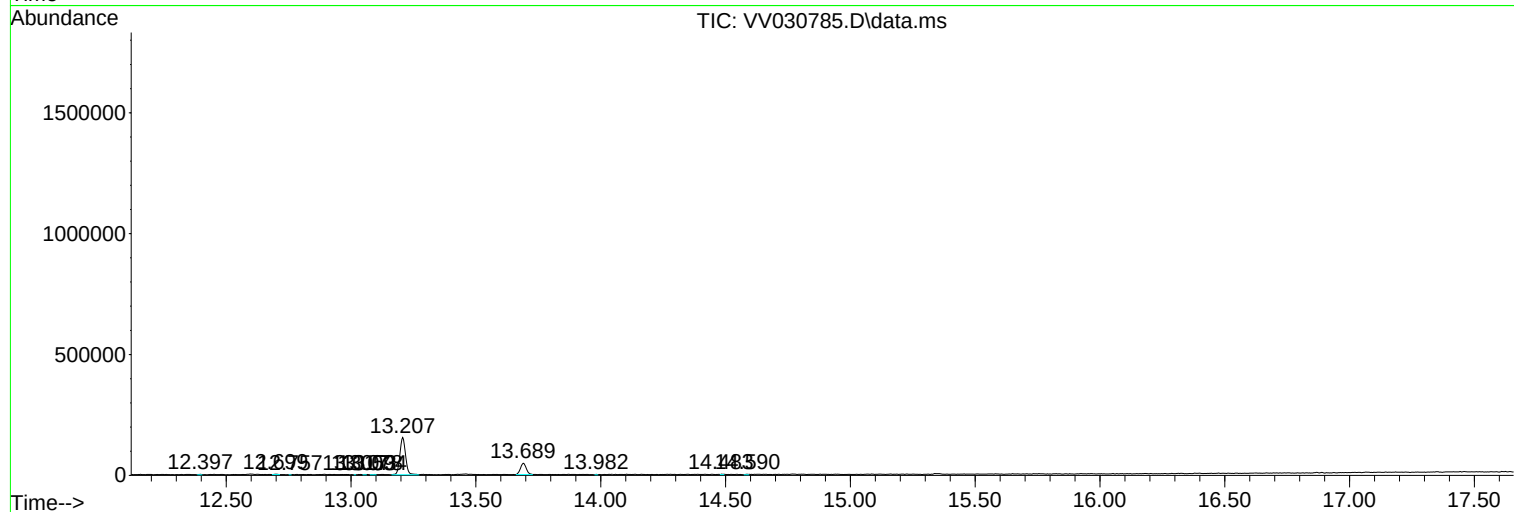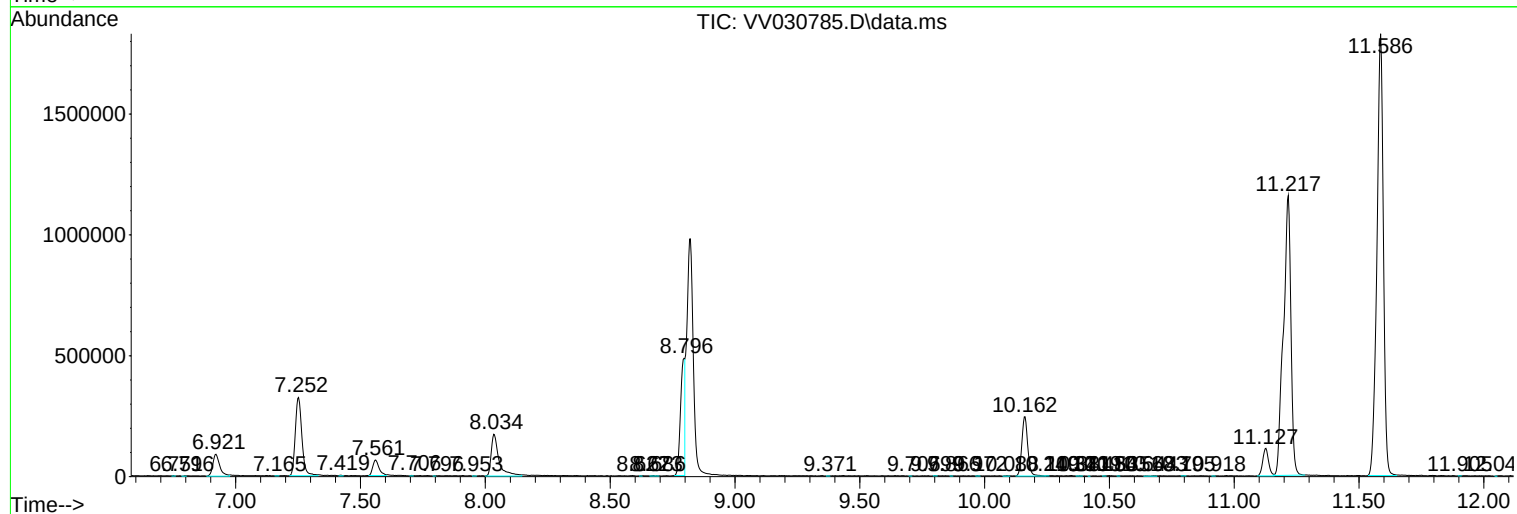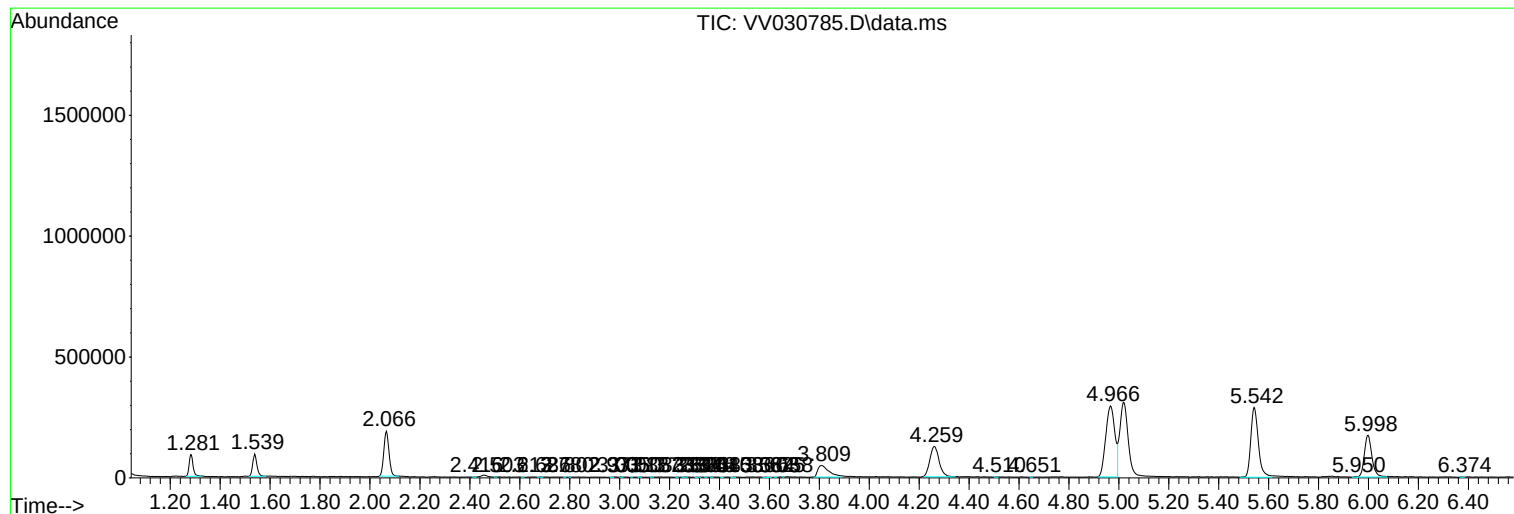

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
Data File : VV030785.D
Acq On : 24 Apr 2023 12:12
Operator : SY/MD
Sample : 02398-03DL 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMN2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
Data File : VV030785.D
Acq On : 24 Apr 2023 12:12
Operator : SY/MD
Sample : 02398-03DL 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMN2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------