

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
 Data File : VV030787.D
 Acq On : 24 Apr 2023 12:59
 Operator : SY/MD
 Sample : 02440-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMQ4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030787.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	70	75	88	rVB	91065	100499	13.03%	1.571%
2	1.539	149	155	165	rVB	87236	100772	13.06%	1.575%
3	2.066	310	319	335	rVB	186806	272949	35.39%	4.266%
4	2.551	468	470	472	rBV3	919	415	0.05%	0.006%
5	2.638	495	497	498	rBV	1178	561	0.07%	0.009%
6	2.674	504	508	512	rBV5	1372	1449	0.19%	0.023%
7	2.789	541	544	546	rBV2	1106	600	0.08%	0.009%
8	2.812	550	551	553	rBV2	1542	742	0.10%	0.012%
9	2.876	569	571	573	rVB3	1226	521	0.07%	0.008%
10	2.918	583	584	586	rVB3	966	360	0.05%	0.006%
11	2.986	603	605	606	rBV2	688	315	0.04%	0.005%
12	2.995	606	608	612	rVV4	830	621	0.08%	0.010%
13	3.124	647	648	651	rBV2	708	386	0.05%	0.006%
14	3.166	658	661	663	rBV4	1137	795	0.10%	0.012%
15	3.256	686	689	691	rVB4	1203	600	0.08%	0.009%
16	3.429	741	743	747	rVB5	1423	836	0.11%	0.013%
17	3.503	764	766	768	rBV3	903	358	0.05%	0.006%
18	3.551	779	781	783	rBV3	1632	886	0.11%	0.014%
19	3.693	823	825	827	rBV3	1057	370	0.05%	0.006%
20	3.725	832	835	836	rBV2	1054	674	0.09%	0.011%
21	3.809	851	861	886	rBV2	48130	147445	19.12%	2.304%
22	4.259	987	1001	1024	rBV	126597	327069	42.40%	5.112%
23	4.503	1076	1077	1082	rVB5	1380	807	0.10%	0.013%
24	4.606	1106	1109	1114	rBV7	1279	1285	0.17%	0.020%
25	4.735	1146	1149	1151	rBV4	1388	1039	0.13%	0.016%
26	4.821	1174	1176	1177	rBV2	807	347	0.04%	0.005%
27	4.857	1183	1187	1188	rBV3	1869	1037	0.13%	0.016%
28	4.883	1194	1195	1196	rBV3	989	320	0.04%	0.005%
29	4.902	1200	1201	1204	rBV3	1286	807	0.10%	0.013%
30	4.966	1205	1221	1246	rVV2	289650	771341	100.00%	12.056%
31	5.342	1336	1338	1341	rVB5	1628	573	0.07%	0.009%
32	5.542	1387	1400	1426	rBV	293989	619548	80.32%	9.683%
33	5.998	1531	1542	1565	rVB	172210	349122	45.26%	5.457%
34	6.452	1679	1683	1685	rBV5	1030	779	0.10%	0.012%
35	6.635	1737	1740	1741	rBV3	1568	844	0.11%	0.013%
36	6.741	1770	1773	1775	rBV4	1691	1137	0.15%	0.018%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042423\
 Data File : VW030787.D
 Acq On : 24 Apr 2023 12:59
 Operator : SY/MD
 Sample : 02440-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMQ4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	6.882	1814	1817	1818	rBV3	1753	874	0.11%	0.014%
38	6.921	1820	1829	1853	rVB	88061	170696	22.13%	2.668%
39	7.252	1920	1932	1950	rBV	325088	580460	75.25%	9.072%
40	7.561	2019	2028	2049	rBV2	63205	115712	15.00%	1.809%
41	7.992	2160	2162	2166	rBV5	1010	917	0.12%	0.014%
42	8.037	2166	2176	2194	rBV	159992	325653	42.22%	5.090%
43	8.680	2374	2376	2381	rBV5	1281	691	0.09%	0.011%
44	8.725	2387	2390	2391	rBV2	1033	547	0.07%	0.009%
45	8.792	2400	2411	2435	rBV	448886	759627	98.48%	11.873%
46	9.043	2487	2489	2490	rBV2	988	367	0.05%	0.006%
47	9.143	2517	2520	2523	rBV5	1418	1063	0.14%	0.017%
48	9.165	2523	2527	2528	rBV4	1674	1220	0.16%	0.019%
49	9.255	2554	2555	2557	rBV2	1104	555	0.07%	0.009%
50	9.435	2608	2611	2613	rBV4	1162	732	0.09%	0.011%
51	9.484	2624	2626	2627	rBV2	898	360	0.05%	0.006%
52	9.808	2725	2727	2730	rBV4	683	324	0.04%	0.005%
53	9.847	2737	2739	2741	rBV3	917	367	0.05%	0.006%
54	9.902	2754	2756	2759	rVB4	1108	577	0.07%	0.009%
55	9.918	2759	2761	2762	rBV3	982	444	0.06%	0.007%
56	10.033	2795	2797	2798	rBV2	1072	561	0.07%	0.009%
57	10.114	2821	2822	2825	rBV3	1119	430	0.06%	0.007%
58	10.159	2825	2836	2859	rBV	247371	395718	51.30%	6.185%
59	10.403	2909	2912	2914	rVB4	1376	843	0.11%	0.013%
60	10.416	2914	2916	2920	rVB5	1002	592	0.08%	0.009%
61	10.435	2920	2922	2926	rBV4	772	527	0.07%	0.008%
62	10.458	2926	2929	2932	rBV3	840	675	0.09%	0.011%
63	10.493	2939	2940	2941	rBV	1089	405	0.05%	0.006%
64	10.551	2954	2958	2961	rVB4	1367	1154	0.15%	0.018%
65	10.599	2966	2973	2976	rBV7	1185	1582	0.21%	0.025%
66	10.895	3064	3065	3067	rVB2	988	305	0.04%	0.005%
67	11.021	3102	3104	3106	rBV3	860	429	0.06%	0.007%
68	11.117	3132	3134	3135	rBV2	1729	902	0.12%	0.014%
69	11.194	3147	3158	3175	rBV	437274	710368	92.10%	11.103%
70	11.471	3242	3244	3249	rBV6	1600	1064	0.14%	0.017%
71	11.570	3263	3275	3294	rBV	347426	583451	75.64%	9.119%
72	11.837	3356	3358	3359	rBV2	999	459	0.06%	0.007%
73	11.943	3386	3391	3392	rBV5	1567	1267	0.16%	0.020%
74	11.969	3397	3399	3402	rBV5	1548	895	0.12%	0.014%
75	12.008	3409	3411	3413	rBV2	1354	746	0.10%	0.012%
76	12.078	3430	3433	3434	rBV3	1602	940	0.12%	0.015%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
 Data File : VV030787.D
 Acq On : 24 Apr 2023 12:59
 Operator : SY/MD
 Sample : 02440-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMQ4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	12.303	3501	3503	3505	rVB2	1279	425	0.06%	0.007%
78	12.387	3524	3529	3532	rBV6	1894	1499	0.19%	0.023%
79	12.419	3537	3539	3542	rBV4	1325	849	0.11%	0.013%
80	12.455	3547	3550	3552	rBV3	1255	746	0.10%	0.012%
81	12.538	3575	3576	3578	rBV3	924	344	0.04%	0.005%
82	12.577	3586	3588	3591	rBV4	1347	768	0.10%	0.012%
83	12.670	3612	3617	3618	rBV5	1060	908	0.12%	0.014%
84	12.715	3628	3631	3633	rBV4	1359	907	0.12%	0.014%
85	12.831	3665	3667	3672	rVB4	1243	563	0.07%	0.009%
86	12.914	3689	3693	3695	rBV4	1137	911	0.12%	0.014%
87	13.091	3746	3748	3749	rBV2	1000	451	0.06%	0.007%
88	13.120	3753	3757	3758	rBV3	1219	725	0.09%	0.011%
89	13.130	3758	3760	3761	rBV2	1174	505	0.07%	0.008%
90	13.162	3768	3770	3776	rBV6	1439	1677	0.22%	0.026%
91	13.506	3876	3877	3880	rVB4	1088	432	0.06%	0.007%
92	13.641	3917	3919	3924	rVB5	1282	852	0.11%	0.013%
93	13.692	3928	3935	3943	rVV10	5247	7731	1.00%	0.121%
94	13.721	3943	3944	3946	rVB2	1207	431	0.06%	0.007%
95	14.014	4032	4035	4037	rBV4	1838	1257	0.16%	0.020%
96	14.136	4071	4073	4075	rBV3	1103	450	0.06%	0.007%
97	14.249	4106	4108	4109	rBV2	732	377	0.05%	0.006%
98	14.323	4128	4131	4133	rBV3	1271	908	0.12%	0.014%
99	14.528	4191	4195	4197	rBV4	1244	1111	0.14%	0.017%
100	14.593	4213	4215	4217	rVB3	1634	639	0.08%	0.010%




Sum of corrected areas: 6398174

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
Data File : VV030787.D
Acq On : 24 Apr 2023 12:59
Operator : SY/MD
Sample : 02440-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMQ4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

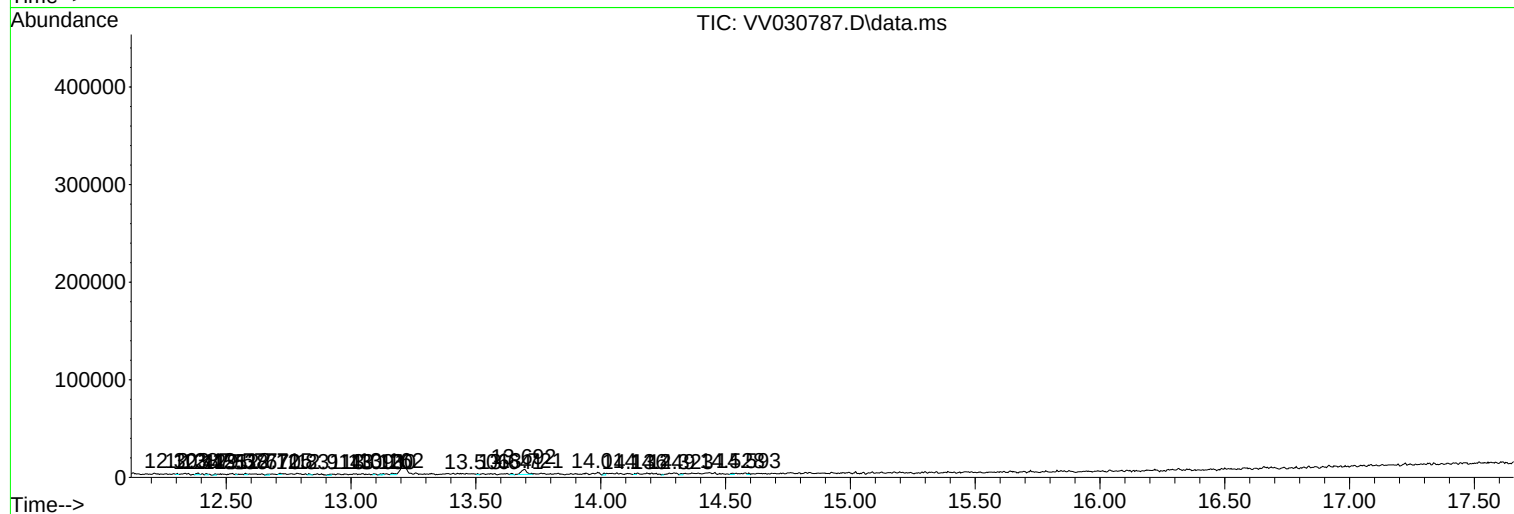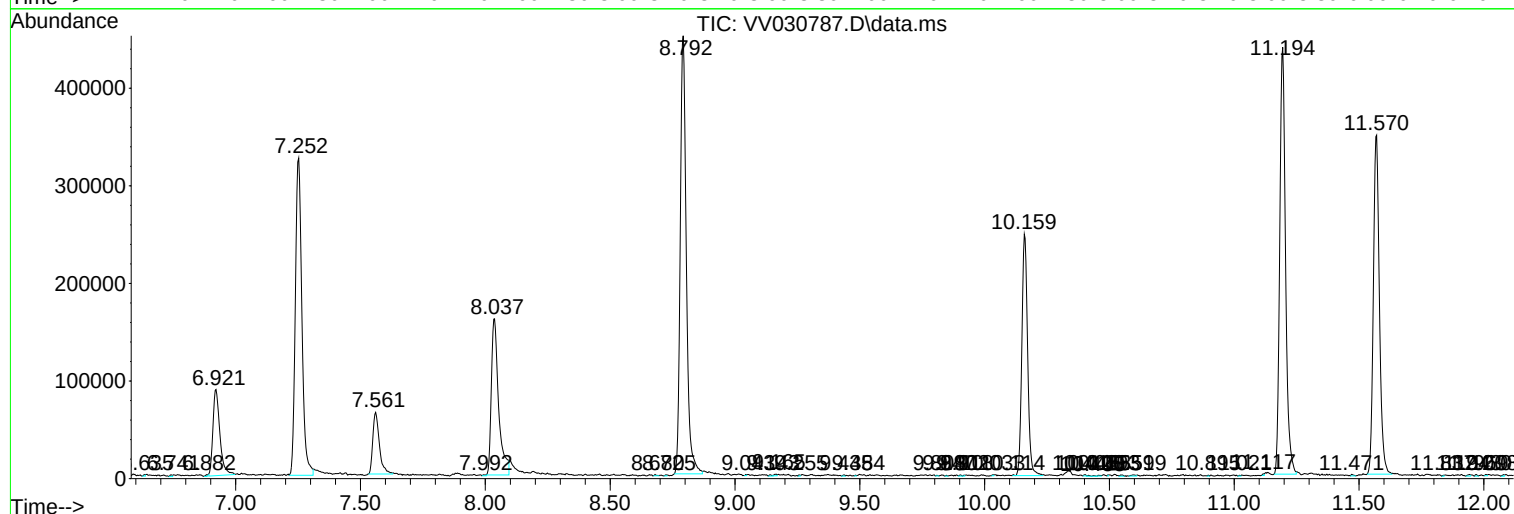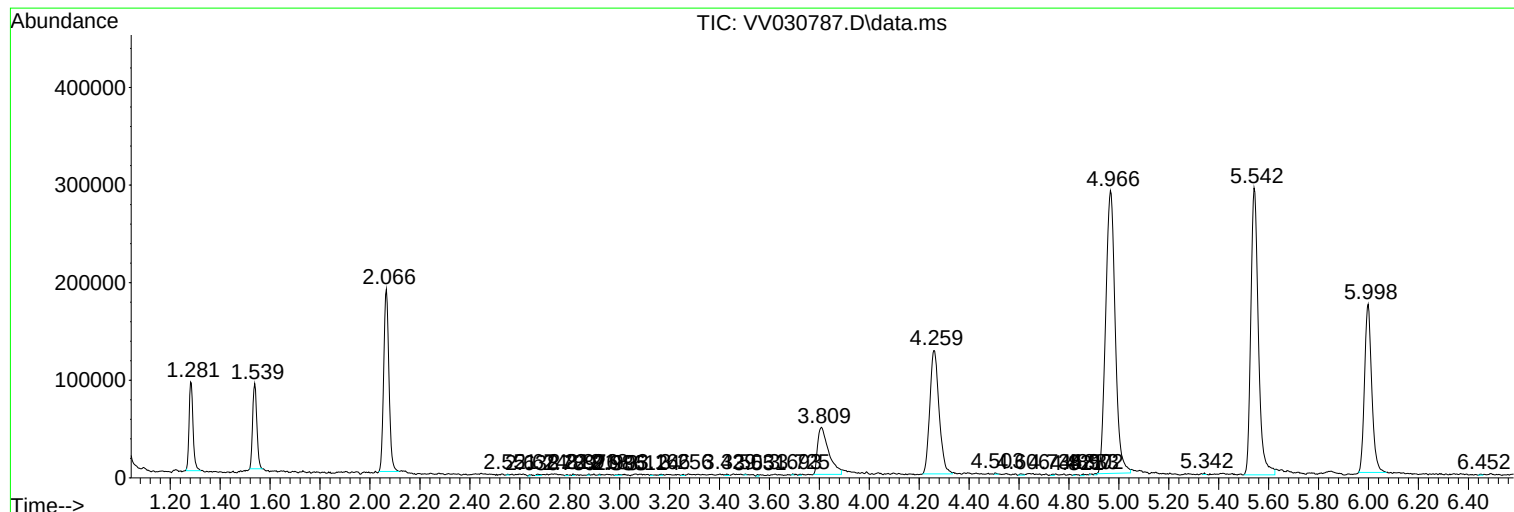

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
Data File : VV030787.D
Acq On : 24 Apr 2023 12:59
Operator : SY/MD
Sample : 02440-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0MQ4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
Data File : VV030787.D
Acq On : 24 Apr 2023 12:59
Operator : SY/MD
Sample : 02440-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0MQ4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
