

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
 Data File : VV030788.D
 Acq On : 24 Apr 2023 13:23
 Operator : SY/MD
 Sample : 02440-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMQ5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030788.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.285	69	76	85	rBV	95171	100556	12.54%	1.534%
2	1.539	148	155	167	rBV	96495	114542	14.28%	1.748%
3	2.066	310	319	332	rBV	191405	277520	34.61%	4.235%
4	2.237	370	372	378	rVB6	1583	1448	0.18%	0.022%
5	2.275	382	384	385	rBV2	1190	511	0.06%	0.008%
6	2.526	458	462	467	rBV8	1294	1254	0.16%	0.019%
7	2.552	467	470	472	rBV3	1267	616	0.08%	0.009%
8	2.658	500	503	507	rVV5	1435	819	0.10%	0.012%
9	2.828	551	556	557	rBV4	782	552	0.07%	0.008%
10	3.076	629	633	635	rVB5	1850	1231	0.15%	0.019%
11	3.092	635	638	642	rBV6	1867	1385	0.17%	0.021%
12	3.140	650	653	658	rBV7	1853	1658	0.21%	0.025%
13	3.275	692	695	696	rBV2	1149	543	0.07%	0.008%
14	3.355	718	720	723	rBV2	1416	792	0.10%	0.012%
15	3.407	732	736	739	rVB5	971	818	0.10%	0.012%
16	3.426	739	742	744	rBV3	1449	1220	0.15%	0.019%
17	3.471	754	756	759	rVB4	1174	516	0.06%	0.008%
18	3.561	781	784	786	rBV4	1102	712	0.09%	0.011%
19	3.606	791	798	802	rBV7	2317	2545	0.32%	0.039%
20	3.645	807	810	816	rBV6	1678	1962	0.24%	0.030%
21	3.687	822	823	826	rVB3	1134	560	0.07%	0.009%
22	3.761	844	846	848	rBV3	1161	721	0.09%	0.011%
23	3.806	850	860	887	rBV	51656	156296	19.49%	2.385%
24	4.259	985	1001	1026	rVV	133417	341696	42.61%	5.214%
25	4.523	1080	1083	1085	rBV4	2137	1343	0.17%	0.020%
26	4.732	1141	1148	1150	rBV6	1577	1472	0.18%	0.022%
27	4.806	1169	1171	1175	rVB5	1806	1148	0.14%	0.018%
28	4.825	1175	1177	1180	rBV4	1029	510	0.06%	0.008%
29	4.860	1184	1188	1192	rBV5	1813	1580	0.20%	0.024%
30	4.902	1196	1201	1202	rBV4	848	756	0.09%	0.012%
31	4.966	1204	1221	1253	rBV2	298032	801844	100.00%	12.235%
32	5.326	1324	1333	1337	rBV9	1702	2694	0.34%	0.041%
33	5.542	1384	1400	1419	rBV	288461	607287	75.74%	9.267%
34	5.841	1485	1493	1496	rBV9	3836	5882	0.73%	0.090%
35	5.998	1530	1542	1565	rBV	174679	364204	45.42%	5.557%
36	6.410	1667	1670	1675	rBV6	1358	1341	0.17%	0.020%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
 Data File : VV030788.D
 Acq On : 24 Apr 2023 13:23
 Operator : SY/MD
 Sample : 02440-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMQ5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	6.587	1721	1725	1727	rBV5	1281	1151	0.14%	0.018%
38	6.645	1740	1743	1745	rBV4	1218	511	0.06%	0.008%
39	6.841	1802	1804	1810	rVB6	1605	1134	0.14%	0.017%
40	6.876	1810	1815	1817	rBV5	1522	1254	0.16%	0.019%
41	6.921	1819	1829	1849	rVV	89277	173261	21.61%	2.644%
42	7.252	1919	1932	1952	rBV	334843	599088	74.71%	9.141%
43	7.503	2007	2010	2012	rBV4	1522	928	0.12%	0.014%
44	7.561	2019	2028	2042	rBV2	65638	118196	14.74%	1.804%
45	7.767	2088	2092	2094	rBV5	1285	1050	0.13%	0.016%
46	7.825	2109	2110	2112	rBV2	1105	527	0.07%	0.008%
47	7.850	2115	2118	2121	rVB4	1354	1067	0.13%	0.016%
48	7.937	2143	2145	2149	rVB4	840	512	0.06%	0.008%
49	8.034	2164	2175	2213	rBV	167272	369554	46.09%	5.639%
50	8.484	2311	2315	2317	rBV3	876	712	0.09%	0.011%
51	8.519	2323	2326	2328	rVB4	1381	709	0.09%	0.011%
52	8.693	2377	2380	2381	rBV3	1171	743	0.09%	0.011%
53	8.793	2399	2411	2436	rBV	449608	760521	94.85%	11.605%
54	9.098	2504	2506	2508	rBV2	1648	751	0.09%	0.011%
55	9.133	2515	2517	2522	rBV6	959	607	0.08%	0.009%
56	9.307	2567	2571	2573	rBV4	794	707	0.09%	0.011%
57	9.516	2632	2636	2637	rBV3	1159	688	0.09%	0.010%
58	9.561	2648	2650	2655	rVB6	1544	913	0.11%	0.014%
59	9.609	2660	2665	2668	rBV5	1946	1377	0.17%	0.021%
60	9.622	2668	2669	2671	rBV2	1124	599	0.07%	0.009%
61	9.760	2710	2712	2716	rVV5	1262	961	0.12%	0.015%
62	9.805	2722	2726	2727	rBV4	1162	917	0.11%	0.014%
63	9.998	2784	2786	2791	rVB5	1576	1124	0.14%	0.017%
64	10.024	2791	2794	2795	rBV3	1117	556	0.07%	0.008%
65	10.159	2823	2836	2857	rBV	250864	406616	50.71%	6.205%
66	10.333	2883	2890	2900	rVB9	4605	8063	1.01%	0.123%
67	10.378	2900	2904	2906	rBV4	2354	1539	0.19%	0.023%
68	10.596	2967	2972	2974	rBV7	1533	924	0.12%	0.014%
69	10.876	3056	3059	3061	rBV4	973	625	0.08%	0.010%
70	10.895	3063	3065	3070	rVB5	1440	690	0.09%	0.011%
71	10.944	3075	3080	3083	rBV6	1073	1225	0.15%	0.019%
72	11.059	3113	3116	3118	rBV3	1355	858	0.11%	0.013%
73	11.194	3146	3158	3177	rBV	422484	687476	85.74%	10.490%
74	11.445	3233	3236	3237	rBV2	2284	1190	0.15%	0.018%
75	11.484	3246	3248	3251	rBV4	1437	707	0.09%	0.011%
76	11.567	3264	3274	3295	rVB	352326	579851	72.31%	8.848%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
 Data File : VV030788.D
 Acq On : 24 Apr 2023 13:23
 Operator : SY/MD
 Sample : 02440-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMQ5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	11.809	3345	3349	3352	rBV5	1489	1279	0.16%	0.020%
78	11.828	3352	3355	3357	rBV4	1147	774	0.10%	0.012%
79	11.879	3367	3371	3376	rVB7	1230	1068	0.13%	0.016%
80	11.915	3380	3382	3385	rBV5	854	516	0.06%	0.008%
81	12.011	3408	3412	3415	rBV7	1518	1245	0.16%	0.019%
82	12.069	3428	3430	3433	rBV4	838	573	0.07%	0.009%
83	12.108	3438	3442	3444	rVB4	1345	891	0.11%	0.014%
84	12.291	3498	3499	3501	rBV2	964	506	0.06%	0.008%
85	12.355	3515	3519	3521	rBV5	1352	1030	0.13%	0.016%
86	12.834	3664	3668	3670	rBV5	1525	1058	0.13%	0.016%
87	12.902	3687	3689	3691	rBV3	1260	634	0.08%	0.010%
88	12.937	3696	3700	3702	rBV4	1407	904	0.11%	0.014%
89	12.982	3710	3714	3718	rVB6	1043	804	0.10%	0.012%
90	13.027	3725	3728	3729	rBV3	1482	942	0.12%	0.014%
91	13.294	3807	3811	3812	rBV3	1246	838	0.10%	0.013%
92	13.513	3875	3879	3882	rBV4	1130	857	0.11%	0.013%
93	13.638	3916	3918	3920	rBV3	1200	529	0.07%	0.008%
94	13.738	3945	3949	3951	rBV5	917	827	0.10%	0.013%
95	13.915	4002	4004	4009	rBV4	1337	1222	0.15%	0.019%
96	14.085	4054	4057	4059	rBV3	1208	659	0.08%	0.010%
97	14.098	4059	4061	4064	rVB4	1584	964	0.12%	0.015%
98	14.124	4064	4069	4074	rVB8	2111	2995	0.37%	0.046%
99	14.699	4246	4248	4253	rVB5	1638	1032	0.13%	0.016%
100	14.953	4325	4327	4328	rBV2	2044	974	0.12%	0.015%




Sum of corrected areas: 6553537

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
Data File : VV030788.D
Acq On : 24 Apr 2023 13:23
Operator : SY/MD
Sample : 02440-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMQ5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

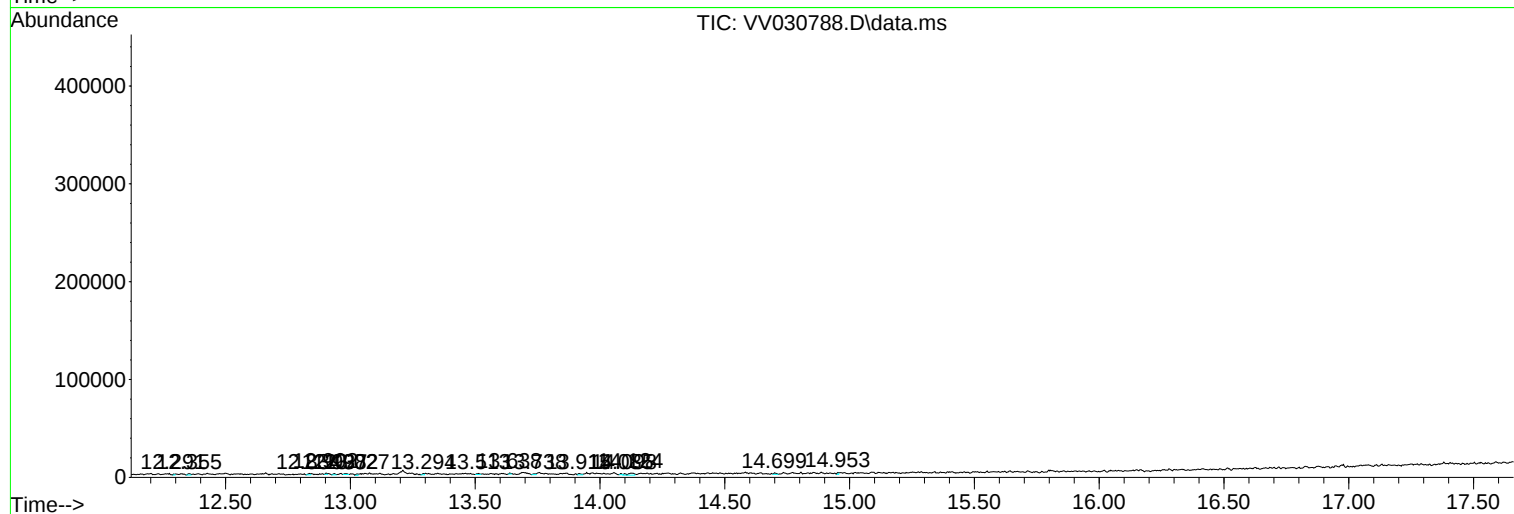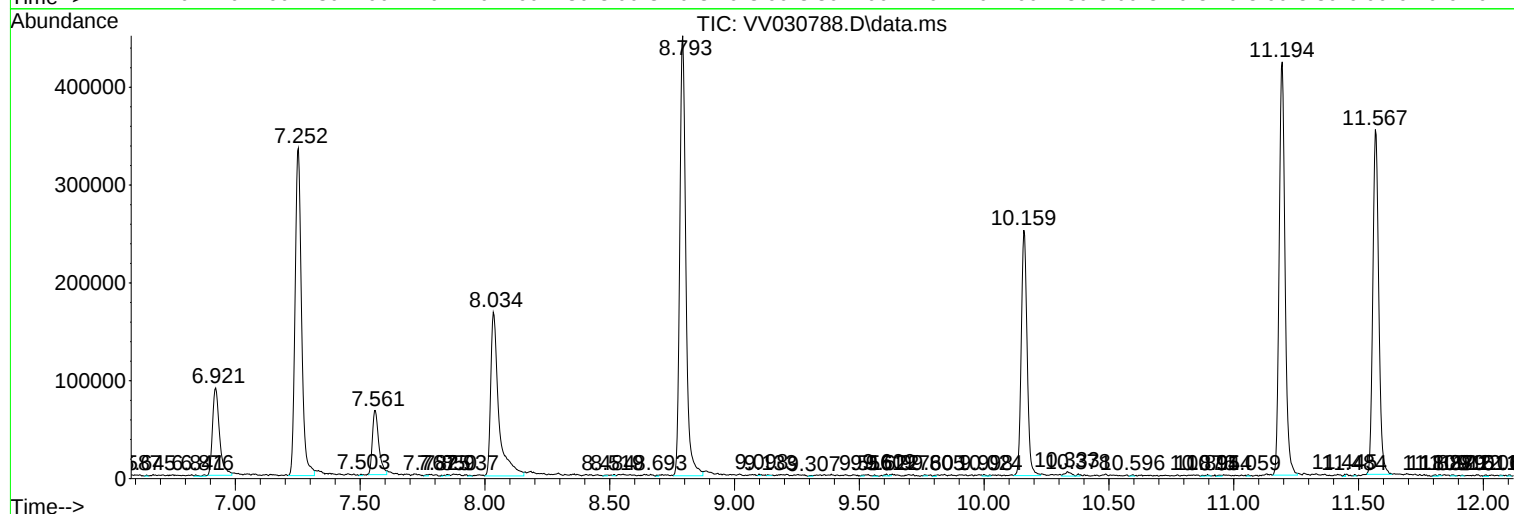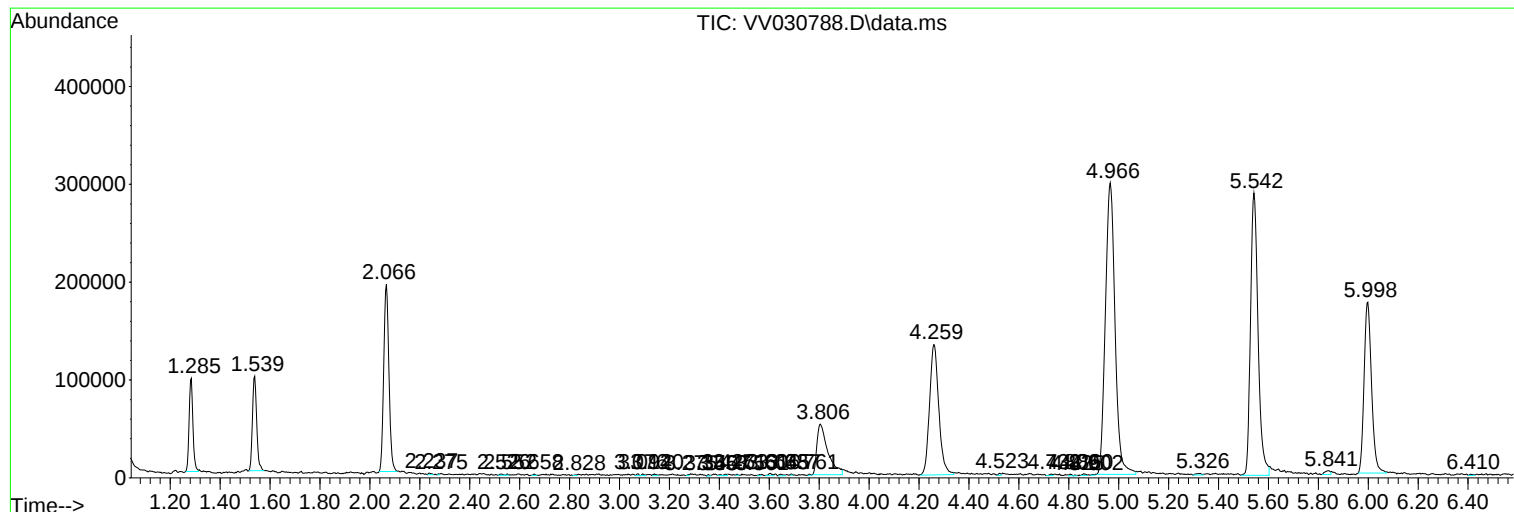

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
Data File : VV030788.D
Acq On : 24 Apr 2023 13:23
Operator : SY/MD
Sample : 02440-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0MQ5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
Data File : VV030788.D
Acq On : 24 Apr 2023 13:23
Operator : SY/MD
Sample : 02440-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0MQ5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc