

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
 Data File : VV030789.D
 Acq On : 24 Apr 2023 13:46
 Operator : SY/MD
 Sample : 02440-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMQ6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030789.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	91	rVB	78379	89184	12.79%	1.600%
2	1.539	148	155	169	rVB	80710	97307	13.96%	1.745%
3	2.066	309	319	330	rBV	165041	239014	34.28%	4.287%
4	2.606	483	487	490	rVV4	1144	906	0.13%	0.016%
5	2.780	534	541	542	rBV6	1306	1176	0.17%	0.021%
6	2.789	542	544	546	rBV2	1301	568	0.08%	0.010%
7	2.879	566	572	573	rBV6	1550	1502	0.22%	0.027%
8	2.989	603	606	610	rVB5	878	637	0.09%	0.011%
9	3.082	630	635	637	rBV6	849	564	0.08%	0.010%
10	3.095	637	639	641	rBV4	1582	946	0.14%	0.017%
11	3.117	644	646	656	rVB9	1509	2022	0.29%	0.036%
12	3.240	677	684	686	rBV8	580	638	0.09%	0.011%
13	3.294	696	701	703	rBV5	988	1037	0.15%	0.019%
14	3.346	712	717	719	rBV6	1562	1139	0.16%	0.020%
15	3.359	719	721	723	rVB3	1356	680	0.10%	0.012%
16	3.413	736	738	741	rBV4	1201	564	0.08%	0.010%
17	3.564	782	785	786	rBV3	953	551	0.08%	0.010%
18	3.735	836	838	842	rVB4	960	529	0.08%	0.009%
19	3.802	850	859	883	rBV	40267	120186	17.24%	2.156%
20	4.101	949	952	953	rBV3	998	523	0.08%	0.009%
21	4.262	986	1002	1023	rBV	113565	294312	42.21%	5.279%
22	4.558	1092	1094	1098	rBV5	1497	851	0.12%	0.015%
23	4.654	1121	1124	1125	rBV2	1347	539	0.08%	0.010%
24	4.818	1173	1175	1178	rBV4	1068	810	0.12%	0.015%
25	4.966	1203	1221	1252	rBV2	249817	697223	100.00%	12.506%
26	5.378	1347	1349	1355	rBV5	1237	1148	0.16%	0.021%
27	5.542	1386	1400	1425	rBV	241085	511950	73.43%	9.183%
28	5.998	1531	1542	1569	rVB	150333	307707	44.13%	5.519%
29	6.320	1640	1642	1646	rBV4	1246	1062	0.15%	0.019%
30	6.391	1661	1664	1669	rVB5	1924	1268	0.18%	0.023%
31	6.670	1748	1751	1754	rBV4	1334	1063	0.15%	0.019%
32	6.748	1773	1775	1778	rBV4	1755	940	0.13%	0.017%
33	6.773	1781	1783	1788	rBV5	1629	1474	0.21%	0.026%
34	6.812	1791	1795	1797	rBV5	743	515	0.07%	0.009%
35	6.921	1818	1829	1847	rBV	76102	149861	21.49%	2.688%
36	7.252	1921	1932	1946	rBV	278231	484591	69.50%	8.692%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
 Data File : VV030789.D
 Acq On : 24 Apr 2023 13:46
 Operator : SY/MD
 Sample : 02440-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMQ6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	7.561	2019	2028	2044	rBV2	54202	97646	14.00%	1.751%
38	7.873	2121	2125	2127	rBV3	1739	1222	0.18%	0.022%
39	8.037	2166	2176	2207	rBV	130228	281581	40.39%	5.051%
40	8.374	2278	2281	2283	rBV4	1666	1060	0.15%	0.019%
41	8.706	2383	2384	2387	rBV3	846	572	0.08%	0.010%
42	8.728	2389	2391	2395	rVB5	1276	659	0.09%	0.012%
43	8.792	2400	2411	2446	rVV	369146	697148	99.99%	12.505%
44	9.063	2491	2495	2496	rBV4	1242	950	0.14%	0.017%
45	9.162	2523	2526	2530	rBV7	1538	1142	0.16%	0.020%
46	9.246	2550	2552	2555	rBV3	943	638	0.09%	0.011%
47	9.300	2567	2569	2574	rVB5	2315	1606	0.23%	0.029%
48	9.326	2574	2577	2578	rBV2	1292	702	0.10%	0.013%
49	9.384	2593	2595	2597	rBV3	1221	629	0.09%	0.011%
50	9.487	2620	2627	2631	rBV7	3138	3463	0.50%	0.062%
51	9.516	2634	2636	2642	rVB6	1562	1072	0.15%	0.019%
52	9.670	2682	2684	2688	rVB4	1180	706	0.10%	0.013%
53	9.744	2704	2707	2709	rBV3	782	519	0.07%	0.009%
54	9.911	2757	2759	2761	rVB3	1811	690	0.10%	0.012%
55	9.931	2761	2765	2767	rBV5	1948	1292	0.19%	0.023%
56	9.995	2783	2785	2790	rVV5	818	814	0.12%	0.015%
57	10.079	2808	2811	2814	rVB5	813	541	0.08%	0.010%
58	10.111	2816	2821	2825	rVV6	1511	1122	0.16%	0.020%
59	10.159	2826	2836	2853	rVV	209248	338447	48.54%	6.071%
60	10.294	2876	2878	2881	rVB4	1165	664	0.10%	0.012%
61	10.336	2884	2891	2893	rBV8	3493	4328	0.62%	0.078%
62	10.468	2929	2932	2933	rBV3	1293	611	0.09%	0.011%
63	10.609	2972	2976	2981	rBV5	1426	991	0.14%	0.018%
64	10.805	3036	3037	3044	rVB6	1503	1465	0.21%	0.026%
65	10.841	3044	3048	3051	rBV6	1731	1630	0.23%	0.029%
66	10.895	3061	3065	3067	rBV4	1299	1111	0.16%	0.020%
67	10.934	3074	3077	3080	rVB4	1734	1122	0.16%	0.020%
68	10.960	3080	3085	3088	rBV5	1516	1687	0.24%	0.030%
69	11.005	3096	3099	3103	rVB3	1563	1244	0.18%	0.022%
70	11.046	3108	3112	3115	rVB5	1131	972	0.14%	0.017%
71	11.082	3121	3123	3125	rBV2	1352	684	0.10%	0.012%
72	11.194	3146	3158	3178	rBV	355053	596605	85.57%	10.701%
73	11.567	3263	3274	3290	rBV	293615	484819	69.54%	8.696%
74	11.744	3327	3329	3332	rBV4	1177	627	0.09%	0.011%
75	11.841	3355	3359	3362	rVB5	1183	823	0.12%	0.015%
76	11.863	3362	3366	3370	rBV7	1717	1597	0.23%	0.029%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
 Data File : VV030789.D
 Acq On : 24 Apr 2023 13:46
 Operator : SY/MD
 Sample : 02440-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMQ6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	11.882	3370	3372	3375	rBV3	1233	683	0.10%	0.012%
78	12.207	3471	3473	3479	rVB7	1492	1382	0.20%	0.025%
79	12.342	3510	3515	3517	rBV5	1784	1738	0.25%	0.031%
80	12.464	3551	3553	3556	rBV4	975	635	0.09%	0.011%
81	12.593	3588	3593	3594	rBV5	1342	1103	0.16%	0.020%
82	12.644	3604	3609	3611	rBV5	1389	1182	0.17%	0.021%
83	12.731	3632	3636	3639	rVB6	1473	997	0.14%	0.018%
84	12.770	3646	3648	3652	rVB4	999	564	0.08%	0.010%
85	12.812	3657	3661	3663	rVB4	1950	1328	0.19%	0.024%
86	12.844	3669	3671	3673	rBV3	1023	529	0.08%	0.009%
87	12.863	3673	3677	3678	rBV3	863	530	0.08%	0.010%
88	12.889	3683	3685	3687	rBV3	1116	620	0.09%	0.011%
89	12.902	3687	3689	3695	rVV6	1276	1116	0.16%	0.020%
90	13.098	3747	3750	3756	rVB7	1744	1624	0.23%	0.029%
91	13.194	3776	3780	3781	rBV4	1899	1201	0.17%	0.022%
92	13.307	3811	3815	3820	rBV6	2022	1992	0.29%	0.036%
93	13.619	3909	3912	3914	rBV4	1317	1122	0.16%	0.020%
94	13.683	3929	3932	3934	rBV4	1953	1384	0.20%	0.025%
95	13.722	3942	3944	3948	rVB5	1030	602	0.09%	0.011%
96	13.840	3977	3981	3982	rBV3	1793	1008	0.14%	0.018%
97	13.882	3991	3994	3997	rVB4	1480	886	0.13%	0.016%
98	13.959	4014	4018	4019	rBV3	1457	979	0.14%	0.018%
99	14.805	4279	4281	4284	rBV3	1100	704	0.10%	0.013%
100	15.101	4370	4373	4374	rBV3	1502	1057	0.15%	0.019%


Sum of corrected areas: 5575154

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
Data File : VV030789.D
Acq On : 24 Apr 2023 13:46
Operator : SY/MD
Sample : 02440-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMQ6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

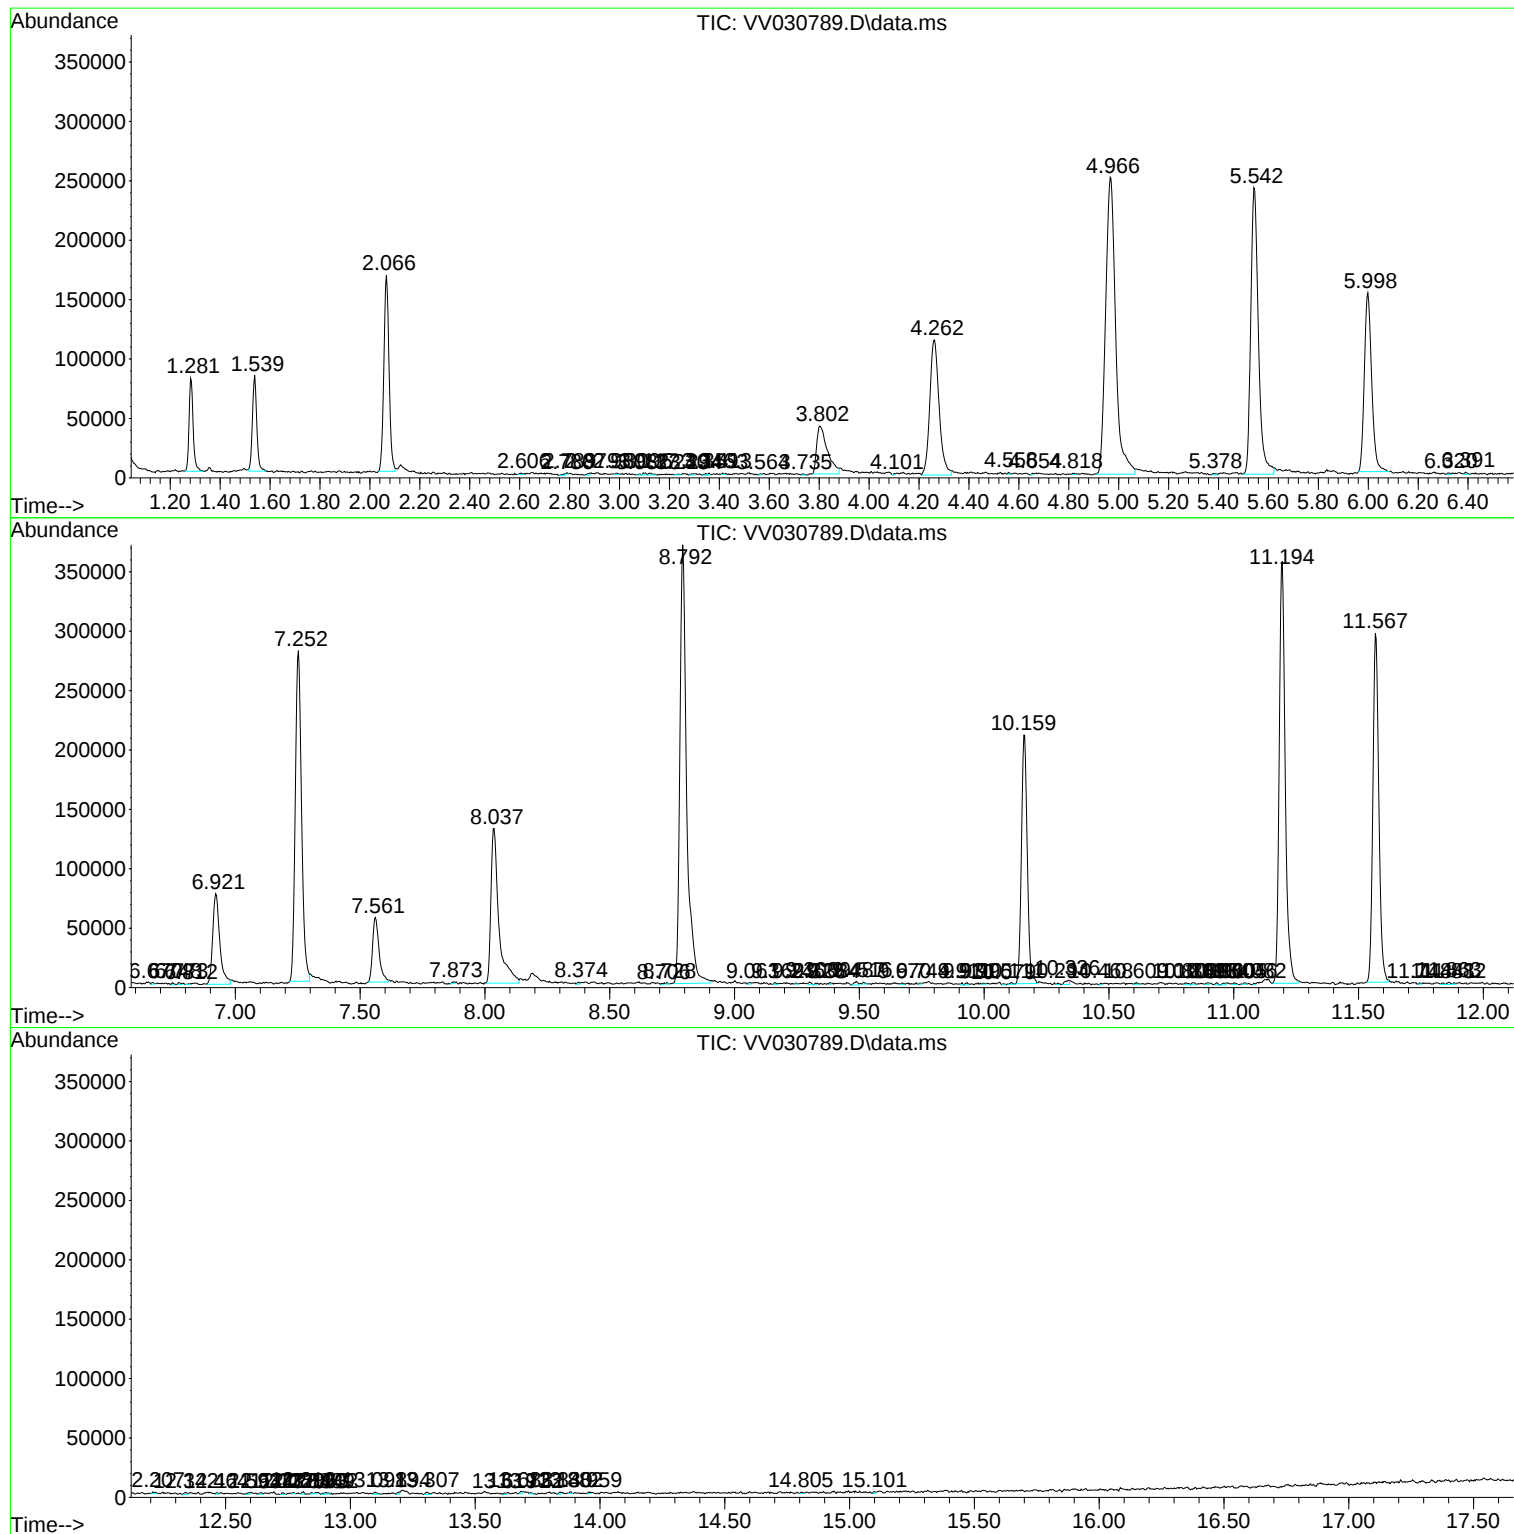

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
Data File : VV030789.D
Acq On : 24 Apr 2023 13:46
Operator : SY/MD
Sample : 02440-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0MQ6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
Data File : VV030789.D
Acq On : 24 Apr 2023 13:46
Operator : SY/MD
Sample : 02440-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0MQ6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------