

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
 Data File : VV030791.D
 Acq On : 24 Apr 2023 14:34
 Operator : SY/MD
 Sample : 02440-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMQ8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030791.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	89	rVB	82828	88610	12.45%	1.667%
2	1.535	148	154	164	rBV	75019	86105	12.09%	1.620%
3	2.066	310	319	331	rBV	169425	241045	33.86%	4.535%
4	2.359	407	410	415	rVB6	1761	1327	0.19%	0.025%
5	2.384	415	418	423	rVB6	1462	1255	0.18%	0.024%
6	2.410	424	426	428	rVB3	1583	595	0.08%	0.011%
7	2.484	448	449	452	rBV3	859	580	0.08%	0.011%
8	2.783	536	542	545	rVB6	1734	1923	0.27%	0.036%
9	2.818	545	553	560	rBV6	2063	3324	0.47%	0.063%
10	2.863	563	567	569	rVB5	1308	776	0.11%	0.015%
11	2.899	572	578	581	rBV7	2107	2241	0.31%	0.042%
12	2.960	593	597	599	rBV4	1438	943	0.13%	0.018%
13	3.095	637	639	644	rVB5	1405	895	0.13%	0.017%
14	3.137	650	652	656	rVB4	969	671	0.09%	0.013%
15	3.211	673	675	677	rBV3	1216	585	0.08%	0.011%
16	3.227	677	680	684	rBV7	935	785	0.11%	0.015%
17	3.378	726	727	732	rVB5	1779	993	0.14%	0.019%
18	3.407	732	736	737	rBV3	1279	982	0.14%	0.018%
19	3.468	753	755	763	rBV6	2013	2320	0.33%	0.044%
20	3.506	763	767	769	rBV3	1331	1042	0.15%	0.020%
21	3.696	822	826	827	rBV4	1097	654	0.09%	0.012%
22	3.725	831	835	836	rBV4	1093	658	0.09%	0.012%
23	3.735	836	838	843	rBV4	1735	1152	0.16%	0.022%
24	3.799	849	858	886	rBV2	44688	128353	18.03%	2.415%
25	4.056	936	938	941	rVB4	949	516	0.07%	0.010%
26	4.259	988	1001	1026	rBV2	113950	291208	40.90%	5.478%
27	4.432	1052	1055	1056	rBV3	1524	1040	0.15%	0.020%
28	4.596	1099	1106	1109	rBV6	1855	2291	0.32%	0.043%
29	4.757	1154	1156	1158	rBV4	1023	636	0.09%	0.012%
30	4.802	1167	1170	1174	rBV6	1198	847	0.12%	0.016%
31	4.966	1203	1221	1251	rBV2	263331	711913	100.00%	13.393%
32	5.323	1330	1332	1335	rBV4	1214	609	0.09%	0.011%
33	5.477	1377	1380	1382	rBV3	1317	892	0.13%	0.017%
34	5.542	1388	1400	1425	rBV	207675	432641	60.77%	8.139%
35	5.818	1480	1486	1489	rBV8	2340	2712	0.38%	0.051%
36	5.895	1508	1510	1514	rBV5	997	749	0.11%	0.014%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
 Data File : VV030791.D
 Acq On : 24 Apr 2023 14:34
 Operator : SY/MD
 Sample : 02440-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMQ8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	5.998	1530	1542	1562	rBV2	158084	322119	45.25%	6.060%
38	6.198	1602	1604	1605	rBV2	1189	554	0.08%	0.010%
39	6.275	1626	1628	1631	rBV4	1687	1053	0.15%	0.020%
40	6.352	1649	1652	1655	rBV4	1310	981	0.14%	0.018%
41	6.506	1698	1700	1701	rBV2	1228	633	0.09%	0.012%
42	6.809	1792	1794	1796	rBV3	1013	688	0.10%	0.013%
43	6.886	1816	1818	1819	rBV2	1359	517	0.07%	0.010%
44	6.921	1819	1829	1846	rBV	77151	149056	20.94%	2.804%
45	7.162	1902	1904	1905	rBV3	1699	671	0.09%	0.013%
46	7.252	1919	1932	1950	rBV	286660	514597	72.28%	9.681%
47	7.561	2019	2028	2044	rBV	57817	106271	14.93%	1.999%
48	7.722	2076	2078	2080	rBV2	1072	568	0.08%	0.011%
49	7.860	2118	2121	2123	rBV4	1468	988	0.14%	0.019%
50	7.934	2142	2144	2147	rBV3	1415	763	0.11%	0.014%
51	8.034	2166	2175	2205	rBV	139908	291830	40.99%	5.490%
52	8.577	2342	2344	2346	rBV2	1350	720	0.10%	0.014%
53	8.696	2379	2381	2383	rBV2	1138	709	0.10%	0.013%
54	8.792	2399	2411	2431	rBV	311897	529267	74.34%	9.957%
55	9.194	2531	2536	2539	rBV7	1498	1356	0.19%	0.026%
56	9.288	2563	2565	2569	rBV4	1459	753	0.11%	0.014%
57	9.407	2600	2602	2604	rBV3	902	665	0.09%	0.013%
58	9.448	2612	2615	2619	rBV6	1719	1798	0.25%	0.034%
59	9.574	2651	2654	2657	rBV5	1392	1293	0.18%	0.024%
60	9.763	2709	2713	2715	rBV5	1279	989	0.14%	0.019%
61	9.886	2749	2751	2756	rVB6	1880	1115	0.16%	0.021%
62	9.924	2756	2763	2765	rBV8	1646	1560	0.22%	0.029%
63	10.159	2824	2836	2855	rBV	216818	354587	49.81%	6.671%
64	10.249	2861	2864	2865	rBV3	1213	705	0.10%	0.013%
65	10.268	2868	2870	2873	rVB3	1714	872	0.12%	0.016%
66	10.484	2933	2937	2940	rVB4	1167	838	0.12%	0.016%
67	10.570	2958	2964	2965	rBV5	1303	1072	0.15%	0.020%
68	10.644	2985	2987	2995	rVB7	1566	1285	0.18%	0.024%
69	10.722	3009	3011	3017	rVB7	1455	857	0.12%	0.016%
70	10.767	3023	3025	3030	rVB5	1289	819	0.12%	0.015%
71	10.966	3083	3087	3090	rBV5	1399	1043	0.15%	0.020%
72	11.075	3119	3121	3124	rBV4	899	639	0.09%	0.012%
73	11.133	3136	3139	3143	rBV5	1643	1360	0.19%	0.026%
74	11.194	3146	3158	3177	rBV	304893	492796	69.22%	9.271%
75	11.570	3264	3275	3294	rVB	298765	488707	68.65%	9.194%
76	12.001	3407	3409	3414	rBV6	1350	742	0.10%	0.014%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
 Data File : VV030791.D
 Acq On : 24 Apr 2023 14:34
 Operator : SY/MD
 Sample : 02440-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMQ8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	12.136	3447	3451	3455	rBV6	1447	1126	0.16%	0.021%
78	12.188	3463	3467	3471	rBV4	1937	1383	0.19%	0.026%
79	12.236	3479	3482	3483	rBV3	898	547	0.08%	0.010%
80	12.291	3494	3499	3500	rBV4	1411	1251	0.18%	0.024%
81	12.377	3524	3526	3530	rVB5	1366	696	0.10%	0.013%
82	12.448	3542	3548	3550	rBV6	1782	1851	0.26%	0.035%
83	12.567	3582	3585	3590	rBV6	1447	1036	0.15%	0.019%
84	12.593	3591	3593	3598	rVV6	1611	878	0.12%	0.017%
85	12.635	3604	3606	3608	rBV3	1026	539	0.08%	0.010%
86	12.699	3624	3626	3628	rBV3	1406	932	0.13%	0.018%
87	12.940	3698	3701	3703	rBV2	1403	990	0.14%	0.019%
88	13.001	3718	3720	3725	rVB7	1731	897	0.13%	0.017%
89	13.059	3736	3738	3743	rVB5	1172	728	0.10%	0.014%
90	13.320	3816	3819	3821	rBV4	1100	767	0.11%	0.014%
91	13.368	3829	3834	3838	rBV7	1279	1460	0.21%	0.027%
92	13.397	3838	3843	3844	rBV5	1035	1001	0.14%	0.019%
93	13.554	3888	3892	3896	rBV7	1769	1600	0.22%	0.030%
94	13.799	3966	3968	3971	rBV3	1171	776	0.11%	0.015%
95	13.844	3980	3982	3983	rBV2	1164	610	0.09%	0.011%
96	14.123	4066	4069	4073	rBV4	1686	1679	0.24%	0.032%
97	14.400	4153	4155	4158	rBV4	1027	547	0.08%	0.010%
98	14.455	4170	4172	4174	rBV3	1335	812	0.11%	0.015%
99	14.532	4193	4196	4198	rBV3	1298	705	0.10%	0.013%
100	14.898	4308	4310	4313	rBV3	1421	976	0.14%	0.018%




Sum of corrected areas: 5315491

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
Data File : VV030791.D
Acq On : 24 Apr 2023 14:34
Operator : SY/MD
Sample : 02440-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMQ8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

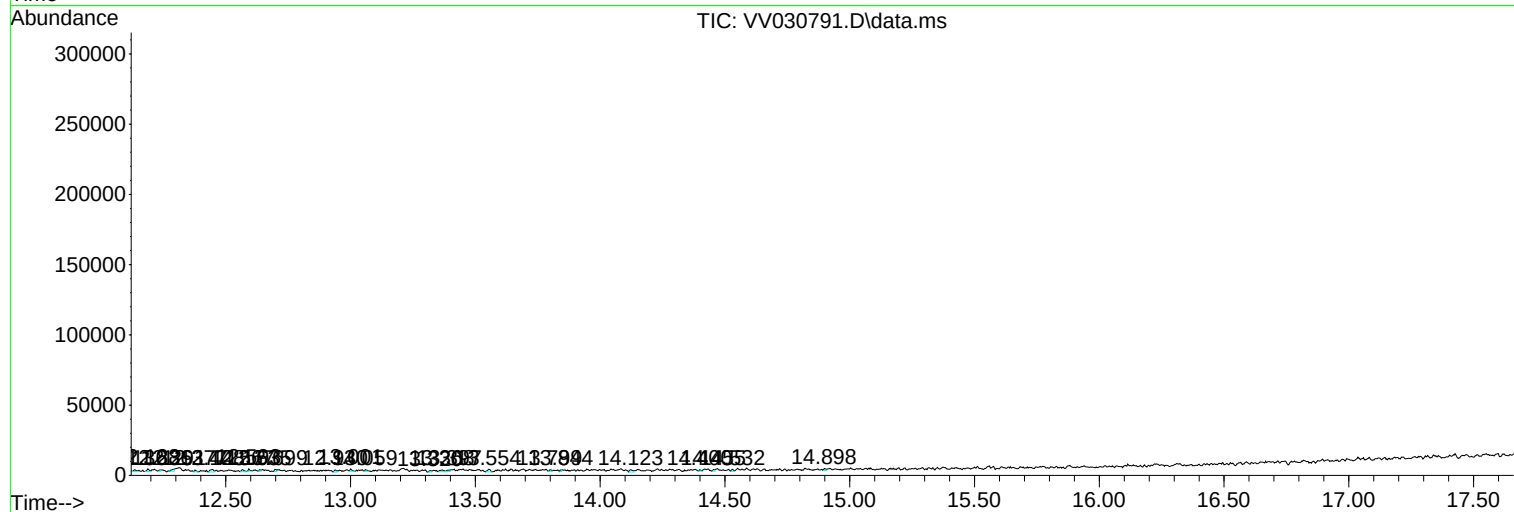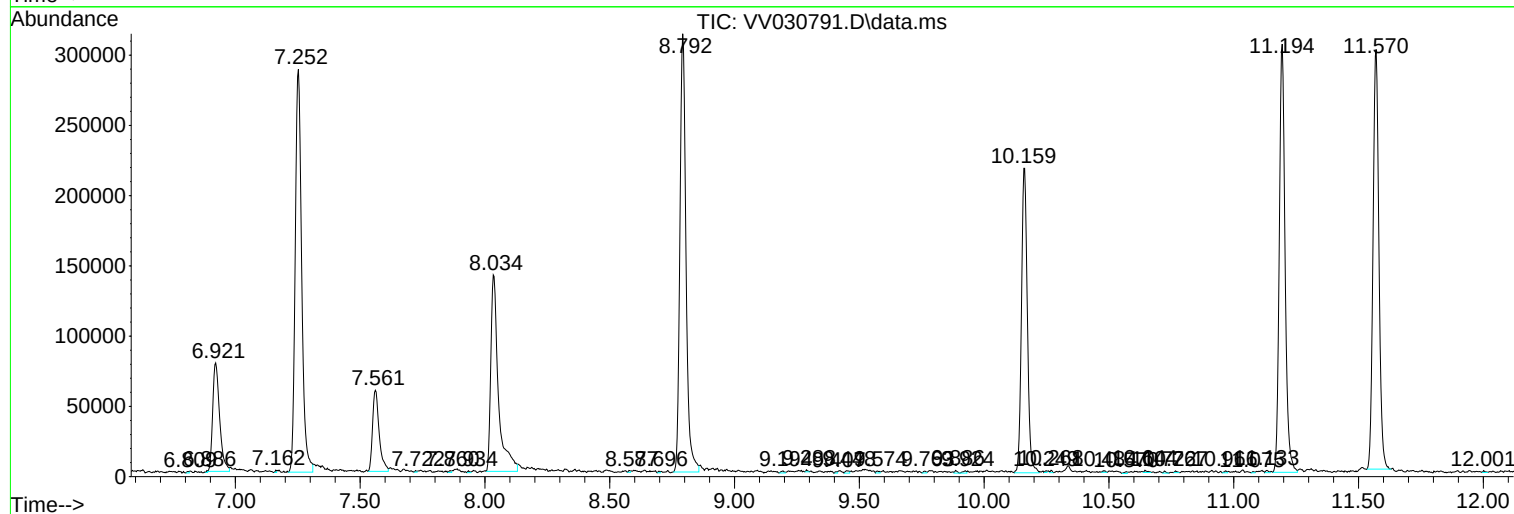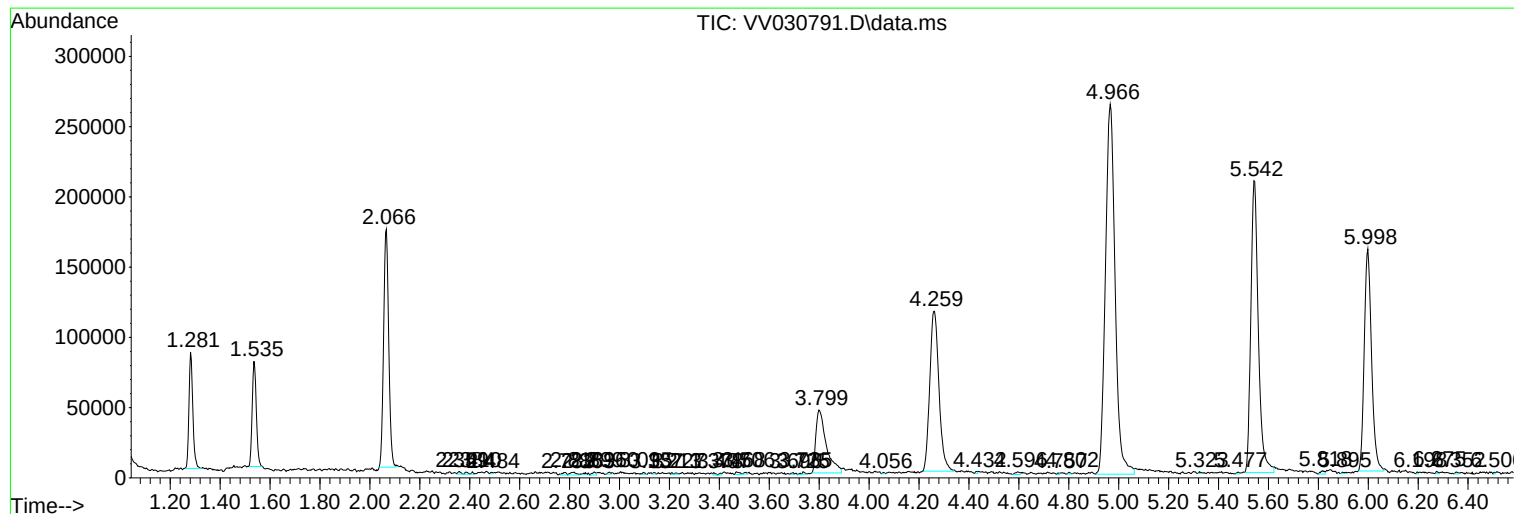

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
Data File : VV030791.D
Acq On : 24 Apr 2023 14:34
Operator : SY/MD
Sample : 02440-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0MQ8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
Data File : VV030791.D
Acq On : 24 Apr 2023 14:34
Operator : SY/MD
Sample : 02440-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0MQ8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc