

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
 Data File : VV030792.D
 Acq On : 24 Apr 2023 14:58
 Operator : SY/MD
 Sample : 02440-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMQ9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030792.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	69	75	85	rBV	75874	81067	12.62%	1.579%
2	1.536	148	154	168	rVB	74033	86197	13.42%	1.679%
3	2.066	310	319	332	rBV	155568	225674	35.14%	4.396%
4	2.539	463	466	473	rBV7	1852	1804	0.28%	0.035%
5	2.581	474	479	480	rBV3	1315	891	0.14%	0.017%
6	2.831	554	557	559	rBV3	1448	931	0.14%	0.018%
7	2.863	565	567	571	rBV4	1362	1130	0.18%	0.022%
8	2.950	592	594	596	rBV3	685	487	0.08%	0.009%
9	3.034	616	620	622	rBV3	1093	636	0.10%	0.012%
10	3.159	656	659	664	rVB7	1829	1292	0.20%	0.025%
11	3.191	667	669	672	rVB4	811	417	0.06%	0.008%
12	3.211	672	675	676	rBV3	1563	714	0.11%	0.014%
13	3.307	701	705	706	rBV3	1425	775	0.12%	0.015%
14	3.375	724	726	733	rBV8	2035	2537	0.40%	0.049%
15	3.510	765	768	770	rBV3	1046	827	0.13%	0.016%
16	3.568	784	786	788	rBV3	743	400	0.06%	0.008%
17	3.580	788	790	791	rBV2	1310	479	0.07%	0.009%
18	3.703	825	828	829	rBV3	1557	577	0.09%	0.011%
19	3.802	848	859	882	rBV2	41602	118726	18.49%	2.313%
20	4.188	976	979	980	rBV3	861	448	0.07%	0.009%
21	4.262	988	1002	1024	rVB2	105412	266801	41.55%	5.197%
22	4.860	1185	1188	1191	rVB5	1331	916	0.14%	0.018%
23	4.902	1198	1201	1203	rBV4	1430	900	0.14%	0.018%
24	4.966	1203	1221	1245	rVV2	242632	642170	100.00%	12.510%
25	5.336	1329	1336	1340	rBV2	2093	2681	0.42%	0.052%
26	5.391	1351	1353	1357	rVB4	1889	1237	0.19%	0.024%
27	5.420	1360	1362	1364	rBV2	2325	1022	0.16%	0.020%
28	5.542	1388	1400	1422	rBV	228520	472359	73.56%	9.202%
29	5.998	1531	1542	1563	rVB	143984	288895	44.99%	5.628%
30	6.211	1606	1608	1611	rBV4	912	402	0.06%	0.008%
31	6.333	1642	1646	1647	rBV4	978	467	0.07%	0.009%
32	6.387	1660	1663	1666	rVB5	1281	966	0.15%	0.019%
33	6.522	1702	1705	1707	rBV3	860	730	0.11%	0.014%
34	6.632	1737	1739	1743	rBV4	1119	791	0.12%	0.015%
35	6.825	1797	1799	1800	rBV2	1374	501	0.08%	0.010%
36	6.921	1819	1829	1841	rBV	69514	129655	20.19%	2.526%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042423\
 Data File : VW030792.D
 Acq On : 24 Apr 2023 14:58
 Operator : SY/MD
 Sample : 02440-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMQ9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	7.085	1877	1880	1882	rBV3	1337	774	0.12%	0.015%
38	7.188	1910	1912	1915	rBV4	1214	691	0.11%	0.013%
39	7.252	1919	1932	1949	rBV	265161	471165	73.37%	9.179%
40	7.529	2014	2018	2019	rBV4	1417	954	0.15%	0.019%
41	7.561	2019	2028	2047	rVV	53223	99151	15.44%	1.932%
42	7.735	2078	2082	2085	rBV5	1971	1487	0.23%	0.029%
43	7.789	2098	2099	2102	rBV3	907	411	0.06%	0.008%
44	7.818	2106	2108	2110	rBV3	1220	683	0.11%	0.013%
45	7.886	2122	2129	2134	rBV7	3201	3973	0.62%	0.077%
46	7.937	2136	2145	2147	rBV8	1679	2113	0.33%	0.041%
47	8.034	2166	2175	2194	rBV	128779	256712	39.98%	5.001%
48	8.471	2309	2311	2316	rBV5	973	666	0.10%	0.013%
49	8.674	2371	2374	2378	rVB5	1722	1294	0.20%	0.025%
50	8.693	2378	2380	2382	rBV3	846	530	0.08%	0.010%
51	8.706	2382	2384	2385	rBV2	1113	422	0.07%	0.008%
52	8.792	2399	2411	2435	rBV	344721	590987	92.03%	11.513%
53	9.230	2545	2547	2551	rBV5	1272	1065	0.17%	0.021%
54	10.066	2804	2807	2812	rBV8	1417	1136	0.18%	0.022%
55	10.162	2824	2837	2854	rBV	202290	325055	50.62%	6.332%
56	10.291	2875	2877	2879	rBV2	1183	593	0.09%	0.012%
57	10.407	2912	2913	2915	rVB2	1369	482	0.08%	0.009%
58	10.423	2915	2918	2921	rBV4	860	548	0.09%	0.011%
59	10.439	2921	2923	2927	rVB4	1030	678	0.11%	0.013%
60	10.464	2927	2931	2937	rBV8	1569	1751	0.27%	0.034%
61	10.545	2954	2956	2959	rBV3	1316	765	0.12%	0.015%
62	10.648	2983	2988	2992	rVB6	2070	2209	0.34%	0.043%
63	10.677	2992	2997	2999	rBV6	1739	1488	0.23%	0.029%
64	10.709	3004	3007	3009	rVB4	1245	621	0.10%	0.012%
65	10.799	3033	3035	3039	rVB4	2166	1473	0.23%	0.029%
66	10.821	3039	3042	3044	rBV4	1226	665	0.10%	0.013%
67	10.837	3044	3047	3049	rBV2	1012	395	0.06%	0.008%
68	10.960	3081	3085	3086	rBV4	849	588	0.09%	0.011%
69	10.985	3091	3093	3094	rBV2	1097	434	0.07%	0.008%
70	11.104	3126	3130	3132	rBV3	1246	871	0.14%	0.017%
71	11.194	3147	3158	3175	rBV	328137	537371	83.68%	10.468%
72	11.339	3201	3203	3207	rVB5	1862	1046	0.16%	0.020%
73	11.503	3246	3254	3255	rBV7	7747	7697	1.20%	0.150%
74	11.571	3264	3275	3292	rVB	285604	457822	71.29%	8.919%
75	11.831	3354	3356	3358	rBV2	1330	907	0.14%	0.018%
76	11.998	3405	3408	3410	rBV4	1157	744	0.12%	0.014%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
 Data File : VV030792.D
 Acq On : 24 Apr 2023 14:58
 Operator : SY/MD
 Sample : 02440-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMQ9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	12.050	3421	3424	3425	rBV3	1680	1003	0.16%	0.020%
78	12.172	3460	3462	3466	rBV5	1168	852	0.13%	0.017%
79	12.252	3485	3487	3490	rVB4	1224	719	0.11%	0.014%
80	12.641	3606	3608	3609	rBV3	1279	528	0.08%	0.010%
81	12.796	3654	3656	3660	rBV4	1122	957	0.15%	0.019%
82	12.921	3693	3695	3699	rVB5	1090	448	0.07%	0.009%
83	13.011	3721	3723	3725	rBV2	862	527	0.08%	0.010%
84	13.101	3749	3751	3752	rBV2	1065	472	0.07%	0.009%
85	13.162	3768	3770	3772	rBV3	1113	565	0.09%	0.011%
86	13.239	3792	3794	3798	rVB5	1413	827	0.13%	0.016%
87	13.268	3801	3803	3805	rBV3	941	583	0.09%	0.011%
88	13.304	3811	3814	3817	rBV5	1005	732	0.11%	0.014%
89	13.403	3843	3845	3848	rVB4	1345	768	0.12%	0.015%
90	13.445	3856	3858	3860	rBV3	1324	598	0.09%	0.012%
91	13.509	3875	3878	3879	rBV3	732	420	0.07%	0.008%
92	13.824	3970	3976	3978	rBV6	1600	1361	0.21%	0.027%
93	13.860	3983	3987	3989	rBV5	1894	1499	0.23%	0.029%
94	13.953	4014	4016	4019	rVB4	1144	588	0.09%	0.011%
95	13.979	4019	4024	4026	rBV6	1911	1727	0.27%	0.034%
96	14.088	4056	4058	4061	rBV4	1058	457	0.07%	0.009%
97	14.107	4061	4064	4065	rBV3	922	630	0.10%	0.012%
98	14.496	4182	4185	4187	rBV4	1361	789	0.12%	0.015%
99	15.098	4369	4372	4373	rBV3	1255	611	0.10%	0.012%
100	15.127	4380	4381	4384	rVB2	1787	740	0.12%	0.014%




Sum of corrected areas: 5133320

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
Data File : VV030792.D
Acq On : 24 Apr 2023 14:58
Operator : SY/MD
Sample : 02440-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMQ9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

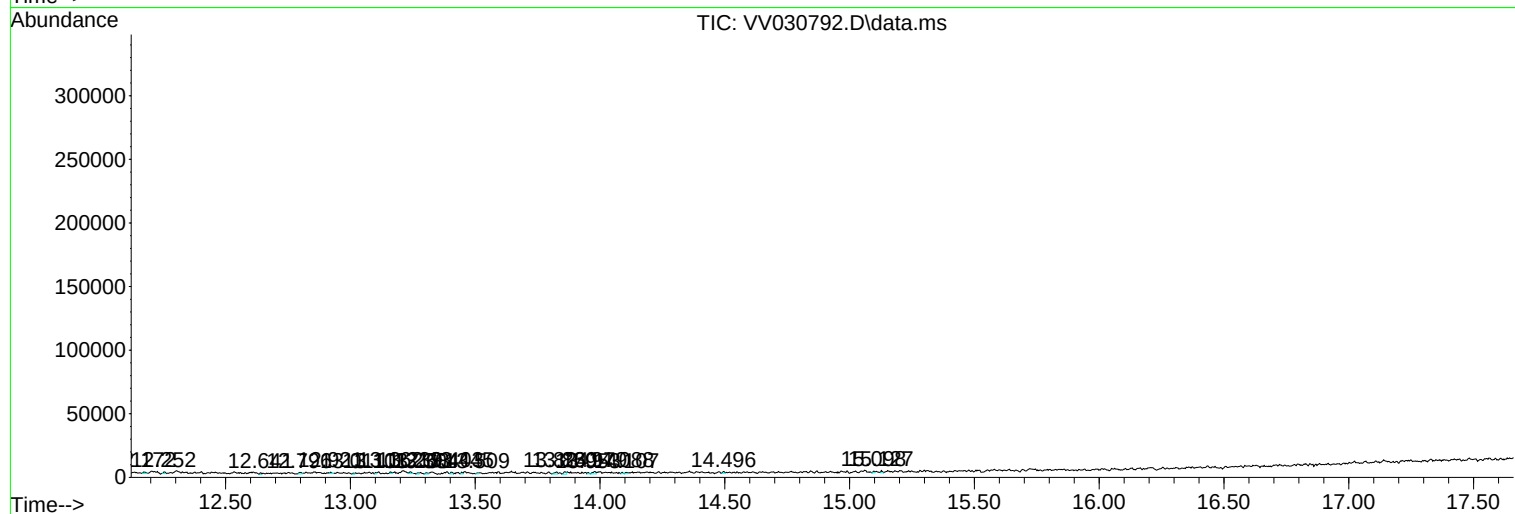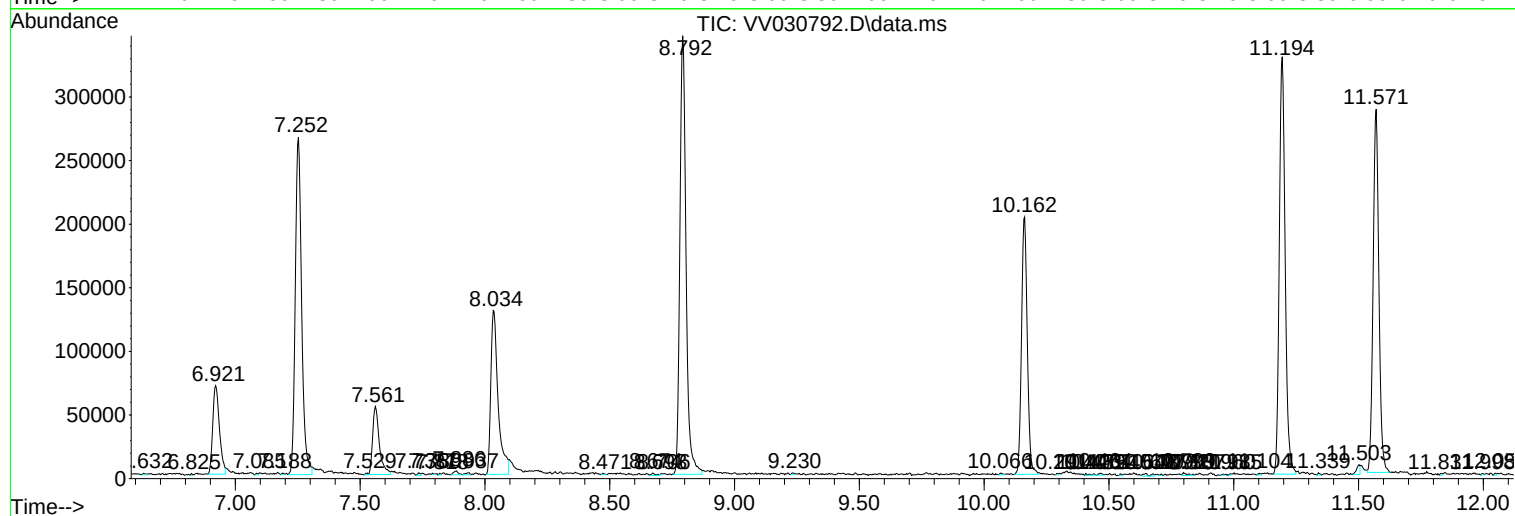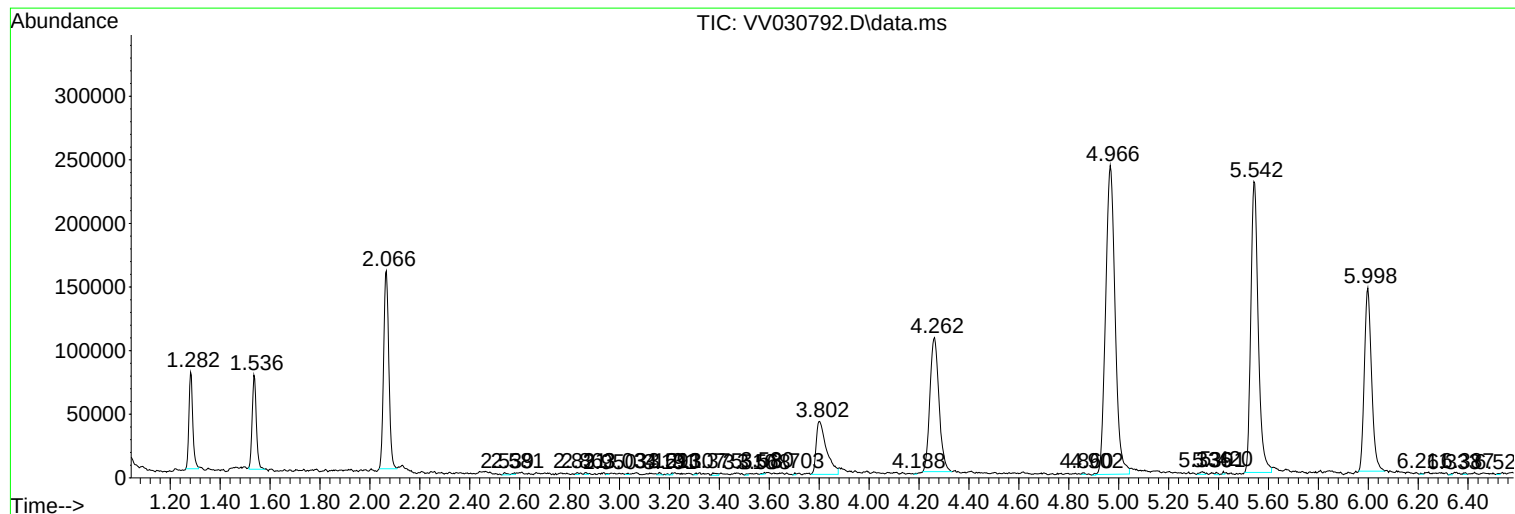

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
Data File : VV030792.D
Acq On : 24 Apr 2023 14:58
Operator : SY/MD
Sample : 02440-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0MQ9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
Data File : VV030792.D
Acq On : 24 Apr 2023 14:58
Operator : SY/MD
Sample : 02440-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0MQ9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------