

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
 Data File : VV030793.D
 Acq On : 24 Apr 2023 15:22
 Operator : SY/MD
 Sample : 02440-15 20X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMR0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M

Title : VOC Analysis

Signal : TIC: VV030793.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	69	75	89	rBV	122675	133622	8.13%	1.545%
2	1.536	148	154	165	rVB	111292	131132	7.98%	1.516%
3	2.066	310	319	338	rVB	236992	347004	21.11%	4.013%
4	2.163	347	349	351	rBV3	1858	916	0.06%	0.011%
5	2.417	426	428	432	rBV4	1147	718	0.04%	0.008%
6	2.442	433	436	437	rBV3	1341	802	0.05%	0.009%
7	2.568	473	475	478	rBV4	1393	991	0.06%	0.011%
8	2.587	478	481	482	rBV3	781	420	0.03%	0.005%
9	2.696	511	515	516	rBV4	1050	845	0.05%	0.010%
10	3.085	634	636	638	rBV3	969	591	0.04%	0.007%
11	3.147	652	655	659	rVB4	1642	1468	0.09%	0.017%
12	3.182	659	666	668	rBV7	1873	1832	0.11%	0.021%
13	3.201	669	672	673	rBV2	1144	518	0.03%	0.006%
14	3.275	692	695	697	rVB4	1188	654	0.04%	0.008%
15	3.407	734	736	738	rBV2	892	569	0.03%	0.007%
16	3.529	771	774	776	rBV3	969	549	0.03%	0.006%
17	3.581	788	790	792	rBV3	1099	658	0.04%	0.008%
18	3.616	796	801	804	rBV5	1213	1372	0.08%	0.016%
19	3.680	819	821	826	rBV5	967	830	0.05%	0.010%
20	3.706	826	829	833	rBV5	1301	1158	0.07%	0.013%
21	3.748	841	842	844	rBV2	860	481	0.03%	0.006%
22	3.796	848	857	878	rVV	58858	159555	9.71%	1.845%
23	4.130	958	961	963	rBV4	1189	779	0.05%	0.009%
24	4.259	988	1001	1020	rBV2	154530	378060	23.00%	4.372%
25	4.597	1103	1106	1108	rBV4	802	457	0.03%	0.005%
26	4.664	1125	1127	1129	rBV3	999	368	0.02%	0.004%
27	4.690	1132	1135	1139	rVB5	1427	1210	0.07%	0.014%
28	4.709	1139	1141	1142	rBV2	1066	354	0.02%	0.004%
29	4.748	1151	1153	1154	rBV2	1389	596	0.04%	0.007%
30	4.876	1190	1193	1194	rBV2	799	540	0.03%	0.006%
31	4.966	1203	1221	1246	rBV2	360062	965747	58.75%	11.168%
32	5.352	1339	1341	1342	rBV2	1325	678	0.04%	0.008%
33	5.426	1363	1364	1366	rBV2	987	514	0.03%	0.006%
34	5.542	1388	1400	1428	rBV	287311	606035	36.87%	7.008%
35	5.995	1529	1541	1564	rBV	209879	434162	26.41%	5.021%
36	6.207	1605	1607	1610	rBV4	758	358	0.02%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042423\
 Data File : VW030793.D
 Acq On : 24 Apr 2023 15:22
 Operator : SY/MD
 Sample : 02440-15 20X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMR0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	6.410	1668	1670	1674	rVB5	1465	1038	0.06%	0.012%
38	6.445	1677	1681	1683	rBV5	1329	1038	0.06%	0.012%
39	6.551	1709	1714	1717	rBV6	1757	1971	0.12%	0.023%
40	6.783	1784	1786	1790	rBV6	1989	1258	0.08%	0.015%
41	6.918	1819	1828	1845	rBV	107898	202354	12.31%	2.340%
42	7.079	1876	1878	1880	rBV3	1643	950	0.06%	0.011%
43	7.156	1900	1902	1907	rVB4	1183	600	0.04%	0.007%
44	7.252	1920	1932	1950	rBV	414224	734265	44.67%	8.491%
45	7.478	2000	2002	2003	rBV	977	329	0.02%	0.004%
46	7.558	2018	2027	2046	rBV	83124	150667	9.17%	1.742%
47	7.889	2128	2130	2133	rBV4	1420	663	0.04%	0.008%
48	7.960	2147	2152	2154	rBV5	1745	1631	0.10%	0.019%
49	8.034	2165	2175	2209	rBV	189454	386928	23.54%	4.475%
50	8.503	2319	2321	2324	rBV3	1425	1056	0.06%	0.012%
51	8.584	2344	2346	2348	rBV2	1342	728	0.04%	0.008%
52	8.793	2399	2411	2438	rBV	448533	833416	50.70%	9.638%
53	9.143	2517	2520	2521	rBV4	1584	939	0.06%	0.011%
54	9.288	2563	2565	2571	rVB7	1743	1022	0.06%	0.012%
55	9.461	2617	2619	2620	rVB2	1419	455	0.03%	0.005%
56	9.516	2632	2636	2638	rBV5	1614	1080	0.07%	0.012%
57	9.529	2638	2640	2645	rBV4	1040	864	0.05%	0.010%
58	9.622	2665	2669	2671	rBV5	1086	961	0.06%	0.011%
59	9.674	2683	2685	2687	rBV3	742	446	0.03%	0.005%
60	9.812	2723	2728	2730	rBV5	1992	1493	0.09%	0.017%
61	9.969	2773	2777	2780	rBV5	1546	1169	0.07%	0.014%
62	10.002	2785	2787	2789	rBV3	987	598	0.04%	0.007%
63	10.095	2814	2816	2822	rVB6	1149	1128	0.07%	0.013%
64	10.159	2825	2836	2849	rBV	290725	459011	27.93%	5.308%
65	10.301	2878	2880	2881	rBV2	1162	400	0.02%	0.005%
66	10.442	2922	2924	2927	rVB4	1335	681	0.04%	0.008%
67	10.461	2928	2930	2933	rBV4	824	513	0.03%	0.006%
68	10.490	2938	2939	2941	rBV2	737	366	0.02%	0.004%
69	10.590	2968	2970	2971	rBV2	1067	356	0.02%	0.004%
70	10.635	2979	2984	2985	rBV5	1533	866	0.05%	0.010%
71	10.680	2993	2998	3001	rBV7	2264	1997	0.12%	0.023%
72	10.799	3031	3035	3037	rBV4	2347	1425	0.09%	0.016%
73	10.831	3041	3045	3047	rBV5	1539	1420	0.09%	0.016%
74	10.873	3056	3058	3060	rBV2	1524	793	0.05%	0.009%
75	11.021	3102	3104	3107	rVB4	1181	613	0.04%	0.007%
76	11.127	3130	3137	3147	rBV2	20552	31653	1.93%	0.366%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
 Data File : VV030793.D
 Acq On : 24 Apr 2023 15:22
 Operator : SY/MD
 Sample : 02440-15 20X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMR0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	11.194	3147	3158	3185	rVB2	441686	841527	51.20%	9.732%
78	11.583	3264	3279	3298	rBV3	734955	1643719	100.00%	19.008%
79	11.828	3351	3355	3358	rBV5	2219	2032	0.12%	0.023%
80	11.966	3396	3398	3400	rBV2	1134	702	0.04%	0.008%
81	12.082	3430	3434	3435	rBV3	1917	1079	0.07%	0.012%
82	12.198	3468	3470	3475	rVB4	1696	1229	0.07%	0.014%
83	12.284	3494	3497	3501	rBV6	1146	1093	0.07%	0.013%
84	12.362	3518	3521	3525	rBV4	1569	1180	0.07%	0.014%
85	12.391	3528	3530	3532	rBV2	1308	647	0.04%	0.007%
86	12.574	3583	3587	3589	rBV5	2205	1632	0.10%	0.019%
87	12.622	3599	3602	3603	rBV3	992	551	0.03%	0.006%
88	12.870	3674	3679	3680	rBV5	1810	1336	0.08%	0.015%
89	12.995	3716	3718	3719	rBV2	1052	421	0.03%	0.005%
90	13.165	3769	3771	3773	rBV3	1114	449	0.03%	0.005%
91	13.207	3775	3784	3797	rVB	70589	111187	6.76%	1.286%
92	13.342	3819	3826	3830	rBV8	1689	2342	0.14%	0.027%
93	13.490	3870	3872	3876	rBV5	1350	767	0.05%	0.009%
94	13.689	3928	3934	3948	rVB3	14514	25039	1.52%	0.290%
95	13.757	3953	3955	3957	rBV2	1046	402	0.02%	0.005%
96	13.770	3957	3959	3964	rBV6	1176	941	0.06%	0.011%
97	13.837	3978	3980	3982	rBV3	1296	592	0.04%	0.007%
98	14.403	4153	4156	4157	rBV3	1404	780	0.05%	0.009%
99	14.548	4199	4201	4204	rBV4	1630	897	0.05%	0.010%
100	14.879	4300	4304	4305	rBV4	1612	1069	0.07%	0.012%




Sum of corrected areas: 8647297

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
Data File : VV030793.D
Acq On : 24 Apr 2023 15:22
Operator : SY/MD
Sample : 02440-15 20X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMR0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

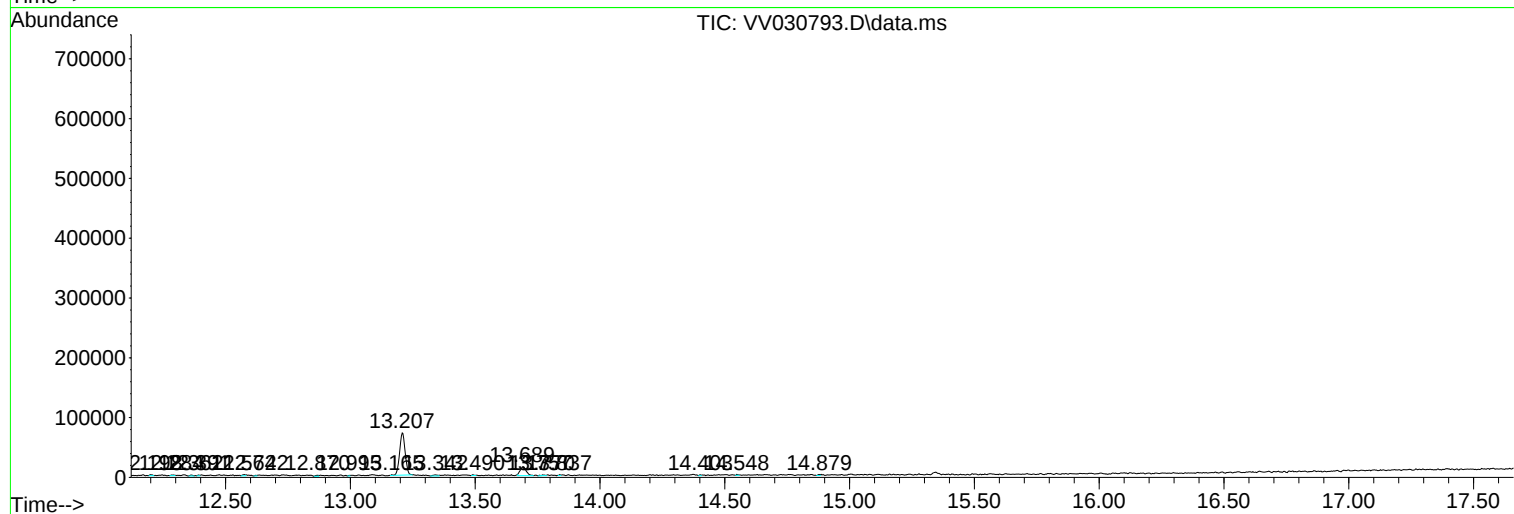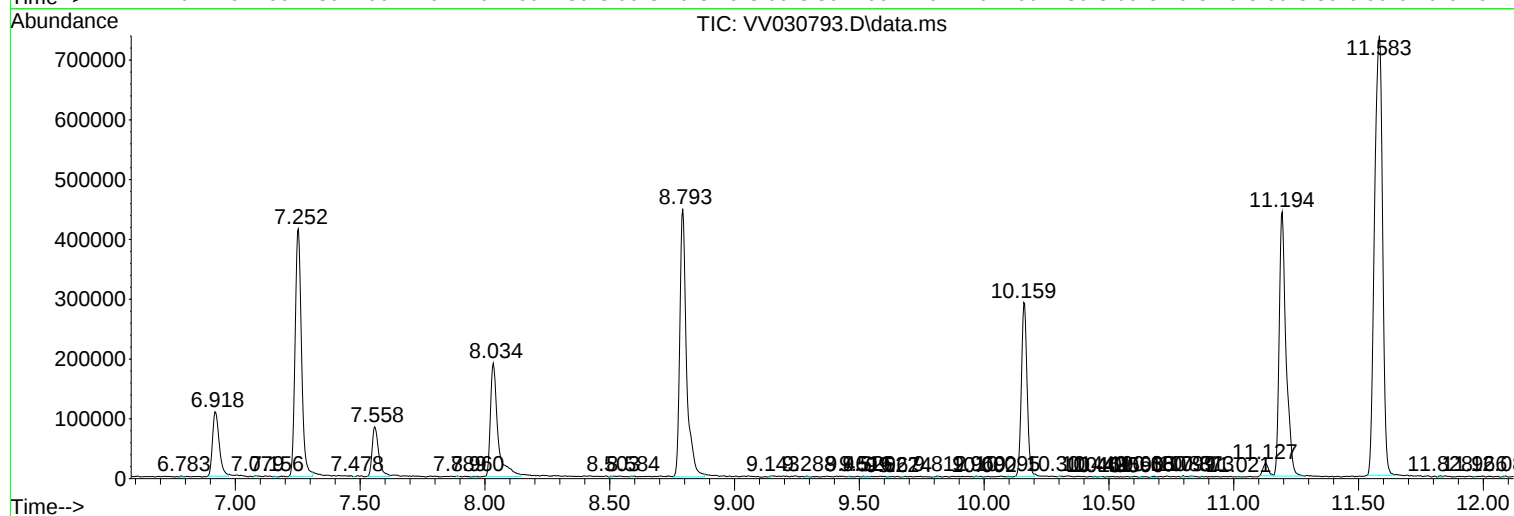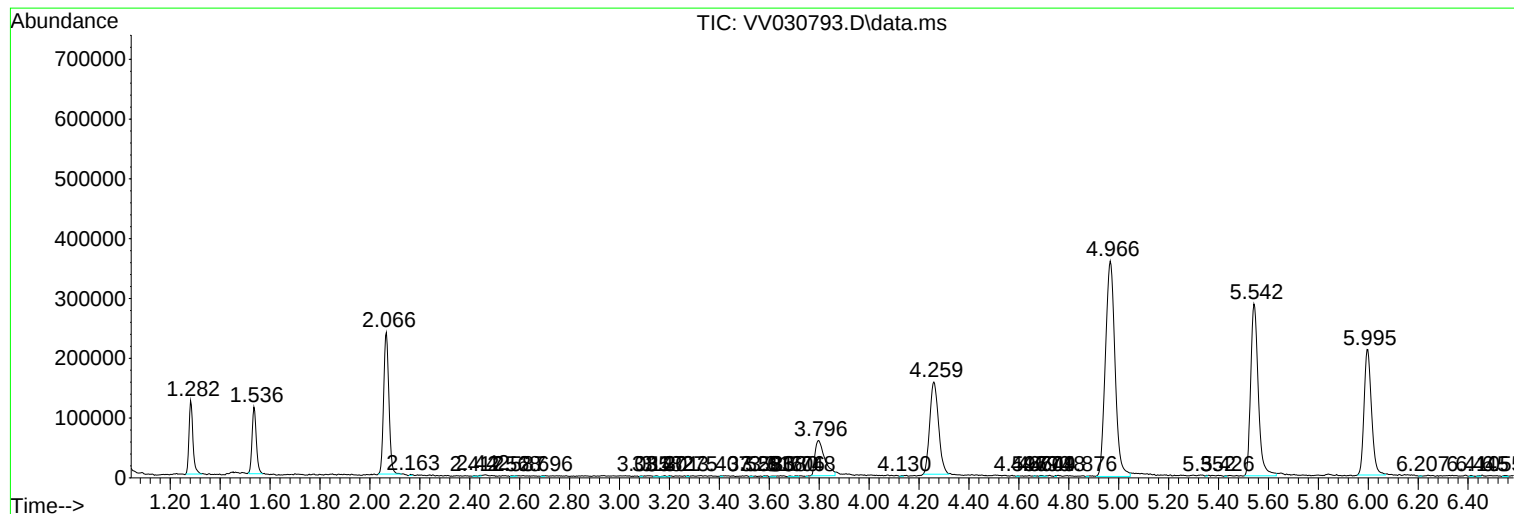

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
Data File : VV030793.D
Acq On : 24 Apr 2023 15:22
Operator : SY/MD
Sample : 02440-15 20X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMR0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
Data File : VV030793.D
Acq On : 24 Apr 2023 15:22
Operator : SY/MD
Sample : 02440-15 20X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMR0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------