

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
 Data File : VV030794.D
 Acq On : 24 Apr 2023 15:46
 Operator : SY/MD
 Sample : 02440-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMQ0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030794.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	86	rBV	81071	87922	2.43%	0.823%
2	1.535	148	154	167	rVB	88414	104838	2.90%	0.981%
3	2.066	310	319	331	rBV	169998	243438	6.73%	2.278%
4	2.555	468	471	472	rBV4	1522	825	0.02%	0.008%
5	2.770	535	538	540	rBV4	1014	662	0.02%	0.006%
6	2.783	540	542	545	rBV4	1046	617	0.02%	0.006%
7	2.883	569	573	577	rVB6	1790	1560	0.04%	0.015%
8	3.040	614	622	623	rBV6	1717	1662	0.05%	0.016%
9	3.072	629	632	634	rBV4	961	697	0.02%	0.007%
10	3.111	640	644	645	rBV4	1076	749	0.02%	0.007%
11	3.169	658	662	665	rBV5	1200	994	0.03%	0.009%
12	3.310	703	706	710	rVB6	1178	921	0.03%	0.009%
13	3.333	710	713	714	rBV3	1010	657	0.02%	0.006%
14	3.368	720	724	726	rBV5	1004	613	0.02%	0.006%
15	3.432	742	744	748	rVV5	1250	897	0.02%	0.008%
16	3.481	754	759	760	rVB5	976	711	0.02%	0.007%
17	3.503	760	766	770	rBV7	1621	1774	0.05%	0.017%
18	3.539	775	777	780	rVB4	1505	662	0.02%	0.006%
19	3.561	782	784	789	rBV6	1012	714	0.02%	0.007%
20	3.706	828	829	832	rBV3	963	647	0.02%	0.006%
21	3.735	836	838	847	rVB9	1172	983	0.03%	0.009%
22	3.802	847	859	884	rBV	54504	168013	4.65%	1.572%
23	4.259	987	1001	1025	rBV	122589	313381	8.67%	2.932%
24	4.561	1091	1095	1096	rBV4	1095	802	0.02%	0.008%
25	4.609	1107	1110	1112	rBV4	1395	877	0.02%	0.008%
26	4.629	1114	1116	1119	rVV3	1301	841	0.02%	0.008%
27	4.834	1177	1180	1182	rBV4	1380	844	0.02%	0.008%
28	4.860	1186	1188	1191	rVB3	1075	618	0.02%	0.006%
29	4.889	1191	1197	1199	rBV6	856	832	0.02%	0.008%
30	4.966	1206	1221	1234	rBV3	267943	711021	19.67%	6.653%
31	5.362	1340	1344	1347	rBV6	1897	1794	0.05%	0.017%
32	5.474	1375	1379	1381	rBV5	1026	651	0.02%	0.006%
33	5.542	1386	1400	1419	rBV2	294978	608840	16.84%	5.697%
34	5.998	1531	1542	1563	rVB	164172	330985	9.15%	3.097%
35	6.484	1690	1693	1695	rBV4	1368	702	0.02%	0.007%
36	6.574	1717	1721	1725	rBV5	1223	1256	0.03%	0.012%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
 Data File : VV030794.D
 Acq On : 24 Apr 2023 15:46
 Operator : SY/MD
 Sample : 02440-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMQ0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	6.625	1735	1737	1742	rVB5	2042	1170	0.03%	0.011%
38	6.731	1767	1770	1774	rBV6	1525	1339	0.04%	0.013%
39	6.825	1796	1799	1803	rBV6	2209	1643	0.05%	0.015%
40	6.921	1816	1829	1845	rBV	83910	158668	4.39%	1.485%
41	7.252	1921	1932	1953	rBV	298361	532565	14.73%	4.983%
42	7.497	2004	2008	2013	rBV7	1581	1476	0.04%	0.014%
43	7.561	2019	2028	2045	rBV	60501	108522	3.00%	1.015%
44	7.796	2096	2101	2104	rBV7	2077	1761	0.05%	0.016%
45	7.818	2105	2108	2110	rVV4	1323	713	0.02%	0.007%
46	7.937	2144	2145	2149	rVB4	1508	789	0.02%	0.007%
47	7.963	2149	2153	2155	rBV4	1529	1130	0.03%	0.011%
48	8.034	2166	2175	2209	rBV	167476	342718	9.48%	3.207%
49	8.432	2296	2299	2302	rBV4	1400	753	0.02%	0.007%
50	8.509	2321	2323	2327	rVB5	1195	714	0.02%	0.007%
51	8.641	2360	2364	2366	rBV4	1611	849	0.02%	0.008%
52	8.664	2370	2371	2375	rVB4	1219	758	0.02%	0.007%
53	8.689	2375	2379	2380	rBV4	952	743	0.02%	0.007%
54	8.821	2400	2420	2460	rBV2	1778073	3615500	100.00%	33.830%
55	9.355	2583	2586	2589	rBV5	1578	1176	0.03%	0.011%
56	9.400	2598	2600	2602	rBV3	1298	700	0.02%	0.007%
57	9.487	2625	2627	2631	rVB4	1367	977	0.03%	0.009%
58	9.609	2663	2665	2669	rVB5	1658	831	0.02%	0.008%
59	9.644	2672	2676	2680	rBV6	1577	1383	0.04%	0.013%
60	9.824	2730	2732	2737	rBV6	1035	966	0.03%	0.009%
61	9.882	2748	2750	2752	rBV3	1497	682	0.02%	0.006%
62	9.960	2771	2774	2780	rVB6	1889	1696	0.05%	0.016%
63	10.001	2783	2787	2788	rBV3	1350	887	0.02%	0.008%
64	10.159	2824	2836	2857	rBV	239616	392933	10.87%	3.677%
65	10.371	2900	2902	2905	rBV2	1485	875	0.02%	0.008%
66	10.458	2926	2929	2930	rBV3	1415	775	0.02%	0.007%
67	10.532	2948	2952	2954	rBV5	1621	1055	0.03%	0.010%
68	10.606	2971	2975	2979	rBV7	1299	1497	0.04%	0.014%
69	10.648	2983	2988	2991	rBV6	1634	1581	0.04%	0.015%
70	10.696	3000	3003	3006	rBV4	1693	1207	0.03%	0.011%
71	10.741	3014	3017	3021	rVB5	1739	1279	0.04%	0.012%
72	10.760	3021	3023	3025	rBV2	1905	928	0.03%	0.009%
73	10.815	3037	3040	3044	rVB7	1398	896	0.02%	0.008%
74	10.837	3044	3047	3048	rBV3	1987	911	0.03%	0.009%
75	10.876	3057	3059	3062	rBV4	1014	745	0.02%	0.007%
76	11.127	3128	3137	3147	rBV	78840	122049	3.38%	1.142%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
 Data File : VV030794.D
 Acq On : 24 Apr 2023 15:46
 Operator : SY/MD
 Sample : 02440-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMQ0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	11.194	3148	3158	3162	rBV	497355	780602	21.59%	7.304%
78	11.413	3223	3226	3229	rBV4	1372	875	0.02%	0.008%
79	11.586	3264	3280	3298	rBV2	807354	1695624	46.90%	15.866%
80	11.747	3326	3330	3331	rBV4	1525	1002	0.03%	0.009%
81	12.210	3471	3474	3478	rVB5	1142	792	0.02%	0.007%
82	12.342	3509	3515	3527	rBV5	4207	7381	0.20%	0.069%
83	12.657	3611	3613	3614	rBV2	1541	779	0.02%	0.007%
84	12.696	3618	3625	3630	rVV8	2723	3982	0.11%	0.037%
85	12.770	3643	3648	3650	rVB6	770	698	0.02%	0.007%
86	12.837	3665	3669	3670	rBV4	1084	847	0.02%	0.008%
87	13.033	3725	3730	3732	rBV5	1395	1229	0.03%	0.011%
88	13.207	3771	3784	3796	rBV	136379	213279	5.90%	1.996%
89	13.615	3909	3911	3916	rVB5	1896	1715	0.05%	0.016%
90	13.638	3916	3918	3920	rBV2	1146	624	0.02%	0.006%
91	13.689	3924	3934	3946	rVV	38689	62514	1.73%	0.585%
92	13.847	3980	3983	3986	rBV4	1508	963	0.03%	0.009%
93	13.879	3990	3993	3998	rBV7	2018	1780	0.05%	0.017%
94	14.053	4045	4047	4049	rBV3	1532	843	0.02%	0.008%
95	14.136	4071	4073	4075	rVB3	1699	657	0.02%	0.006%
96	14.271	4111	4115	4117	rBV4	1404	1173	0.03%	0.011%
97	14.635	4226	4228	4231	rBV4	1217	720	0.02%	0.007%
98	14.712	4250	4252	4255	rBV2	1596	1095	0.03%	0.010%
99	14.744	4255	4262	4266	rBV8	4190	5322	0.15%	0.050%
100	15.085	4366	4368	4371	rBV4	1483	979	0.03%	0.009%




Sum of corrected areas: 10687315

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
Data File : VV030794.D
Acq On : 24 Apr 2023 15:46
Operator : SY/MD
Sample : 02440-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMQ0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

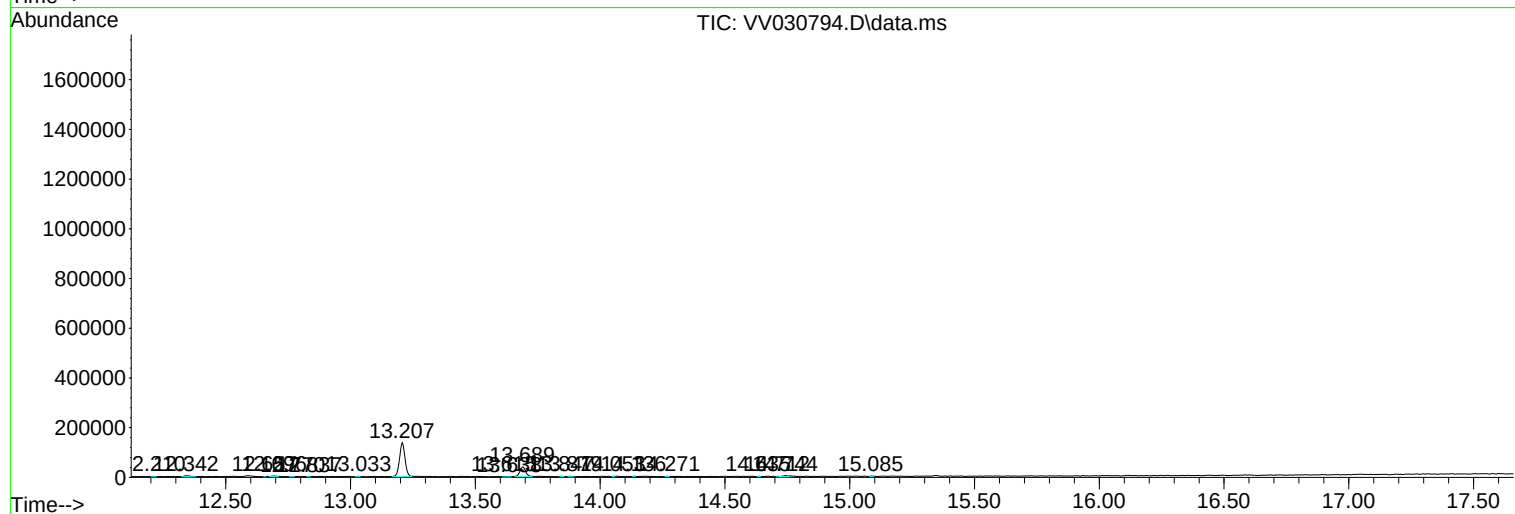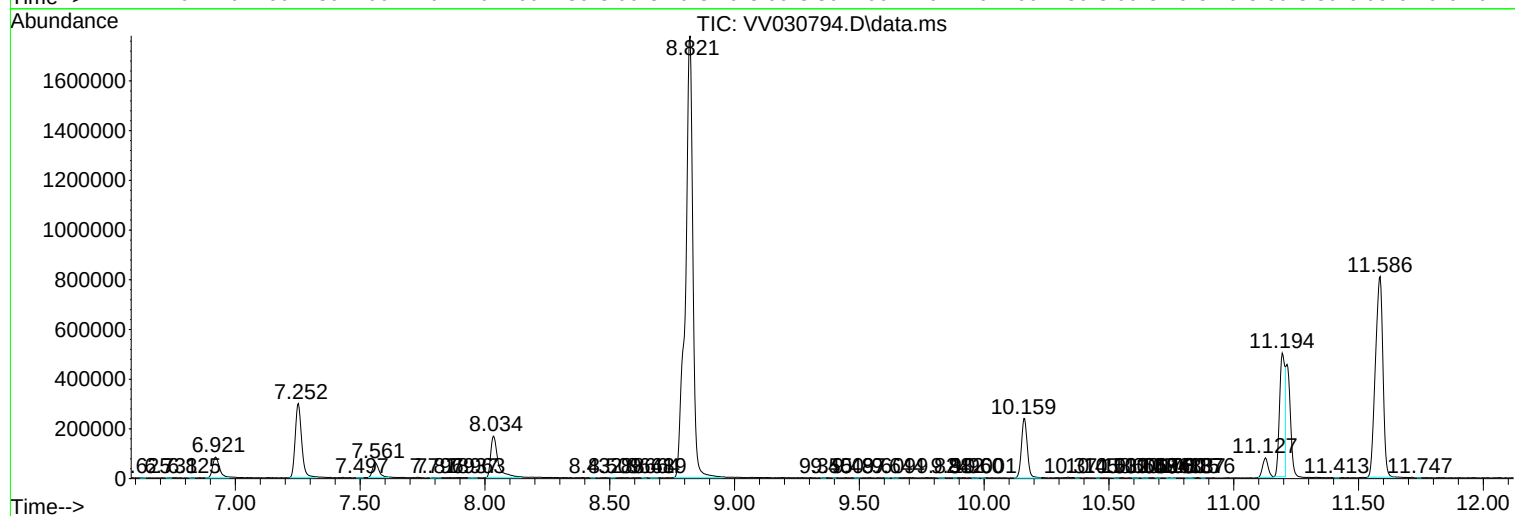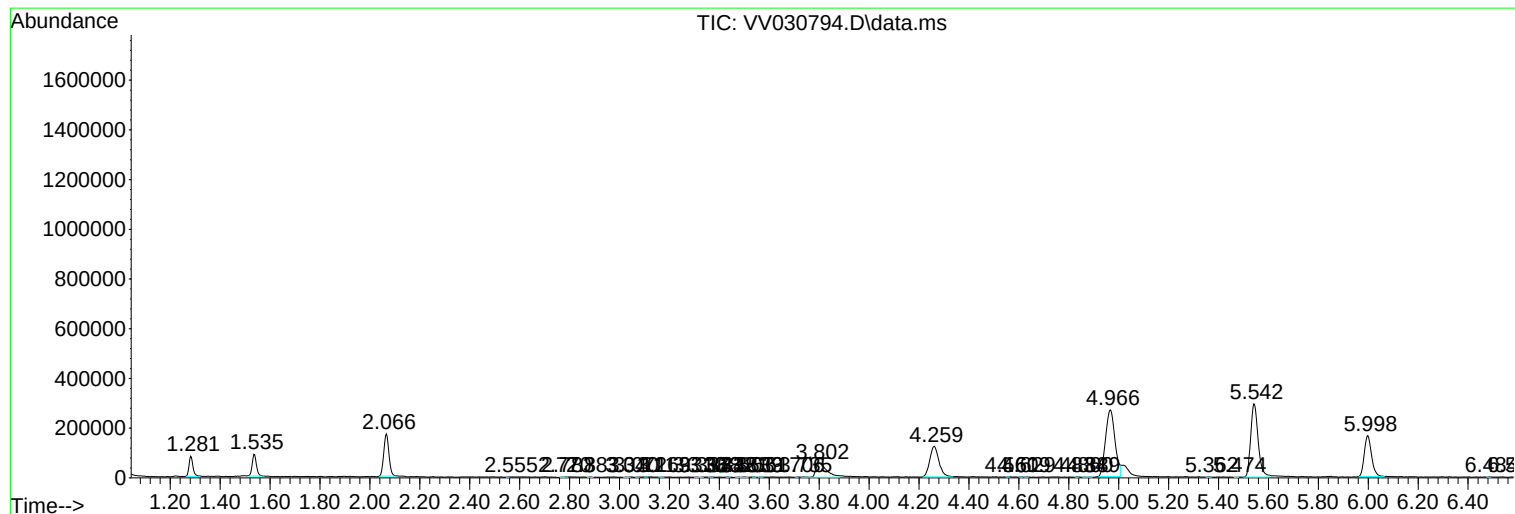

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
Data File : VV030794.D
Acq On : 24 Apr 2023 15:46
Operator : SY/MD
Sample : 02440-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMQ0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
Data File : VV030794.D
Acq On : 24 Apr 2023 15:46
Operator : SY/MD
Sample : 02440-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0MQ0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc