

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
 Data File : VV030796.D
 Acq On : 24 Apr 2023 16:34
 Operator : SY/MD
 Sample : 02440-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMR1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030796.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	86	rBV	86398	91358	12.51%	1.524%
2	1.539	148	155	168	rVB	84061	106958	14.64%	1.784%
3	2.066	310	319	336	rVB	174328	253540	34.71%	4.230%
4	2.494	450	452	455	rBV3	1140	881	0.12%	0.015%
5	2.551	466	470	473	rBV6	1764	1391	0.19%	0.023%
6	2.703	515	517	523	rVB7	1331	857	0.12%	0.014%
7	2.780	536	541	545	rBV6	1701	1966	0.27%	0.033%
8	2.815	550	552	553	rBV2	1276	526	0.07%	0.009%
9	2.912	576	582	584	rBV6	1851	1797	0.25%	0.030%
10	3.018	613	615	619	rVB3	1224	825	0.11%	0.014%
11	3.066	628	630	631	rBV2	1497	449	0.06%	0.007%
12	3.236	678	683	684	rBV5	1295	1101	0.15%	0.018%
13	3.333	711	713	716	rBV4	1494	899	0.12%	0.015%
14	3.400	732	734	737	rVB3	1041	469	0.06%	0.008%
15	3.416	737	739	741	rBV3	1446	733	0.10%	0.012%
16	3.442	745	747	751	rVB3	855	455	0.06%	0.008%
17	3.465	751	754	755	rBV3	801	480	0.07%	0.008%
18	3.516	768	770	772	rBV3	966	635	0.09%	0.011%
19	3.619	798	802	804	rBV4	1524	1220	0.17%	0.020%
20	3.696	820	826	827	rBV5	1192	1254	0.17%	0.021%
21	3.725	834	835	838	rBV2	985	559	0.08%	0.009%
22	3.802	850	859	890	rBV2	48373	140872	19.29%	2.350%
23	4.259	990	1001	1023	rVB	119872	300260	41.11%	5.009%
24	4.606	1105	1109	1110	rBV4	1539	1187	0.16%	0.020%
25	4.670	1124	1129	1131	rBV6	1134	1146	0.16%	0.019%
26	4.757	1152	1156	1160	rBV6	1278	1468	0.20%	0.024%
27	4.828	1173	1178	1179	rBV5	1260	962	0.13%	0.016%
28	4.892	1194	1198	1199	rBV4	817	508	0.07%	0.008%
29	4.966	1202	1221	1244	rBV2	271418	730414	100.00%	12.186%
30	5.185	1288	1289	1291	rBV2	1100	505	0.07%	0.008%
31	5.368	1344	1346	1348	rBV3	1417	886	0.12%	0.015%
32	5.542	1389	1400	1428	rBV	270606	560267	76.71%	9.347%
33	5.953	1525	1528	1529	rBV3	1346	775	0.11%	0.013%
34	5.998	1530	1542	1561	rVV2	161970	334929	45.85%	5.588%
35	6.246	1616	1619	1620	rBV3	1304	725	0.10%	0.012%
36	6.484	1691	1693	1698	rVB6	1735	965	0.13%	0.016%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042423\
 Data File : VW030796.D
 Acq On : 24 Apr 2023 16:34
 Operator : SY/MD
 Sample : 02440-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMR1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	6.506	1698	1700	1701	rBV2	1779	840	0.12%	0.014%
38	6.644	1741	1743	1747	rBV5	1207	805	0.11%	0.013%
39	6.831	1798	1801	1802	rBV3	1030	663	0.09%	0.011%
40	6.921	1819	1829	1847	rBV	84435	155291	21.26%	2.591%
41	7.101	1882	1885	1886	rBV3	1440	800	0.11%	0.013%
42	7.252	1920	1932	1959	rBV	297404	540798	74.04%	9.022%
43	7.561	2018	2028	2045	rBV	60169	113855	15.59%	1.899%
44	7.818	2106	2108	2111	rBV4	1050	522	0.07%	0.009%
45	7.841	2113	2115	2120	rVB6	1370	889	0.12%	0.015%
46	7.963	2151	2153	2156	rVV4	1228	598	0.08%	0.010%
47	8.037	2167	2176	2209	rBV	160961	333960	45.72%	5.572%
48	8.487	2314	2316	2323	rVB7	1981	1752	0.24%	0.029%
49	8.519	2323	2326	2328	rBV4	1908	1148	0.16%	0.019%
50	8.657	2367	2369	2371	rBV2	1102	493	0.07%	0.008%
51	8.792	2399	2411	2433	rBV	423185	714466	97.82%	11.920%
52	9.159	2522	2525	2526	rBV3	1810	1226	0.17%	0.020%
53	9.352	2582	2585	2586	rBV4	1042	493	0.07%	0.008%
54	9.403	2595	2601	2602	rBV5	2238	1732	0.24%	0.029%
55	9.480	2623	2625	2628	rBV4	1764	1209	0.17%	0.020%
56	9.615	2664	2667	2668	rBV3	1436	918	0.13%	0.015%
57	9.657	2678	2680	2683	rBV4	1611	1158	0.16%	0.019%
58	9.705	2692	2695	2699	rBV4	1833	1345	0.18%	0.022%
59	9.860	2736	2743	2748	rBV9	1502	2198	0.30%	0.037%
60	9.898	2752	2755	2757	rBV3	1214	916	0.13%	0.015%
61	10.011	2787	2790	2792	rBV3	1370	1056	0.14%	0.018%
62	10.059	2804	2805	2807	rBV2	884	454	0.06%	0.008%
63	10.085	2811	2813	2815	rBV3	884	536	0.07%	0.009%
64	10.162	2826	2837	2855	rBV	232755	372729	51.03%	6.218%
65	10.281	2872	2874	2877	rVB4	1432	664	0.09%	0.011%
66	10.316	2883	2885	2888	rBV3	2117	1483	0.20%	0.025%
67	10.512	2943	2946	2949	rBV4	985	668	0.09%	0.011%
68	10.857	3049	3053	3057	rBV6	2068	1696	0.23%	0.028%
69	10.876	3057	3059	3061	rBV3	909	522	0.07%	0.009%
70	10.934	3075	3077	3079	rBV2	1778	1133	0.16%	0.019%
71	10.969	3087	3088	3091	rBV3	845	604	0.08%	0.010%
72	10.995	3093	3096	3100	rVB7	1785	1107	0.15%	0.018%
73	11.194	3145	3158	3176	rBV	395769	638563	87.42%	10.653%
74	11.451	3236	3238	3243	rVV6	919	767	0.11%	0.013%
75	11.500	3250	3253	3255	rBV3	1643	1093	0.15%	0.018%
76	11.570	3264	3275	3290	rBV	323188	527410	72.21%	8.799%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
 Data File : VV030796.D
 Acq On : 24 Apr 2023 16:34
 Operator : SY/MD
 Sample : 02440-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMR1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	11.776	3336	3339	3340	rBV3	916	539	0.07%	0.009%
78	11.808	3346	3349	3350	rBV2	1817	885	0.12%	0.015%
79	12.011	3410	3412	3415	rBV4	1069	556	0.08%	0.009%
80	12.127	3446	3448	3450	rBV3	1480	720	0.10%	0.012%
81	12.165	3457	3460	3461	rBV2	1153	600	0.08%	0.010%
82	12.400	3530	3533	3535	rBV3	956	607	0.08%	0.010%
83	12.435	3541	3544	3549	rBV6	1626	1167	0.16%	0.019%
84	12.487	3555	3560	3561	rBV3	869	649	0.09%	0.011%
85	12.548	3576	3579	3581	rBV4	1152	803	0.11%	0.013%
86	12.770	3645	3648	3650	rVV4	1912	1250	0.17%	0.021%
87	12.792	3653	3655	3661	rVB6	1103	925	0.13%	0.015%
88	13.065	3738	3740	3743	rBV4	1586	1088	0.15%	0.018%
89	13.397	3841	3843	3845	rBV3	1284	809	0.11%	0.013%
90	13.442	3856	3857	3860	rBV3	1177	786	0.11%	0.013%
91	13.516	3878	3880	3882	rBV2	1600	942	0.13%	0.016%
92	13.590	3902	3903	3905	rVB2	1751	548	0.08%	0.009%
93	13.622	3910	3913	3914	rBV3	990	560	0.08%	0.009%
94	13.638	3914	3918	3921	rBV6	1370	943	0.13%	0.016%
95	13.934	4007	4010	4014	rBV6	1349	1442	0.20%	0.024%
96	13.979	4021	4024	4026	rBV4	1939	1119	0.15%	0.019%
97	14.400	4153	4155	4156	rBV2	1337	602	0.08%	0.010%
98	14.699	4245	4248	4253	rBV6	1580	1639	0.22%	0.027%
99	14.757	4263	4266	4270	rVB6	1655	1033	0.14%	0.017%
100	14.776	4270	4272	4274	rBV3	1718	974	0.13%	0.016%




Sum of corrected areas: 5993968

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
Data File : VV030796.D
Acq On : 24 Apr 2023 16:34
Operator : SY/MD
Sample : 02440-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMR1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

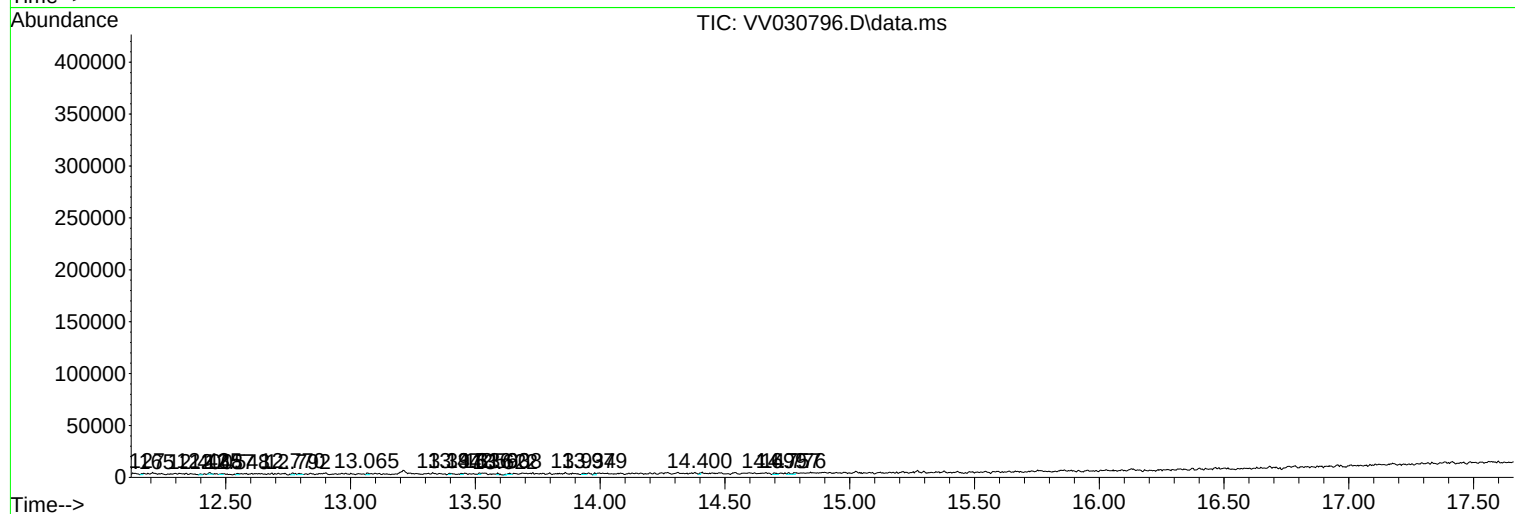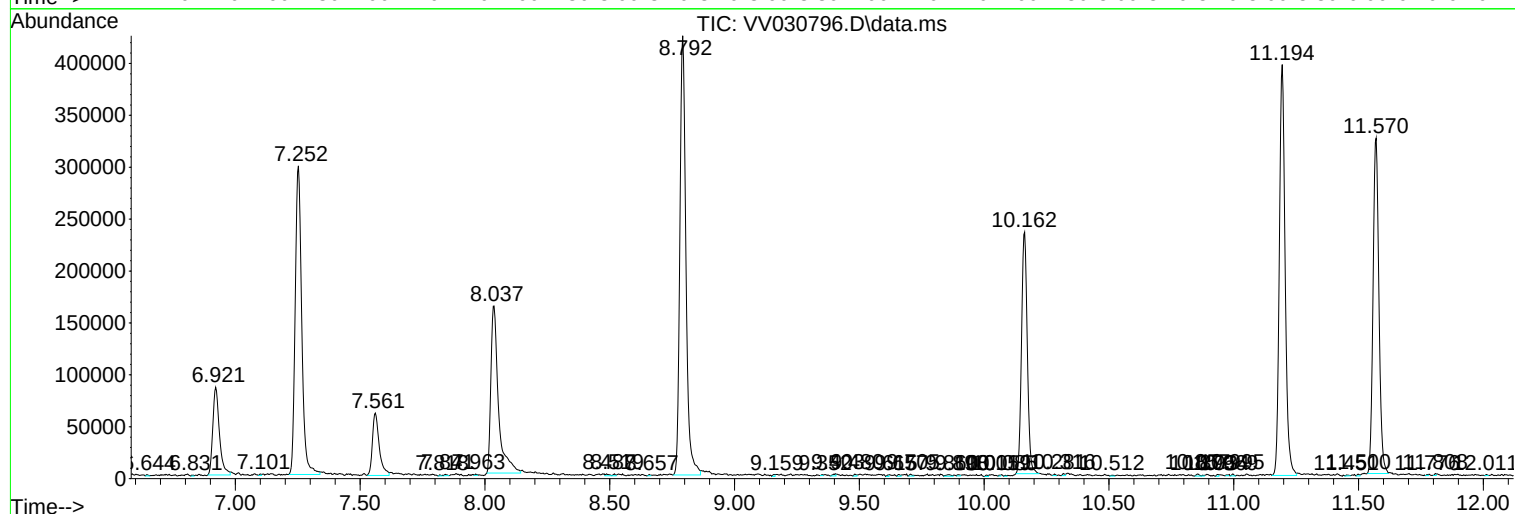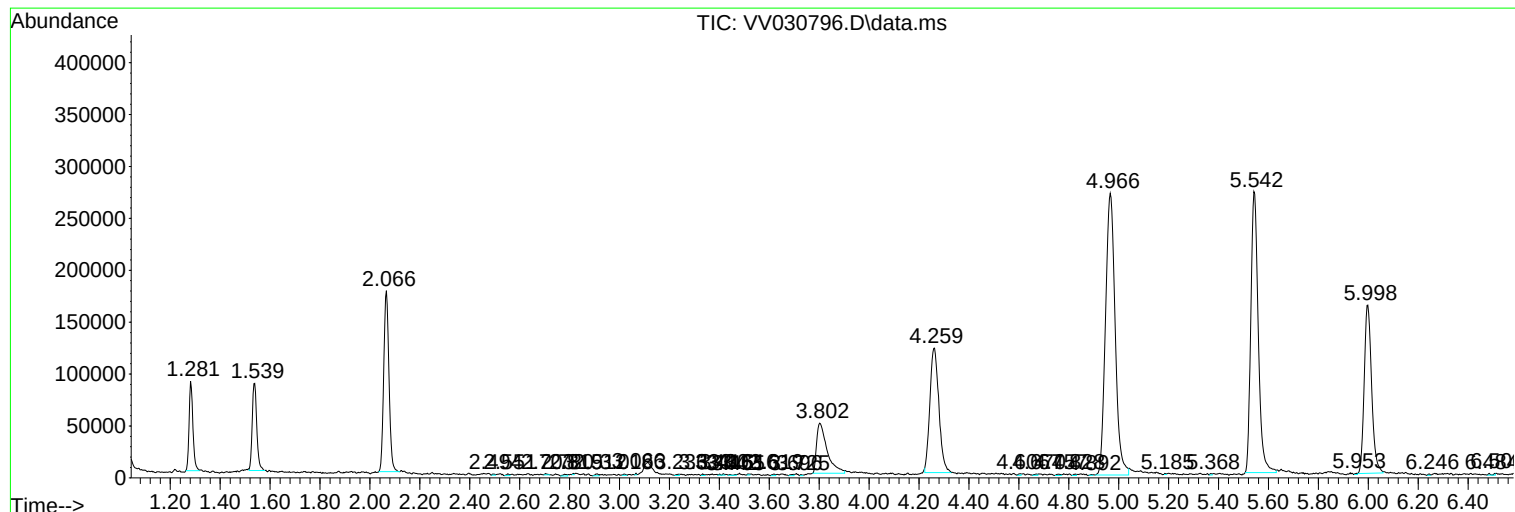

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
Data File : VV030796.D
Acq On : 24 Apr 2023 16:34
Operator : SY/MD
Sample : 02440-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMR1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
Data File : VV030796.D
Acq On : 24 Apr 2023 16:34
Operator : SY/MD
Sample : 02440-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMR1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc