

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
 Data File : VV030797.D
 Acq On : 24 Apr 2023 16:58
 Operator : SY/MD
 Sample : 02440-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMR2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030797.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	90	rVB	80326	91951	11.86%	1.512%
2	1.539	148	155	167	rBV	82050	98127	12.66%	1.613%
3	2.066	310	319	334	rBV	173663	249812	32.22%	4.107%
4	2.243	372	374	375	rBV2	1533	645	0.08%	0.011%
5	2.413	422	427	433	rBV9	1576	2382	0.31%	0.039%
6	2.523	457	461	468	rBV8	1485	1677	0.22%	0.028%
7	2.564	472	474	479	rVB5	1575	963	0.12%	0.016%
8	2.899	575	578	581	rBV3	1181	570	0.07%	0.009%
9	3.011	612	613	615	rBV2	1183	593	0.08%	0.010%
10	3.185	664	667	670	rBV5	1494	1274	0.16%	0.021%
11	3.201	670	672	675	rVB4	1308	759	0.10%	0.012%
12	3.217	675	677	680	rVB5	1501	792	0.10%	0.013%
13	3.243	680	685	686	rBV4	1371	1113	0.14%	0.018%
14	3.291	698	700	701	rBV	1435	531	0.07%	0.009%
15	3.413	734	738	743	rVB7	1600	1310	0.17%	0.022%
16	3.449	747	749	754	rBV6	1127	930	0.12%	0.015%
17	3.751	840	843	846	rBV5	1410	1163	0.15%	0.019%
18	3.805	851	860	880	rBV	48804	137153	17.69%	2.255%
19	4.066	938	941	942	rBV2	1775	849	0.11%	0.014%
20	4.182	975	977	979	rBV3	1473	742	0.10%	0.012%
21	4.262	988	1002	1021	rBV	119035	303091	39.09%	4.983%
22	4.477	1067	1069	1072	rBV3	1326	666	0.09%	0.011%
23	4.522	1081	1083	1086	rBV4	1446	831	0.11%	0.014%
24	4.564	1093	1096	1099	rBV4	1659	1402	0.18%	0.023%
25	4.661	1124	1126	1131	rVB4	1769	1237	0.16%	0.020%
26	4.686	1132	1134	1139	rVB6	1411	883	0.11%	0.015%
27	4.712	1139	1142	1147	rBV6	1642	1611	0.21%	0.026%
28	4.741	1147	1151	1152	rBV3	871	672	0.09%	0.011%
29	4.793	1165	1167	1171	rVV4	2059	1488	0.19%	0.024%
30	4.966	1205	1221	1249	rVV2	272381	775401	100.00%	12.747%
31	5.220	1298	1300	1306	rVB7	2511	1825	0.24%	0.030%
32	5.252	1306	1310	1312	rBV6	1159	973	0.13%	0.016%
33	5.394	1351	1354	1355	rBV2	1710	800	0.10%	0.013%
34	5.542	1389	1400	1425	rBV	274198	567514	73.19%	9.329%
35	5.921	1516	1518	1523	rVB4	1687	1070	0.14%	0.018%
36	5.998	1530	1542	1566	rVB	160766	331821	42.79%	5.455%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
 Data File : VV030797.D
 Acq On : 24 Apr 2023 16:58
 Operator : SY/MD
 Sample : 02440-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMR2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	6.297	1633	1635	1638	rVB4	1961	988	0.13%	0.016%
38	6.317	1638	1641	1642	rBV4	882	586	0.08%	0.010%
39	6.368	1656	1657	1661	rVB4	1200	567	0.07%	0.009%
40	6.442	1678	1680	1683	rBV4	1006	681	0.09%	0.011%
41	6.538	1706	1710	1713	rBV5	1287	978	0.13%	0.016%
42	6.616	1732	1734	1740	rBV6	1366	1080	0.14%	0.018%
43	6.686	1754	1756	1759	rBV4	1421	1006	0.13%	0.017%
44	6.834	1799	1802	1805	rBV4	1155	957	0.12%	0.016%
45	6.921	1818	1829	1850	rBV	81594	160495	20.70%	2.638%
46	7.198	1913	1915	1918	rBV4	1300	705	0.09%	0.012%
47	7.252	1920	1932	1951	rBV	299605	534501	68.93%	8.787%
48	7.513	2010	2013	2015	rBV4	1170	882	0.11%	0.014%
49	7.561	2020	2028	2040	rVV	57109	98029	12.64%	1.612%
50	7.783	2094	2097	2100	rBV3	1773	1170	0.15%	0.019%
51	7.876	2124	2126	2128	rBV3	1493	632	0.08%	0.010%
52	8.034	2163	2175	2209	rBV	153802	345893	44.61%	5.686%
53	8.452	2302	2305	2309	rBV6	1116	1001	0.13%	0.016%
54	8.619	2351	2357	2358	rBV5	1618	1378	0.18%	0.023%
55	8.702	2380	2383	2384	rBV2	1467	639	0.08%	0.011%
56	8.792	2396	2411	2437	rBV	426200	739113	95.32%	12.150%
57	9.233	2544	2548	2549	rBV4	1175	876	0.11%	0.014%
58	9.304	2567	2570	2572	rBV3	1403	629	0.08%	0.010%
59	9.413	2601	2604	2606	rBV3	1146	724	0.09%	0.012%
60	9.480	2621	2625	2626	rBV3	936	627	0.08%	0.010%
61	9.538	2641	2643	2644	rBV2	1404	528	0.07%	0.009%
62	9.673	2682	2685	2688	rBV6	1230	964	0.12%	0.016%
63	9.731	2700	2703	2704	rBV3	1239	784	0.10%	0.013%
64	9.857	2739	2742	2743	rBV3	990	619	0.08%	0.010%
65	9.924	2760	2763	2764	rVB3	1595	641	0.08%	0.011%
66	9.992	2781	2784	2785	rBV2	989	510	0.07%	0.008%
67	10.162	2826	2837	2860	rVB	235340	381422	49.19%	6.270%
68	10.246	2860	2863	2869	rBV6	1235	1448	0.19%	0.024%
69	10.416	2913	2916	2917	rBV2	1008	573	0.07%	0.009%
70	10.738	3012	3016	3020	rBV6	1416	1550	0.20%	0.025%
71	10.773	3025	3027	3029	rBV2	798	531	0.07%	0.009%
72	10.869	3053	3057	3058	rBV4	1118	756	0.10%	0.012%
73	10.879	3058	3060	3063	rVV3	1309	666	0.09%	0.011%
74	11.014	3099	3102	3104	rBV3	1283	702	0.09%	0.012%
75	11.050	3111	3113	3117	rBV5	1053	550	0.07%	0.009%
76	11.194	3147	3158	3180	rBV	405470	655974	84.60%	10.784%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
 Data File : VV030797.D
 Acq On : 24 Apr 2023 16:58
 Operator : SY/MD
 Sample : 02440-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMR2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	11.455	3237	3239	3243	rVB4	1354	789	0.10%	0.013%
78	11.490	3247	3250	3252	rBV3	1958	1175	0.15%	0.019%
79	11.570	3264	3275	3296	rVB	326851	532697	68.70%	8.757%
80	11.818	3349	3352	3354	rBV4	1753	955	0.12%	0.016%
81	12.226	3476	3479	3481	rBV4	756	579	0.07%	0.010%
82	12.323	3507	3509	3511	rVB3	1503	675	0.09%	0.011%
83	12.493	3556	3562	3566	rBV8	1045	1290	0.17%	0.021%
84	12.693	3621	3624	3627	rVB5	1386	903	0.12%	0.015%
85	12.712	3627	3630	3632	rBV4	1437	784	0.10%	0.013%
86	12.808	3658	3660	3665	rVB6	1048	584	0.08%	0.010%
87	12.937	3695	3700	3704	rBV6	1280	1106	0.14%	0.018%
88	12.966	3707	3709	3714	rVB5	1810	1374	0.18%	0.023%
89	12.998	3716	3719	3723	rVB6	1745	1021	0.13%	0.017%
90	13.014	3723	3724	3726	rBV2	1227	611	0.08%	0.010%
91	13.117	3750	3756	3758	rBV6	1182	1081	0.14%	0.018%
92	13.136	3758	3762	3765	rBV5	1116	864	0.11%	0.014%
93	13.352	3827	3829	3836	rVV5	1503	1356	0.17%	0.022%
94	13.384	3836	3839	3843	rVB6	1605	1116	0.14%	0.018%
95	13.850	3981	3984	3987	rBV5	1191	1054	0.14%	0.017%
96	13.947	4011	4014	4017	rBV3	1855	1120	0.14%	0.018%
97	14.082	4052	4056	4058	rBV5	1350	1023	0.13%	0.017%
98	14.387	4147	4151	4153	rBV5	1431	1161	0.15%	0.019%
99	14.509	4186	4189	4194	rBV6	1166	1387	0.18%	0.023%
100	14.934	4317	4321	4322	rBV4	2007	1395	0.18%	0.023%




Sum of corrected areas: 6083076

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
Data File : VV030797.D
Acq On : 24 Apr 2023 16:58
Operator : SY/MD
Sample : 02440-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMR2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

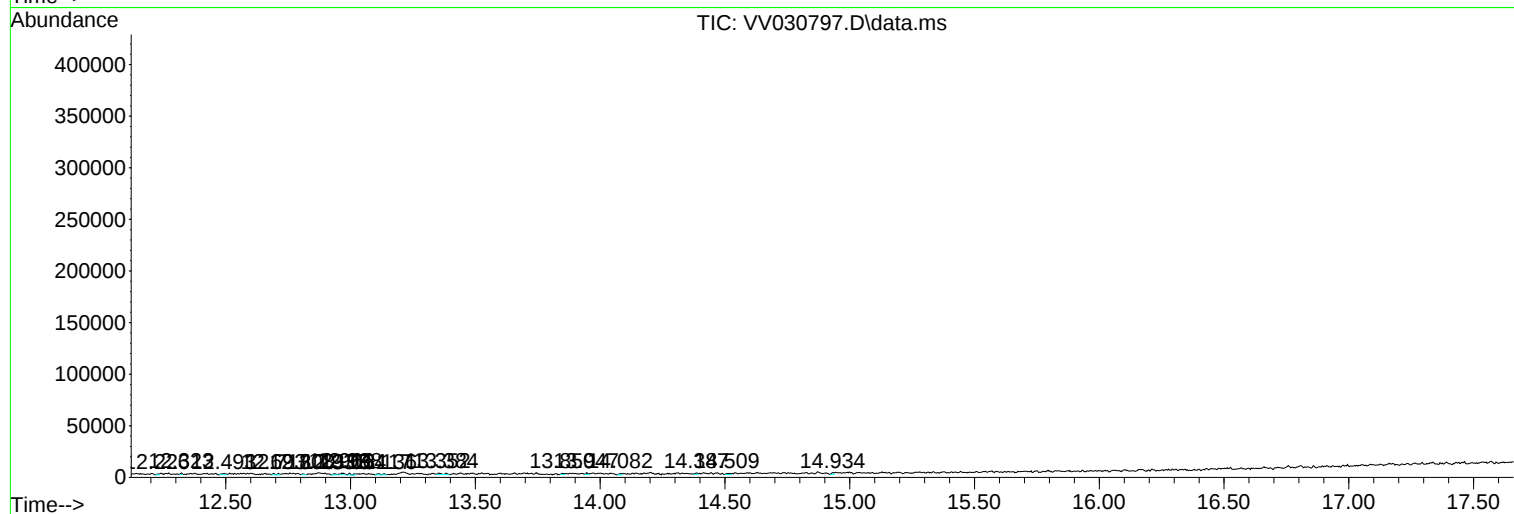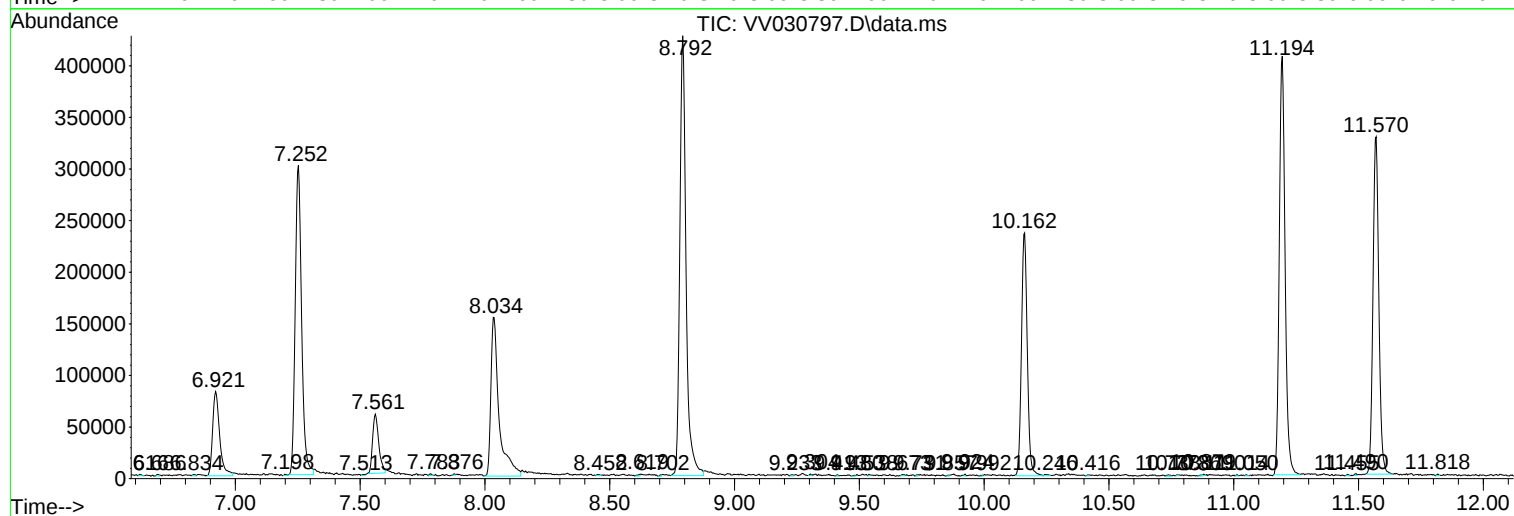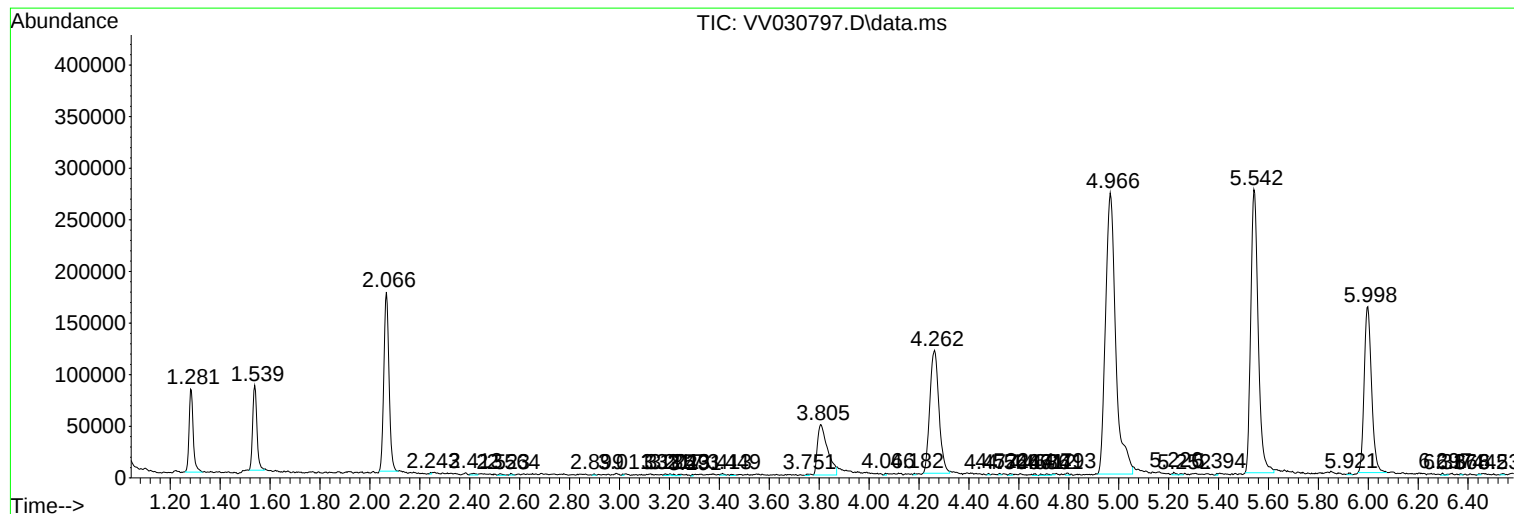

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
Data File : VV030797.D
Acq On : 24 Apr 2023 16:58
Operator : SY/MD
Sample : 02440-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMR2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
Data File : VV030797.D
Acq On : 24 Apr 2023 16:58
Operator : SY/MD
Sample : 02440-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMR2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------