

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
 Data File : VV030798.D
 Acq On : 24 Apr 2023 17:22
 Operator : SY/MD
 Sample : 02440-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMR3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030798.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.285	70	76	93	rVB	86647	95121	12.87%	1.535%
2	1.539	148	155	168	rVB	89378	104175	14.09%	1.681%
3	2.066	310	319	336	rVB	174336	255463	34.55%	4.121%
4	2.394	418	421	423	rBV3	1050	785	0.11%	0.013%
5	2.793	542	545	546	rBV3	1588	840	0.11%	0.014%
6	2.831	551	557	558	rBV6	1105	913	0.12%	0.015%
7	2.870	562	569	570	rBV6	1218	1336	0.18%	0.022%
8	2.966	596	599	600	rBV3	1507	806	0.11%	0.013%
9	3.047	622	624	628	rVB5	1585	957	0.13%	0.015%
10	3.140	650	653	656	rBV5	1391	1183	0.16%	0.019%
11	3.195	667	670	671	rBV4	1215	833	0.11%	0.013%
12	3.477	756	758	761	rBV3	1370	921	0.12%	0.015%
13	3.805	849	860	888	rBV2	47152	150803	20.40%	2.433%
14	4.162	966	971	975	rBV9	1466	1549	0.21%	0.025%
15	4.262	983	1002	1024	rBV	123984	323737	43.79%	5.223%
16	4.577	1098	1100	1104	rBV4	1292	807	0.11%	0.013%
17	4.609	1104	1110	1114	rBV7	1403	1217	0.16%	0.020%
18	4.690	1131	1135	1140	rBV6	1062	1308	0.18%	0.021%
19	4.838	1177	1181	1186	rVB6	1828	1786	0.24%	0.029%
20	4.870	1186	1191	1193	rBV5	1390	989	0.13%	0.016%
21	4.883	1193	1195	1197	rBV2	1382	737	0.10%	0.012%
22	4.899	1197	1200	1203	rBV5	1050	834	0.11%	0.013%
23	4.966	1205	1221	1246	rBV2	275552	739378	100.00%	11.929%
24	5.542	1388	1400	1423	rBV	280946	588393	79.58%	9.493%
25	5.789	1474	1477	1478	rBV2	1517	743	0.10%	0.012%
26	5.998	1529	1542	1561	rBV3	164318	344528	46.60%	5.558%
27	6.342	1647	1649	1654	rVB5	1290	1018	0.14%	0.016%
28	6.645	1740	1743	1746	rBV5	1430	986	0.13%	0.016%
29	6.805	1791	1793	1797	rVB4	1627	834	0.11%	0.013%
30	6.870	1809	1813	1817	rBV7	2203	1663	0.22%	0.027%
31	6.918	1819	1828	1843	rBV	82703	155262	21.00%	2.505%
32	7.252	1920	1932	1953	rBV	306230	550169	74.41%	8.876%
33	7.561	2020	2028	2046	rBV	59837	103744	14.03%	1.674%
34	7.808	2103	2105	2108	rVV4	1338	746	0.10%	0.012%
35	7.937	2141	2145	2150	rBV7	1253	1337	0.18%	0.022%
36	8.037	2163	2176	2202	rBV	157913	348308	47.11%	5.619%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
 Data File : VV030798.D
 Acq On : 24 Apr 2023 17:22
 Operator : SY/MD
 Sample : 02440-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMR3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	8.725	2388	2390	2394	rBV5	1349	1007	0.14%	0.016%
38	8.792	2399	2411	2432	rBV	435986	735078	99.42%	11.859%
39	8.998	2472	2475	2477	rBV4	1557	1248	0.17%	0.020%
40	9.101	2503	2507	2510	rBV6	1003	895	0.12%	0.014%
41	9.162	2524	2526	2528	rVV3	1544	836	0.11%	0.013%
42	9.188	2532	2534	2539	rVV7	1233	972	0.13%	0.016%
43	9.210	2539	2541	2545	rVB6	1618	831	0.11%	0.013%
44	9.262	2553	2557	2558	rBV3	1637	1011	0.14%	0.016%
45	9.307	2569	2571	2575	rVB5	1691	1077	0.15%	0.017%
46	9.333	2575	2579	2581	rBV3	1928	1403	0.19%	0.023%
47	9.461	2617	2619	2621	rBV3	1015	707	0.10%	0.011%
48	9.484	2624	2626	2630	rVV5	1172	934	0.13%	0.015%
49	9.509	2632	2634	2637	rVB4	1431	740	0.10%	0.012%
50	9.609	2663	2665	2668	rBV3	1133	849	0.11%	0.014%
51	9.641	2673	2675	2679	rVB5	1160	765	0.10%	0.012%
52	9.667	2679	2683	2685	rBV5	1538	1259	0.17%	0.020%
53	9.706	2693	2695	2699	rVB5	1244	703	0.10%	0.011%
54	9.763	2710	2713	2716	rBV5	1009	767	0.10%	0.012%
55	9.898	2753	2755	2761	rVB7	1292	986	0.13%	0.016%
56	9.927	2761	2764	2767	rBV5	1364	1146	0.15%	0.018%
57	10.030	2794	2796	2801	rBV6	968	720	0.10%	0.012%
58	10.159	2825	2836	2857	rBV	247494	395876	53.54%	6.387%
59	10.387	2903	2907	2910	rBV6	885	707	0.10%	0.011%
60	10.522	2946	2949	2952	rBV5	1154	1056	0.14%	0.017%
61	10.561	2957	2961	2965	rBV7	1219	1475	0.20%	0.024%
62	10.628	2980	2982	2985	rBV4	1430	895	0.12%	0.014%
63	10.677	2993	2997	2999	rBV4	1805	1456	0.20%	0.023%
64	11.120	3133	3135	3138	rBV4	1239	774	0.10%	0.012%
65	11.140	3138	3141	3144	rVB4	1841	1296	0.18%	0.021%
66	11.194	3144	3158	3178	rBV	420556	673001	91.02%	10.858%
67	11.490	3244	3250	3252	rBV6	1755	1639	0.22%	0.026%
68	11.570	3260	3275	3291	rBV	328516	547626	74.07%	8.835%
69	11.812	3347	3350	3352	rVB4	1458	967	0.13%	0.016%
70	11.824	3352	3354	3356	rBV3	1152	749	0.10%	0.012%
71	11.940	3387	3390	3392	rBV3	1054	753	0.10%	0.012%
72	12.078	3430	3433	3437	rVB4	1291	725	0.10%	0.012%
73	12.120	3442	3446	3447	rBV4	1041	785	0.11%	0.013%
74	12.194	3466	3469	3472	rBV4	1346	932	0.13%	0.015%
75	12.480	3556	3558	3561	rBV4	978	722	0.10%	0.012%
76	12.603	3594	3596	3602	rVB7	2219	1779	0.24%	0.029%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
 Data File : VV030798.D
 Acq On : 24 Apr 2023 17:22
 Operator : SY/MD
 Sample : 02440-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMR3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	12.680	3618	3620	3625	rVB4	1698	1207	0.16%	0.019%
78	12.705	3625	3628	3633	rBV6	1195	1247	0.17%	0.020%
79	12.738	3633	3638	3641	rBV8	1081	1119	0.15%	0.018%
80	12.956	3702	3706	3710	rBV6	1492	1231	0.17%	0.020%
81	12.979	3710	3713	3716	rBV4	1527	1173	0.16%	0.019%
82	13.059	3733	3738	3743	rVV7	1873	1673	0.23%	0.027%
83	13.133	3759	3761	3765	rVB4	1493	1073	0.15%	0.017%
84	13.281	3805	3807	3810	rBV3	1169	695	0.09%	0.011%
85	13.451	3856	3860	3862	rBV5	1553	1181	0.16%	0.019%
86	13.548	3887	3890	3892	rBV2	1181	817	0.11%	0.013%
87	13.635	3915	3917	3922	rVB5	1832	1079	0.15%	0.017%
88	13.773	3957	3960	3963	rBV5	1392	923	0.12%	0.015%
89	13.869	3984	3990	3992	rBV5	1690	1412	0.19%	0.023%
90	13.892	3995	3997	4001	rBV5	1939	1333	0.18%	0.022%
91	14.120	4066	4068	4073	rVB6	1142	754	0.10%	0.012%
92	14.310	4124	4127	4130	rBV3	1228	775	0.10%	0.013%
93	14.458	4169	4173	4174	rBV2	1578	934	0.13%	0.015%
94	14.606	4215	4219	4221	rBV4	1852	1123	0.15%	0.018%
95	14.654	4229	4234	4235	rBV4	1279	1208	0.16%	0.019%
96	14.709	4249	4251	4255	rBV5	1101	827	0.11%	0.013%
97	14.856	4292	4297	4299	rBV6	1581	1499	0.20%	0.024%
98	15.172	4391	4395	4397	rBV4	2192	1538	0.21%	0.025%
99	15.316	4438	4440	4443	rBV3	1994	1358	0.18%	0.022%
100	15.429	4472	4475	4476	rBV3	1774	828	0.11%	0.013%




Sum of corrected areas: 6198363

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
Data File : VV030798.D
Acq On : 24 Apr 2023 17:22
Operator : SY/MD
Sample : 02440-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMR3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

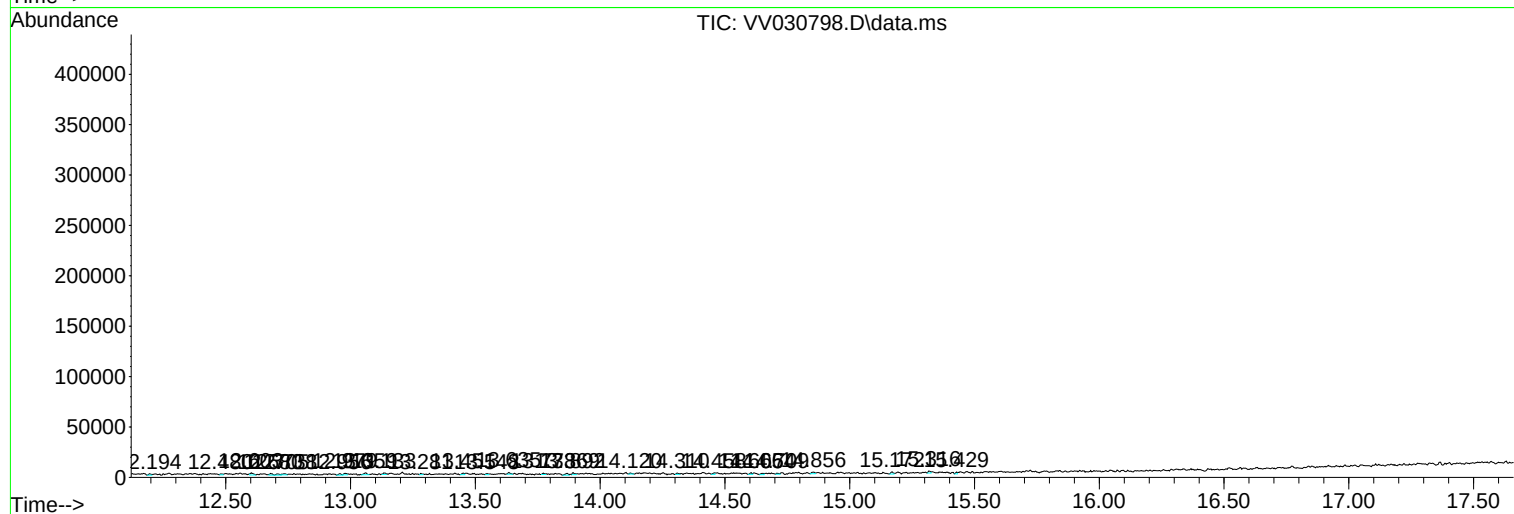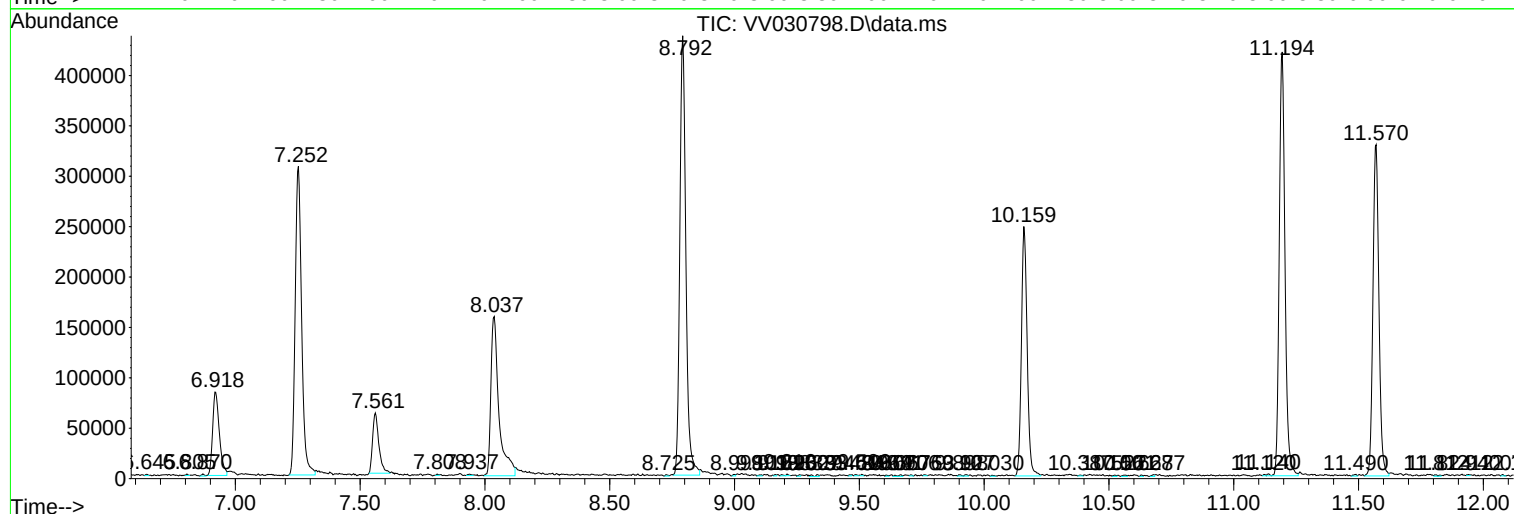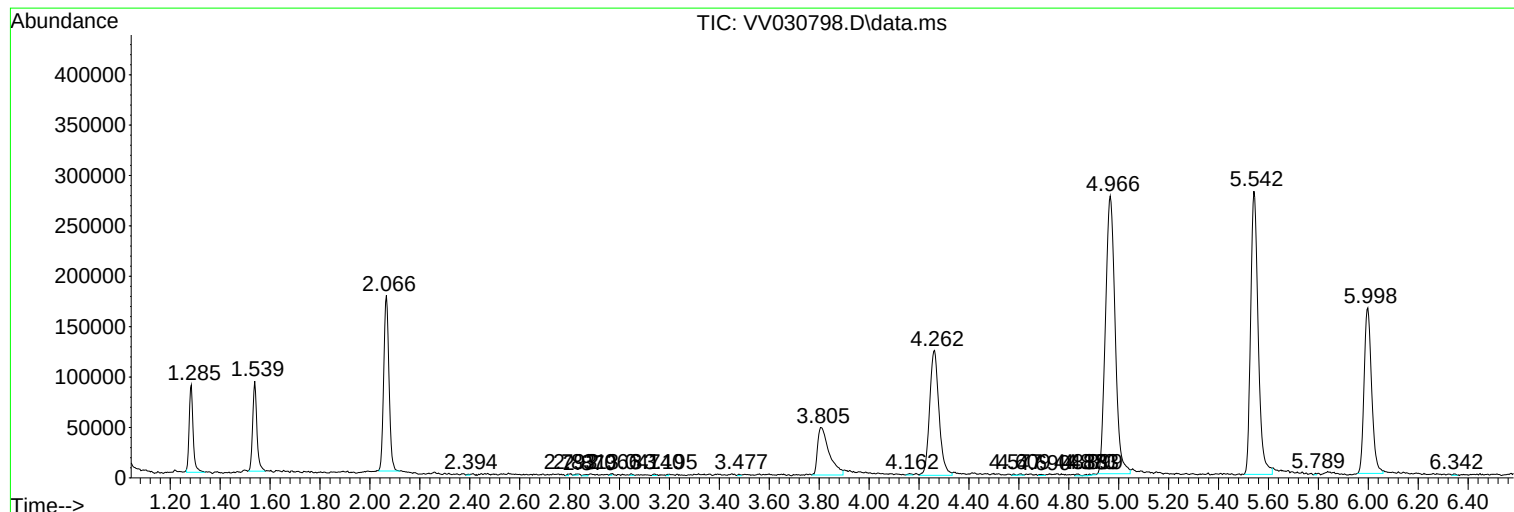

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
Data File : VV030798.D
Acq On : 24 Apr 2023 17:22
Operator : SY/MD
Sample : 02440-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMR3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
Data File : VV030798.D
Acq On : 24 Apr 2023 17:22
Operator : SY/MD
Sample : 02440-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMR3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------