

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
 Data File : VV030800.D
 Acq On : 24 Apr 2023 18:10
 Operator : SY/MD
 Sample : 02479-20
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW194

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030800.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.285	69	76	96	rVB	82658	93695	13.29%	1.580%
2	1.539	148	155	168	rVB	85408	97997	13.90%	1.653%
3	2.066	309	319	337	rBV	163918	244133	34.62%	4.118%
4	2.349	406	407	410	rBV3	1021	709	0.10%	0.012%
5	2.384	416	418	420	rVB3	1898	742	0.11%	0.013%
6	2.400	420	423	427	rBV6	1751	1464	0.21%	0.025%
7	2.426	428	431	436	rVV7	1523	1659	0.24%	0.028%
8	2.455	436	440	446	rVV8	2150	2886	0.41%	0.049%
9	2.490	449	451	456	rVB6	671	545	0.08%	0.009%
10	2.603	484	486	488	rBV3	913	523	0.07%	0.009%
11	2.728	522	525	527	rBV4	1859	1317	0.19%	0.022%
12	2.844	558	561	564	rBV5	1033	743	0.11%	0.013%
13	3.246	684	686	689	rVB4	1291	636	0.09%	0.011%
14	3.265	689	692	694	rBV3	1104	747	0.11%	0.013%
15	3.314	703	707	710	rBV5	1435	963	0.14%	0.016%
16	3.330	710	712	716	rBV5	759	627	0.09%	0.011%
17	3.352	716	719	722	rVB5	1304	826	0.12%	0.014%
18	3.506	763	767	769	rBV5	1508	1067	0.15%	0.018%
19	3.532	771	775	776	rBV3	1521	769	0.11%	0.013%
20	3.580	788	790	794	rVB5	964	554	0.08%	0.009%
21	3.680	817	821	828	rBV8	1505	1614	0.23%	0.027%
22	3.712	828	831	834	rVB5	963	725	0.10%	0.012%
23	3.809	850	861	887	rBV2	48519	148420	21.05%	2.503%
24	4.175	972	975	976	rBV3	1689	891	0.13%	0.015%
25	4.259	986	1001	1023	rBV	118519	303955	43.11%	5.126%
26	4.767	1156	1159	1162	rBV4	1324	1031	0.15%	0.017%
27	4.886	1191	1196	1197	rBV5	1248	635	0.09%	0.011%
28	4.966	1205	1221	1244	rBV2	260401	693350	98.33%	11.694%
29	5.214	1296	1298	1304	rVB6	1425	1004	0.14%	0.017%
30	5.265	1311	1314	1315	rBV2	1371	791	0.11%	0.013%
31	5.471	1374	1378	1379	rBV2	1360	812	0.12%	0.014%
32	5.542	1388	1400	1419	rBV	276604	572141	81.14%	9.650%
33	5.998	1530	1542	1562	rBV2	157894	324317	45.99%	5.470%
34	6.239	1614	1617	1618	rBV3	1329	759	0.11%	0.013%
35	6.481	1688	1692	1694	rBV5	1210	1031	0.15%	0.017%
36	6.526	1704	1706	1709	rBV3	1177	526	0.07%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042423\
 Data File : VW030800.D
 Acq On : 24 Apr 2023 18:10
 Operator : SY/MD
 Sample : 02479-20
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW194

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	6.574	1717	1721	1724	rBV5	1464	1434	0.20%	0.024%
38	6.921	1818	1829	1851	rBV	78826	154573	21.92%	2.607%
39	7.198	1913	1915	1918	rBV4	1063	658	0.09%	0.011%
40	7.252	1920	1932	1951	rBV	282825	507801	72.02%	8.565%
41	7.561	2019	2028	2045	rBV	56847	101398	14.38%	1.710%
42	7.751	2085	2087	2091	rBV4	1672	1125	0.16%	0.019%
43	7.969	2153	2155	2158	rBV4	1041	719	0.10%	0.012%
44	8.034	2166	2175	2209	rBV	159235	345726	49.03%	5.831%
45	8.439	2299	2301	2303	rBV3	1210	589	0.08%	0.010%
46	8.509	2322	2323	2326	rBV3	1217	760	0.11%	0.013%
47	8.554	2332	2337	2340	rBV7	1888	1998	0.28%	0.034%
48	8.638	2360	2363	2364	rBV3	1278	729	0.10%	0.012%
49	8.709	2382	2385	2386	rBV3	1343	778	0.11%	0.013%
50	8.725	2386	2390	2393	rVB6	1513	1055	0.15%	0.018%
51	8.792	2400	2411	2429	rBV	421033	705125	100.00%	11.893%
52	8.976	2465	2468	2471	rBV4	1623	1120	0.16%	0.019%
53	9.284	2560	2564	2566	rBV4	1188	885	0.13%	0.015%
54	9.471	2621	2622	2626	rBV4	1038	592	0.08%	0.010%
55	9.493	2627	2629	2633	rVV4	871	608	0.09%	0.010%
56	9.628	2665	2671	2672	rBV6	1530	1404	0.20%	0.024%
57	9.841	2733	2737	2738	rBV4	1005	667	0.09%	0.011%
58	9.895	2752	2754	2756	rVB3	1173	567	0.08%	0.010%
59	9.956	2771	2773	2775	rVV3	1465	574	0.08%	0.010%
60	10.001	2783	2787	2791	rBV5	1157	938	0.13%	0.016%
61	10.059	2802	2805	2806	rBV3	1546	776	0.11%	0.013%
62	10.085	2811	2813	2815	rVB3	1417	533	0.08%	0.009%
63	10.159	2823	2836	2856	rBV	232413	383834	54.43%	6.474%
64	10.252	2862	2865	2866	rBV2	1216	689	0.10%	0.012%
65	10.590	2968	2970	2974	rBV4	1013	899	0.13%	0.015%
66	10.702	3001	3005	3008	rBV6	1597	1312	0.19%	0.022%
67	10.950	3077	3082	3085	rBV6	1327	1529	0.22%	0.026%
68	10.982	3089	3092	3094	rVB4	1081	678	0.10%	0.011%
69	11.127	3133	3137	3144	rBV9	1201	1616	0.23%	0.027%
70	11.194	3147	3158	3174	rVV	410709	655709	92.99%	11.059%
71	11.448	3235	3237	3240	rBV3	1261	853	0.12%	0.014%
72	11.567	3262	3274	3295	rBV	309251	514971	73.03%	8.685%
73	11.908	3378	3380	3385	rBV6	1453	1327	0.19%	0.022%
74	12.136	3448	3451	3452	rBV3	1490	653	0.09%	0.011%
75	12.188	3463	3467	3470	rBV6	1407	1455	0.21%	0.025%
76	12.506	3562	3566	3570	rBV5	1356	1326	0.19%	0.022%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
 Data File : VV030800.D
 Acq On : 24 Apr 2023 18:10
 Operator : SY/MD
 Sample : 02479-20
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW194

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	12.532	3570	3574	3577	rVB6	1408	1292	0.18%	0.022%
78	12.683	3620	3621	3624	rVB2	1524	578	0.08%	0.010%
79	12.699	3624	3626	3629	rBV4	1232	907	0.13%	0.015%
80	12.757	3641	3644	3645	rBV3	1100	629	0.09%	0.011%
81	12.818	3658	3663	3665	rBV5	1786	1328	0.19%	0.022%
82	12.895	3685	3687	3690	rBV4	1114	817	0.12%	0.014%
83	13.094	3743	3749	3751	rBV6	1483	1242	0.18%	0.021%
84	13.252	3795	3798	3799	rVV3	1227	633	0.09%	0.011%
85	13.339	3824	3825	3829	rVB4	1605	751	0.11%	0.013%
86	13.545	3888	3889	3891	rBV2	1056	525	0.07%	0.009%
87	13.628	3912	3915	3917	rBV3	2192	1335	0.19%	0.023%
88	13.657	3921	3924	3927	rBV4	991	843	0.12%	0.014%
89	13.725	3943	3945	3948	rBV4	1480	848	0.12%	0.014%
90	14.130	4068	4071	4073	rBV3	1386	865	0.12%	0.015%
91	14.181	4082	4087	4090	rBV6	1791	1940	0.28%	0.033%
92	14.226	4097	4101	4103	rBV5	1047	954	0.14%	0.016%
93	14.352	4138	4140	4142	rBV3	1103	520	0.07%	0.009%
94	14.381	4147	4149	4155	rVB5	1045	940	0.13%	0.016%
95	14.455	4168	4172	4174	rBV5	2426	1744	0.25%	0.029%
96	14.503	4185	4187	4192	rVB6	2019	1228	0.17%	0.021%
97	14.612	4217	4221	4222	rBV5	1864	1331	0.19%	0.022%
98	14.651	4227	4233	4235	rBV6	1710	1778	0.25%	0.030%
99	14.670	4237	4239	4243	rBV4	1151	941	0.13%	0.016%
100	14.914	4313	4315	4316	rBV2	1566	558	0.08%	0.009%




Sum of corrected areas: 5929114

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
Data File : VV030800.D
Acq On : 24 Apr 2023 18:10
Operator : SY/MD
Sample : 02479-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW194

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

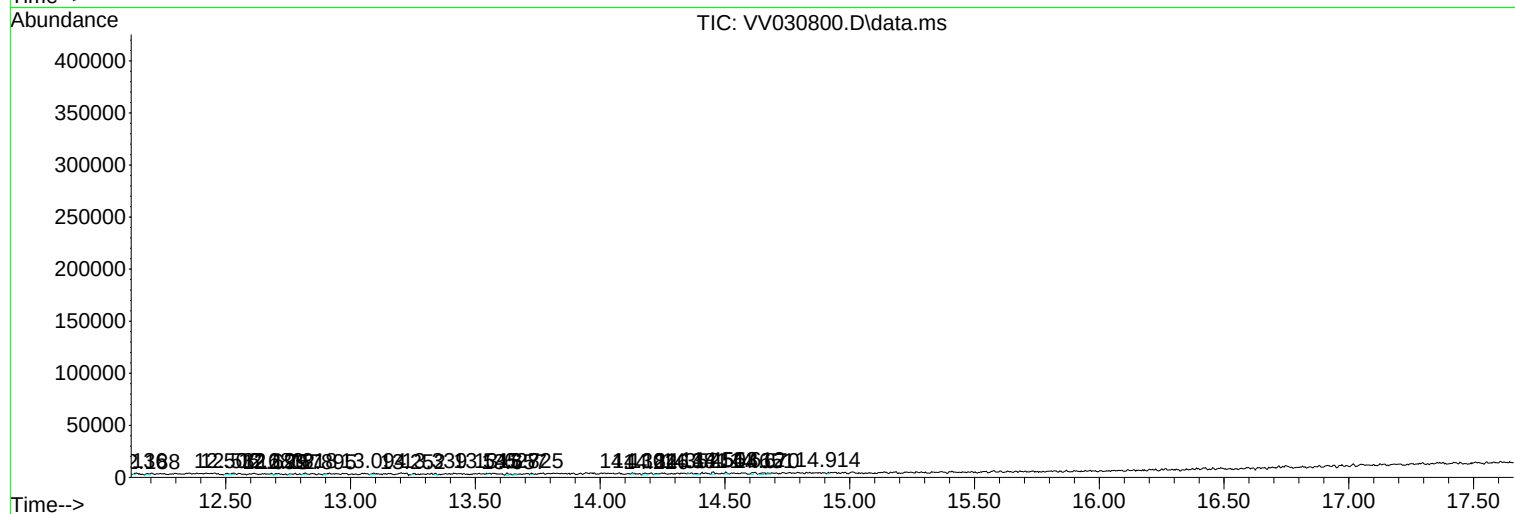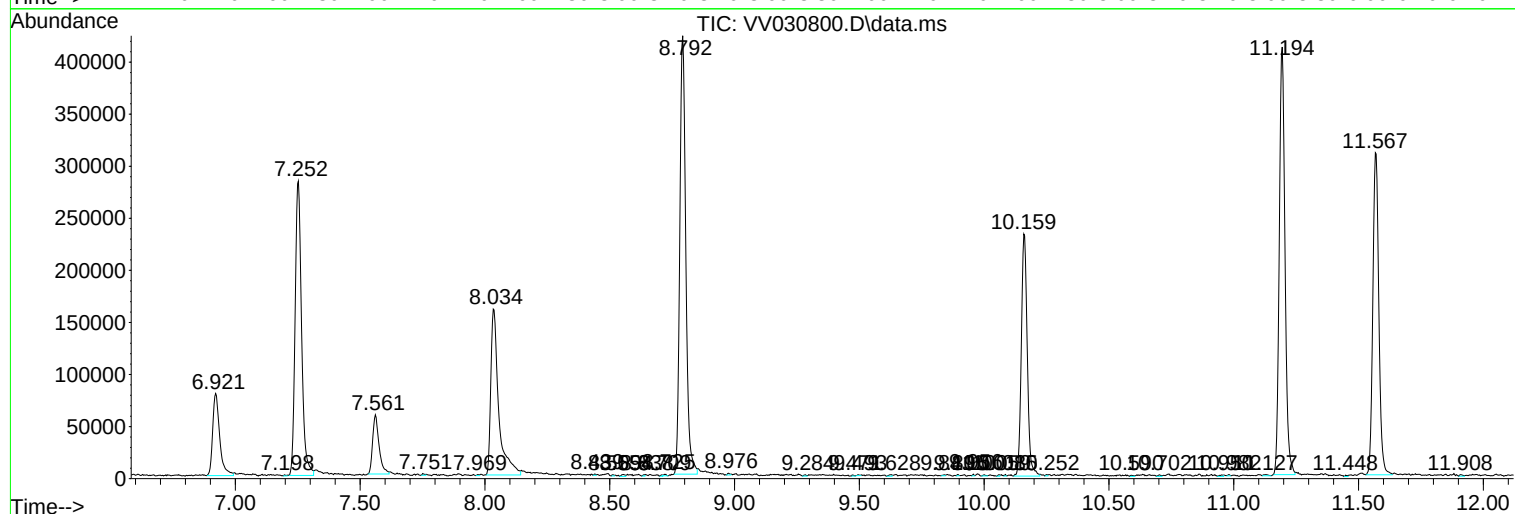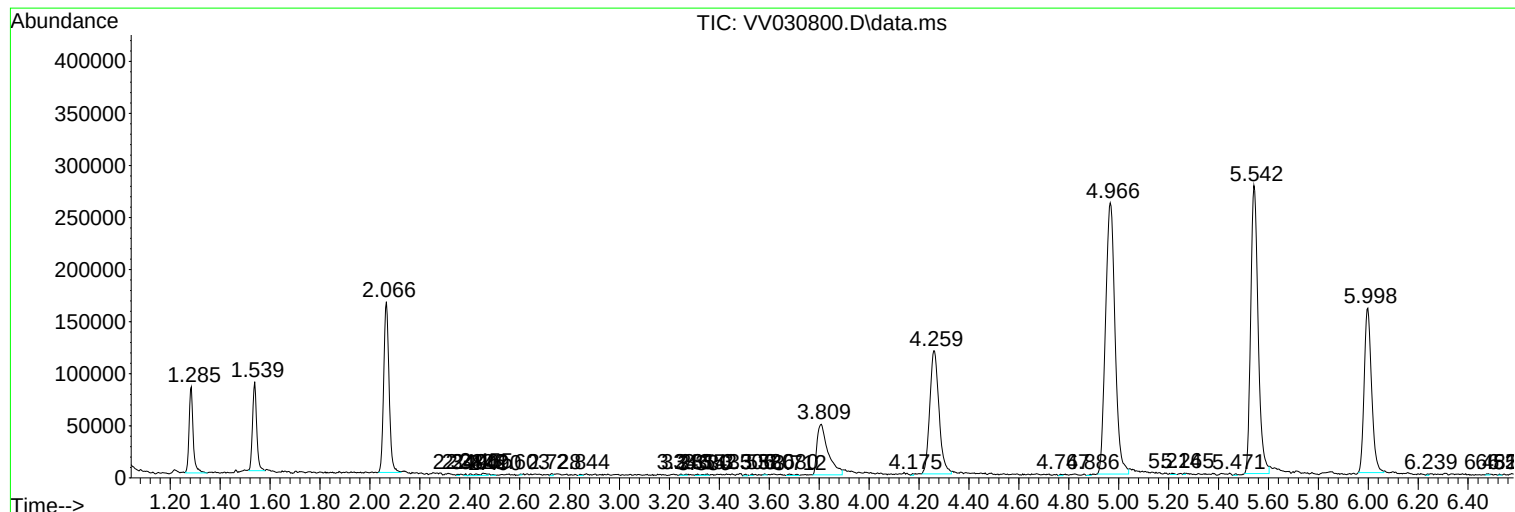

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
Data File : VV030800.D
Acq On : 24 Apr 2023 18:10
Operator : SY/MD
Sample : 02479-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW194

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
Data File : VV030800.D
Acq On : 24 Apr 2023 18:10
Operator : SY/MD
Sample : 02479-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW194

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------