

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
 Data File : VV030801.D
 Acq On : 24 Apr 2023 18:34
 Operator : SY/MD
 Sample : 02479-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW972

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030801.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	69	75	88	rVB	77392	84989	11.93%	1.448%
2	1.536	148	154	166	rVB	79251	93749	13.16%	1.597%
3	2.066	310	319	335	rVB	159562	234313	32.88%	3.991%
4	2.465	441	443	449	rVB5	2539	1996	0.28%	0.034%
5	2.494	449	452	453	rBV3	1621	924	0.13%	0.016%
6	2.568	471	475	480	rBV7	1498	1440	0.20%	0.025%
7	2.622	488	492	495	rBV6	1359	1387	0.19%	0.024%
8	2.658	500	503	505	rVB3	1293	740	0.10%	0.013%
9	2.863	565	567	571	rBV5	1140	756	0.11%	0.013%
10	2.982	599	604	608	rVB6	1391	1134	0.16%	0.019%
11	3.002	608	610	612	rBV3	889	520	0.07%	0.009%
12	3.056	624	627	633	rVB8	1191	1160	0.16%	0.020%
13	3.227	675	680	683	rBV6	1558	1312	0.18%	0.022%
14	3.365	717	723	724	rBV4	1471	1273	0.18%	0.022%
15	3.404	732	735	739	rBV5	1625	1313	0.18%	0.022%
16	3.423	739	741	745	rVV5	1660	1024	0.14%	0.017%
17	3.445	746	748	752	rVB5	1537	862	0.12%	0.015%
18	3.558	781	783	787	rVB3	1382	1103	0.15%	0.019%
19	3.587	787	792	796	rBV7	2007	2295	0.32%	0.039%
20	3.722	831	834	836	rBV4	1038	759	0.11%	0.013%
21	3.806	851	860	882	rBV2	47094	143484	20.14%	2.444%
22	4.185	974	978	981	rBV5	1723	1482	0.21%	0.025%
23	4.259	984	1001	1025	rVV	117255	310349	43.55%	5.286%
24	4.764	1156	1158	1162	rVB3	1093	588	0.08%	0.010%
25	4.966	1205	1221	1249	rBV3	253081	684119	96.00%	11.653%
26	5.223	1296	1301	1302	rBV4	1758	1145	0.16%	0.020%
27	5.294	1321	1323	1325	rBV2	1423	938	0.13%	0.016%
28	5.449	1369	1371	1374	rVB4	1769	738	0.10%	0.013%
29	5.468	1374	1377	1379	rBV4	990	695	0.10%	0.012%
30	5.542	1387	1400	1421	rBV	278212	579727	81.35%	9.875%
31	5.998	1530	1542	1564	rBV	156197	319678	44.86%	5.445%
32	6.307	1636	1638	1640	rBV3	1148	507	0.07%	0.009%
33	6.461	1685	1686	1689	rBV3	1193	569	0.08%	0.010%
34	6.567	1715	1719	1720	rBV3	1840	1052	0.15%	0.018%
35	6.886	1815	1818	1819	rBV3	1162	683	0.10%	0.012%
36	6.921	1819	1829	1848	rVV2	77147	147288	20.67%	2.509%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042423\
 Data File : VW030801.D
 Acq On : 24 Apr 2023 18:34
 Operator : SY/MD
 Sample : 02479-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW972

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	7.252	1920	1932	1947	rBV	274464	493480	69.25%	8.406%
38	7.561	2017	2028	2044	rBV	58314	109941	15.43%	1.873%
39	7.992	2160	2162	2165	rBV4	1392	558	0.08%	0.010%
40	8.034	2166	2175	2212	rBV	160071	349376	49.03%	5.951%
41	8.413	2291	2293	2294	rBV2	1191	501	0.07%	0.009%
42	8.452	2302	2305	2307	rBV3	1098	539	0.08%	0.009%
43	8.542	2330	2333	2337	rVB4	1777	1136	0.16%	0.019%
44	8.590	2345	2348	2350	rBV4	1102	669	0.09%	0.011%
45	8.677	2373	2375	2380	rVB6	1318	894	0.13%	0.015%
46	8.715	2384	2387	2390	rBV5	724	565	0.08%	0.010%
47	8.792	2400	2411	2435	rBV	418984	712593	100.00%	12.138%
48	9.320	2571	2575	2579	rBV7	1899	1558	0.22%	0.027%
49	9.419	2602	2606	2608	rVV5	1328	1045	0.15%	0.018%
50	9.548	2644	2646	2648	rBV3	1141	593	0.08%	0.010%
51	9.577	2653	2655	2660	rBV6	1011	711	0.10%	0.012%
52	9.645	2673	2676	2679	rBV5	873	701	0.10%	0.012%
53	9.783	2717	2719	2722	rVB4	1145	531	0.07%	0.009%
54	9.831	2731	2734	2736	rBV4	946	715	0.10%	0.012%
55	9.886	2747	2751	2752	rBV3	1082	584	0.08%	0.010%
56	10.120	2818	2824	2825	rBV5	1184	1238	0.17%	0.021%
57	10.159	2825	2836	2851	rVV	232122	376035	52.77%	6.405%
58	10.336	2886	2891	2897	rVV9	2556	3312	0.46%	0.056%
59	10.407	2909	2913	2915	rBV5	1531	1193	0.17%	0.020%
60	10.722	3007	3011	3012	rBV4	803	567	0.08%	0.010%
61	10.757	3018	3022	3023	rBV3	1588	1041	0.15%	0.018%
62	10.789	3029	3032	3033	rBV3	1648	779	0.11%	0.013%
63	10.966	3084	3087	3090	rBV4	1354	1021	0.14%	0.017%
64	11.030	3105	3107	3114	rVB7	1328	1225	0.17%	0.021%
65	11.062	3114	3117	3119	rVB3	921	526	0.07%	0.009%
66	11.082	3119	3123	3127	rBV6	1029	959	0.13%	0.016%
67	11.194	3147	3158	3175	rBV	402249	650273	91.25%	11.077%
68	11.570	3264	3275	3295	rVB	307043	502682	70.54%	8.563%
69	11.728	3322	3324	3327	rBV4	1243	682	0.10%	0.012%
70	11.876	3368	3370	3371	rBV2	1398	531	0.07%	0.009%
71	11.898	3373	3377	3379	rBV5	1154	891	0.13%	0.015%
72	11.953	3392	3394	3397	rBV4	824	546	0.08%	0.009%
73	11.969	3397	3399	3403	rBV5	1478	940	0.13%	0.016%
74	12.104	3439	3441	3442	rBV2	1253	495	0.07%	0.008%
75	12.165	3457	3460	3463	rBV6	1304	915	0.13%	0.016%
76	12.320	3501	3508	3511	rBV6	1544	2108	0.30%	0.036%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
 Data File : VV030801.D
 Acq On : 24 Apr 2023 18:34
 Operator : SY/MD
 Sample : 02479-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW972

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	12.336	3511	3513	3516	rVV3	845	581	0.08%	0.010%
78	12.635	3604	3606	3609	rVB3	1215	602	0.08%	0.010%
79	12.657	3611	3613	3615	rVV2	1197	620	0.09%	0.011%
80	12.686	3618	3622	3623	rBV4	1061	853	0.12%	0.015%
81	12.760	3641	3645	3649	rBV6	1581	1340	0.19%	0.023%
82	12.873	3679	3680	3683	rVB3	1126	464	0.07%	0.008%
83	12.889	3683	3685	3687	rVV3	1236	499	0.07%	0.008%
84	12.934	3696	3699	3701	rBV4	1155	640	0.09%	0.011%
85	13.066	3737	3740	3741	rBV2	1417	634	0.09%	0.011%
86	13.082	3741	3745	3748	rVV6	1850	1501	0.21%	0.026%
87	13.095	3748	3749	3753	rVB3	1115	640	0.09%	0.011%
88	13.136	3759	3762	3765	rBV5	1391	1138	0.16%	0.019%
89	13.191	3777	3779	3781	rVV3	1323	659	0.09%	0.011%
90	13.236	3790	3793	3795	rBV4	1137	807	0.11%	0.014%
91	13.291	3808	3810	3812	rBV3	1114	599	0.08%	0.010%
92	13.390	3836	3841	3843	rBV5	1216	1097	0.15%	0.019%
93	13.413	3846	3848	3849	rBV2	1413	497	0.07%	0.008%
94	13.513	3875	3879	3880	rBV4	1162	671	0.09%	0.011%
95	13.583	3900	3901	3904	rBV4	975	488	0.07%	0.008%
96	13.609	3907	3909	3914	rVB6	1887	1200	0.17%	0.020%
97	14.149	4072	4077	4079	rBV5	1265	1267	0.18%	0.022%
98	14.300	4122	4124	4127	rBV3	1530	845	0.12%	0.014%
99	14.464	4170	4175	4176	rBV5	1421	1153	0.16%	0.020%
100	14.628	4224	4226	4228	rBV2	2046	1197	0.17%	0.020%




Sum of corrected areas: 5870732

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
Data File : VV030801.D
Acq On : 24 Apr 2023 18:34
Operator : SY/MD
Sample : 02479-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW972

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

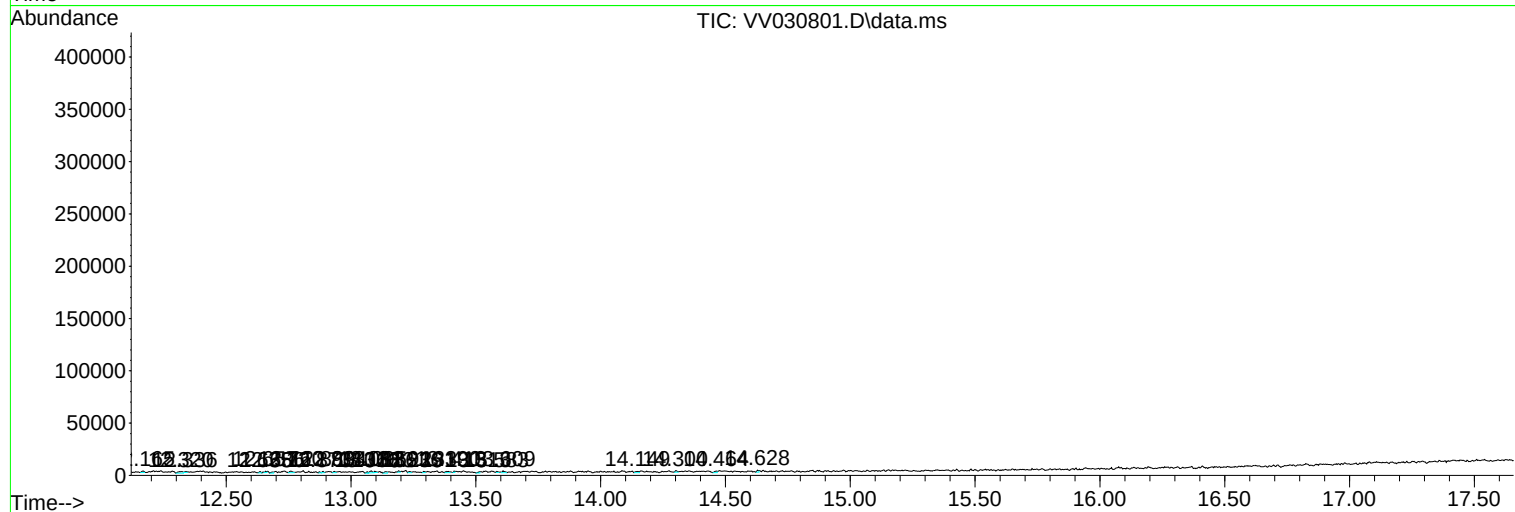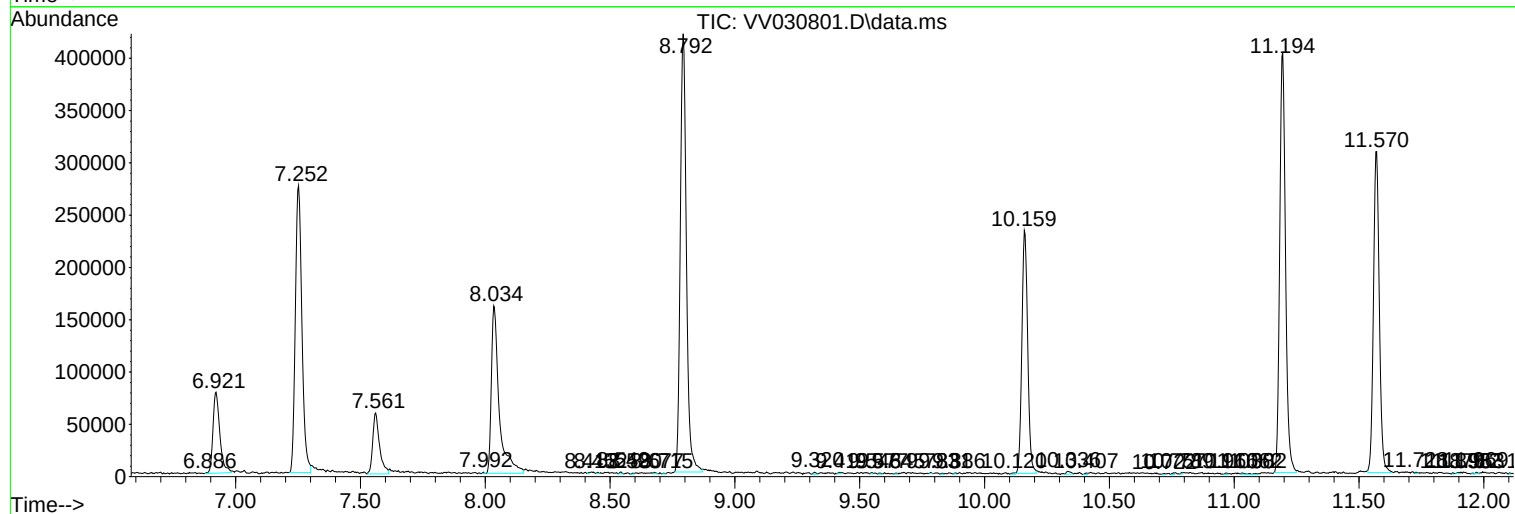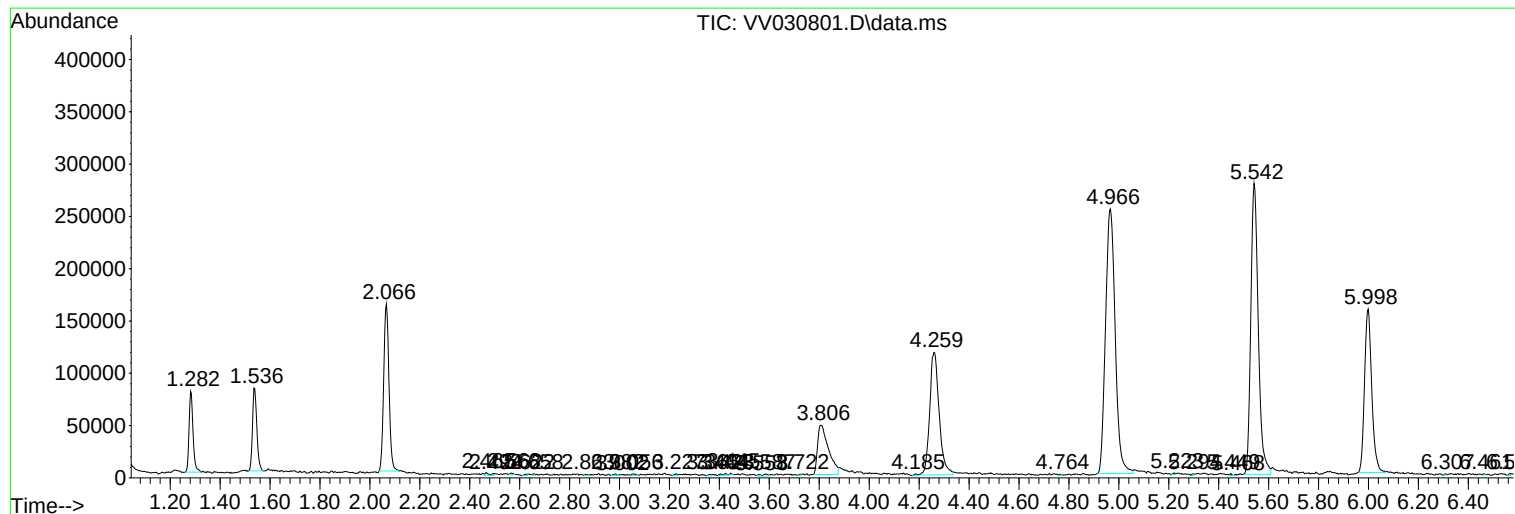

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
Data File : VV030801.D
Acq On : 24 Apr 2023 18:34
Operator : SY/MD
Sample : 02479-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW972

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
Data File : VV030801.D
Acq On : 24 Apr 2023 18:34
Operator : SY/MD
Sample : 02479-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW972

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------