

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
 Data File : VV030802.D
 Acq On : 24 Apr 2023 18:58
 Operator : SY/MD
 Sample : 02440-15 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMR0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030802.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.185	43	45	47	rBV3	1453	846	0.03%	0.010%
2	1.285	69	76	86	rBV	78667	84750	3.29%	0.952%
3	1.539	148	155	167	rVB	85671	99993	3.88%	1.124%
4	2.066	310	319	333	rBV	160723	232691	9.03%	2.615%
5	2.455	433	440	451	rVB3	14810	25674	1.00%	0.289%
6	2.577	475	478	482	rBV6	1798	1061	0.04%	0.012%
7	2.780	539	541	546	rBV6	1441	989	0.04%	0.011%
8	2.921	579	585	586	rBV6	1046	977	0.04%	0.011%
9	2.986	600	605	610	rBV7	2070	2458	0.10%	0.028%
10	3.021	614	616	619	rVV3	1495	669	0.03%	0.008%
11	3.056	622	627	632	rBV8	1415	1049	0.04%	0.012%
12	3.182	662	666	669	rBV7	1870	1715	0.07%	0.019%
13	3.278	694	696	699	rVB3	1410	593	0.02%	0.007%
14	3.310	703	706	707	rBV3	1897	1028	0.04%	0.012%
15	3.397	729	733	734	rBV4	1024	660	0.03%	0.007%
16	3.497	762	764	766	rBV4	1069	561	0.02%	0.006%
17	3.535	774	776	777	rBV2	1171	536	0.02%	0.006%
18	3.693	823	825	827	rVB3	1364	597	0.02%	0.007%
19	3.709	827	830	832	rBV3	1202	745	0.03%	0.008%
20	3.744	836	841	843	rBV5	1288	1009	0.04%	0.011%
21	3.805	850	860	884	rBV2	48835	144923	5.62%	1.629%
22	4.043	931	934	935	rBV3	1826	1000	0.04%	0.011%
23	4.117	955	957	962	rBV4	1430	1006	0.04%	0.011%
24	4.259	987	1001	1025	rBV	116056	292087	11.34%	3.283%
25	4.838	1179	1181	1185	rVB5	930	563	0.02%	0.006%
26	4.866	1185	1190	1192	rBV5	1205	1192	0.05%	0.013%
27	4.966	1204	1221	1241	rBV2	260005	693386	26.91%	7.793%
28	5.333	1333	1335	1337	rBV3	1708	875	0.03%	0.010%
29	5.374	1346	1348	1350	rBV3	1720	772	0.03%	0.009%
30	5.542	1388	1400	1425	rBV	284197	595978	23.13%	6.698%
31	5.998	1531	1542	1558	rBV2	153499	307268	11.92%	3.453%
32	6.284	1626	1631	1632	rBV5	1732	1273	0.05%	0.014%
33	6.419	1669	1673	1676	rVB6	1479	1026	0.04%	0.012%
34	6.439	1677	1679	1683	rBV5	1371	849	0.03%	0.010%
35	6.571	1717	1720	1721	rBV2	1239	677	0.03%	0.008%
36	6.690	1755	1757	1760	rBV4	1187	799	0.03%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042423\
 Data File : VW030802.D
 Acq On : 24 Apr 2023 18:58
 Operator : SY/MD
 Sample : 02440-15 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMR0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	6.715	1763	1765	1766	rBV2	964	525	0.02%	0.006%
38	6.792	1787	1789	1793	rBV5	1371	846	0.03%	0.010%
39	6.815	1794	1796	1800	rVV5	795	537	0.02%	0.006%
40	6.921	1820	1829	1843	rBV	75327	138859	5.39%	1.561%
41	7.114	1886	1889	1892	rBV4	1434	1088	0.04%	0.012%
42	7.143	1896	1898	1901	rBV5	1320	728	0.03%	0.008%
43	7.178	1907	1909	1913	rBV5	1786	1300	0.05%	0.015%
44	7.252	1918	1932	1953	rBV	283133	513729	19.94%	5.774%
45	7.561	2017	2028	2050	rBV	57907	111179	4.31%	1.249%
46	7.686	2064	2067	2068	rBV3	1085	538	0.02%	0.006%
47	7.760	2088	2090	2093	rBV4	1533	872	0.03%	0.010%
48	7.850	2117	2118	2120	rBV2	951	478	0.02%	0.005%
49	7.931	2140	2143	2145	rVB3	1040	496	0.02%	0.006%
50	8.034	2163	2175	2210	rBV	166236	353438	13.72%	3.972%
51	8.792	2398	2411	2438	rBV2	450608	916151	35.55%	10.296%
52	8.950	2458	2460	2462	rBV4	1889	1080	0.04%	0.012%
53	9.059	2492	2494	2500	rBV6	1093	571	0.02%	0.006%
54	9.185	2529	2533	2536	rBV5	1951	1526	0.06%	0.017%
55	9.355	2584	2586	2587	rVV2	1276	481	0.02%	0.005%
56	9.381	2591	2594	2596	rBV3	1020	647	0.03%	0.007%
57	9.413	2603	2604	2612	rVB6	1546	1559	0.06%	0.018%
58	9.445	2612	2614	2615	rBV2	1275	641	0.02%	0.007%
59	9.506	2630	2633	2634	rBV3	1659	683	0.03%	0.008%
60	9.535	2639	2642	2643	rBV3	994	596	0.02%	0.007%
61	9.554	2646	2648	2650	rVB3	1213	490	0.02%	0.006%
62	9.570	2650	2653	2656	rVB3	1553	866	0.03%	0.010%
63	9.654	2676	2679	2683	rBV4	1679	1847	0.07%	0.021%
64	9.960	2771	2774	2775	rBV3	1081	498	0.02%	0.006%
65	10.159	2826	2836	2856	rVB	233649	375490	14.57%	4.220%
66	10.332	2888	2890	2891	rBV2	1225	501	0.02%	0.006%
67	10.397	2909	2910	2914	rBV2	782	494	0.02%	0.006%
68	10.525	2947	2950	2955	rBV7	1932	1607	0.06%	0.018%
69	10.641	2983	2986	2988	rBV3	1073	801	0.03%	0.009%
70	10.754	3018	3021	3023	rBV5	1420	923	0.04%	0.010%
71	10.844	3047	3049	3051	rBV2	1200	567	0.02%	0.006%
72	10.863	3051	3055	3056	rVV4	1011	637	0.02%	0.007%
73	10.889	3059	3063	3066	rVV5	1243	755	0.03%	0.008%
74	10.969	3086	3088	3090	rVB3	1401	661	0.03%	0.007%
75	10.985	3090	3093	3094	rBV3	1183	697	0.03%	0.008%
76	11.127	3128	3137	3146	rBV	42000	68786	2.67%	0.773%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
 Data File : VV030802.D
 Acq On : 24 Apr 2023 18:58
 Operator : SY/MD
 Sample : 02440-15 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMR0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	11.194	3148	3158	3181	rVB2	457908	1010922	39.23%	11.361%
78	11.471	3242	3244	3247	rVB4	1412	759	0.03%	0.009%
79	11.516	3256	3258	3261	rBV4	1266	881	0.03%	0.010%
80	11.586	3263	3280	3301	rVV2	1391164	2576814	100.00%	28.959%
81	11.895	3374	3376	3378	rBV3	1768	808	0.03%	0.009%
82	11.918	3381	3383	3390	rBV7	1073	1244	0.05%	0.014%
83	12.043	3420	3422	3424	rVB3	1841	758	0.03%	0.009%
84	12.062	3424	3428	3430	rBV5	1853	1333	0.05%	0.015%
85	12.310	3503	3505	3508	rVB3	1922	1117	0.04%	0.013%
86	12.332	3508	3512	3513	rBV4	1855	1048	0.04%	0.012%
87	12.455	3548	3550	3554	rBV4	1171	684	0.03%	0.008%
88	12.538	3574	3576	3577	rBV2	1373	493	0.02%	0.006%
89	12.648	3605	3610	3611	rBV5	1592	1239	0.05%	0.014%
90	12.918	3692	3694	3695	rBV2	1137	471	0.02%	0.005%
91	13.207	3774	3784	3795	rBV	155455	238494	9.26%	2.680%
92	13.490	3869	3872	3873	rBV3	1455	668	0.03%	0.008%
93	13.689	3926	3934	3947	rVB2	30661	47932	1.86%	0.539%
94	13.914	4002	4004	4008	rVB5	1575	683	0.03%	0.008%
95	13.959	4015	4018	4021	rBV4	1435	932	0.04%	0.010%
96	14.107	4062	4064	4066	rBV3	1087	478	0.02%	0.005%
97	14.165	4077	4082	4083	rBV5	1041	1033	0.04%	0.012%
98	14.509	4188	4189	4191	rVB2	1695	472	0.02%	0.005%
99	14.528	4191	4195	4197	rBV4	2465	1658	0.06%	0.019%
100	14.934	4319	4321	4325	rBV5	1118	649	0.03%	0.007%




Sum of corrected areas: 8898013

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
Data File : VV030802.D
Acq On : 24 Apr 2023 18:58
Operator : SY/MD
Sample : 02440-15 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMR0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

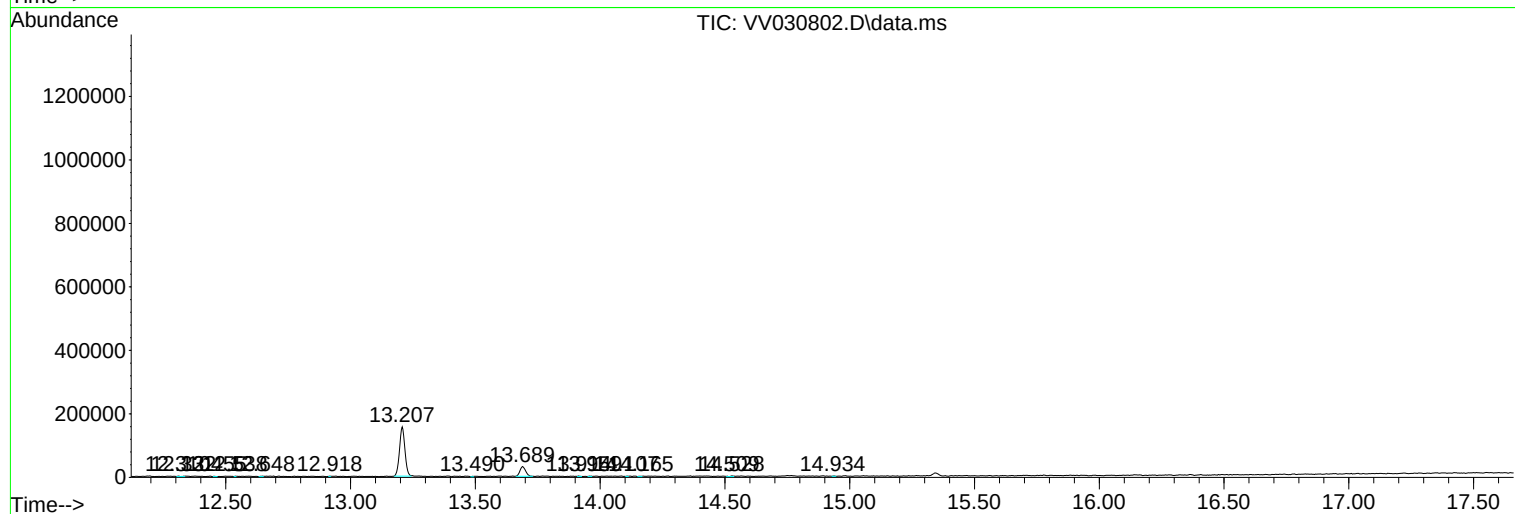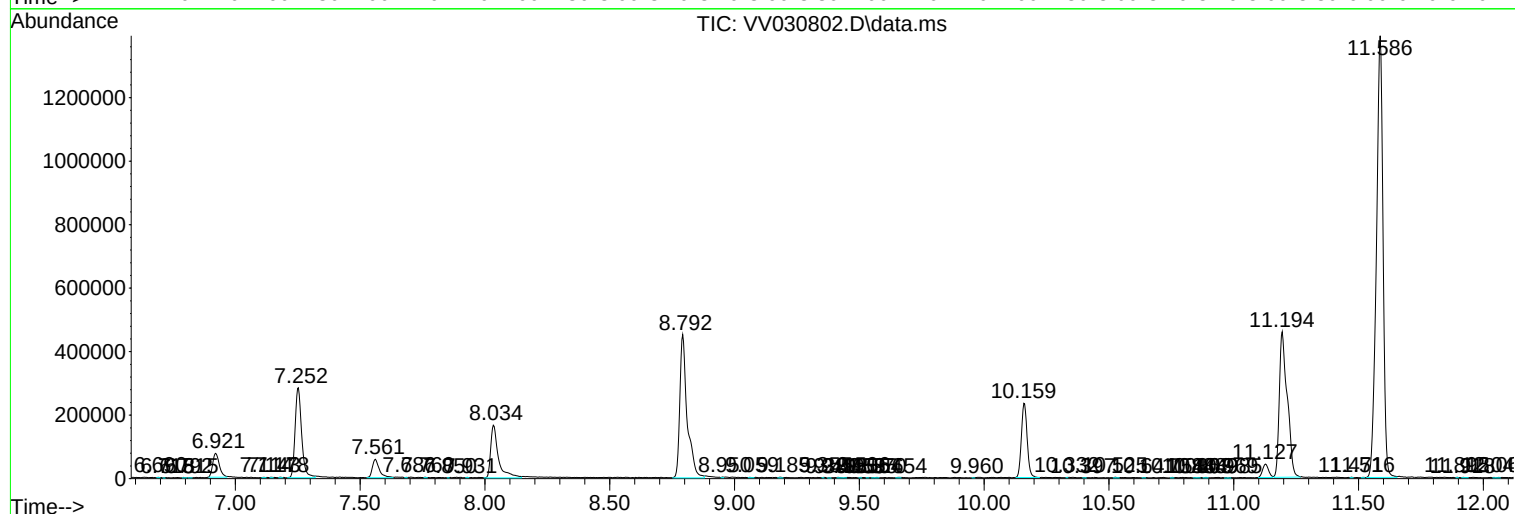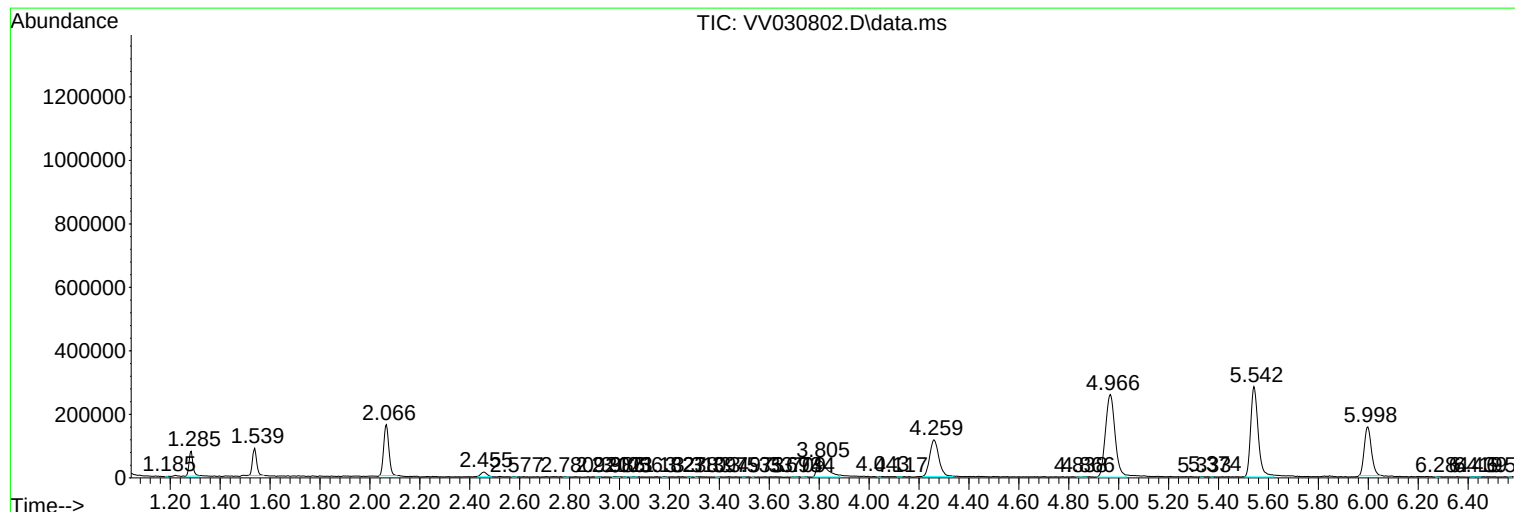

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
Data File : VV030802.D
Acq On : 24 Apr 2023 18:58
Operator : SY/MD
Sample : 02440-15 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMR0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
Data File : VV030802.D
Acq On : 24 Apr 2023 18:58
Operator : SY/MD
Sample : 02440-15 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMR0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------