

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
 Data File : VV030803.D
 Acq On : 24 Apr 2023 19:21
 Operator : SY/MD
 Sample : 02398-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMN4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030803.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.285	69	76	88	rBV	116140	123677	14.18%	1.723%
2	1.539	148	155	167	rVB	104686	125408	14.38%	1.747%
3	2.066	310	319	335	rVB	214105	314843	36.10%	4.387%
4	2.313	393	396	397	rBV3	972	483	0.06%	0.007%
5	2.439	433	435	436	rBV2	1120	386	0.04%	0.005%
6	2.545	464	468	469	rBV4	1847	1330	0.15%	0.019%
7	2.670	506	507	510	rBV3	857	504	0.06%	0.007%
8	2.802	547	548	552	rVB4	840	427	0.05%	0.006%
9	2.828	552	556	560	rVB7	1333	1227	0.14%	0.017%
10	2.854	560	564	567	rBV4	1149	1133	0.13%	0.016%
11	2.902	576	579	580	rBV3	711	418	0.05%	0.006%
12	3.104	639	642	645	rBV3	1336	1023	0.12%	0.014%
13	3.159	657	659	660	rBV2	888	405	0.05%	0.006%
14	3.169	660	662	665	rVV3	1071	611	0.07%	0.009%
15	3.243	681	685	687	rBV4	1377	802	0.09%	0.011%
16	3.281	694	697	702	rVB6	1271	1207	0.14%	0.017%
17	3.387	728	730	733	rBV4	803	416	0.05%	0.006%
18	3.413	736	738	741	rVB5	1809	852	0.10%	0.012%
19	3.474	755	757	759	rVB2	1376	548	0.06%	0.008%
20	3.606	795	798	799	rBV3	1525	1023	0.12%	0.014%
21	3.664	814	816	817	rBV3	1005	415	0.05%	0.006%
22	3.805	850	860	883	rBV2	58457	179111	20.54%	2.496%
23	4.259	987	1001	1028	rBV2	143029	382360	43.84%	5.328%
24	4.680	1130	1132	1138	rVB6	1674	1184	0.14%	0.016%
25	4.860	1186	1188	1190	rVB4	1108	487	0.06%	0.007%
26	4.886	1193	1196	1198	rVV4	1388	627	0.07%	0.009%
27	4.966	1204	1221	1252	rBV2	320530	872109	100.00%	12.152%
28	5.474	1376	1379	1380	rBV3	977	588	0.07%	0.008%
29	5.542	1385	1400	1425	rBV	279061	589637	67.61%	8.216%
30	5.998	1530	1542	1560	rBV2	187378	382610	43.87%	5.331%
31	6.214	1607	1609	1611	rBV3	1390	594	0.07%	0.008%
32	6.394	1661	1665	1667	rBV4	875	890	0.10%	0.012%
33	6.481	1690	1692	1697	rVB5	1511	1213	0.14%	0.017%
34	6.503	1697	1699	1703	rBV4	1405	1115	0.13%	0.016%
35	6.567	1716	1719	1722	rBV3	1300	692	0.08%	0.010%
36	6.654	1742	1746	1748	rBV4	2208	1752	0.20%	0.024%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042423\
 Data File : VW030803.D
 Acq On : 24 Apr 2023 19:21
 Operator : SY/MD
 Sample : 02398-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMN4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	6.738	1769	1772	1776	rVB5	1679	1290	0.15%	0.018%
38	6.821	1796	1798	1802	rVB5	1537	984	0.11%	0.014%
39	6.847	1802	1806	1807	rBV3	1024	689	0.08%	0.010%
40	6.921	1819	1829	1845	rBV	94705	180444	20.69%	2.514%
41	7.140	1892	1897	1899	rBV6	1429	1304	0.15%	0.018%
42	7.252	1920	1932	1956	rBV	368206	662331	75.95%	9.229%
43	7.487	2003	2005	2006	rBV2	1386	523	0.06%	0.007%
44	7.561	2019	2028	2049	rBV	69501	127994	14.68%	1.783%
45	7.754	2085	2088	2089	rBV3	1090	663	0.08%	0.009%
46	7.821	2107	2109	2110	rBV2	1325	467	0.05%	0.007%
47	8.033	2166	2175	2207	rBV	167551	357504	40.99%	4.981%
48	8.406	2289	2291	2294	rVB4	1308	497	0.06%	0.007%
49	8.792	2400	2411	2440	rBV2	431730	860551	98.67%	11.991%
50	9.423	2605	2607	2608	rBV2	1276	501	0.06%	0.007%
51	9.435	2608	2611	2614	rVV4	1715	1417	0.16%	0.020%
52	9.500	2629	2631	2635	rVB4	897	401	0.05%	0.006%
53	9.635	2670	2673	2675	rBV4	1822	1106	0.13%	0.015%
54	9.712	2695	2697	2701	rVB3	1644	1129	0.13%	0.016%
55	9.734	2701	2704	2709	rBV5	2453	2306	0.26%	0.032%
56	9.860	2741	2743	2745	rBV4	1141	422	0.05%	0.006%
57	9.898	2753	2755	2756	rBV2	916	397	0.05%	0.006%
58	10.017	2788	2792	2797	rVB6	981	880	0.10%	0.012%
59	10.040	2797	2799	2801	rBV3	837	433	0.05%	0.006%
60	10.159	2825	2836	2852	rVV	260581	418185	47.95%	5.827%
61	10.381	2901	2905	2908	rBV5	1408	1252	0.14%	0.017%
62	10.461	2929	2930	2933	rBV3	955	428	0.05%	0.006%
63	10.487	2935	2938	2940	rVV4	1166	761	0.09%	0.011%
64	10.506	2942	2944	2948	rVB4	1640	785	0.09%	0.011%
65	10.667	2988	2994	2996	rBV6	1982	1974	0.23%	0.028%
66	10.767	3023	3025	3026	rBV2	1063	381	0.04%	0.005%
67	10.834	3044	3046	3047	rBV2	1332	565	0.06%	0.008%
68	10.908	3066	3069	3072	rVB4	1479	926	0.11%	0.013%
69	10.934	3072	3077	3083	rBV9	1545	2177	0.25%	0.030%
70	10.992	3093	3095	3101	rVB6	1647	1123	0.13%	0.016%
71	11.049	3110	3113	3115	rBV4	1131	717	0.08%	0.010%
72	11.098	3123	3128	3130	rBV5	1836	1463	0.17%	0.020%
73	11.194	3147	3158	3179	rBV	413055	733920	84.15%	10.226%
74	11.419	3226	3228	3231	rBV4	1352	543	0.06%	0.008%
75	11.570	3263	3275	3295	rBV2	402281	728856	83.57%	10.156%
76	11.786	3339	3342	3345	rBV4	1468	1133	0.13%	0.016%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
 Data File : VV030803.D
 Acq On : 24 Apr 2023 19:21
 Operator : SY/MD
 Sample : 02398-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMN4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	11.930	3383	3387	3389	rBV5	1164	925	0.11%	0.013%
78	11.988	3399	3405	3410	rVB9	1602	2050	0.24%	0.029%
79	12.014	3410	3413	3415	rBV4	810	573	0.07%	0.008%
80	12.114	3442	3444	3447	rBV4	875	507	0.06%	0.007%
81	12.175	3461	3463	3466	rBV4	934	525	0.06%	0.007%
82	12.268	3488	3492	3494	rBV4	2013	1354	0.16%	0.019%
83	12.323	3506	3509	3510	rBV3	1039	586	0.07%	0.008%
84	12.593	3587	3593	3597	rBV8	1763	2252	0.26%	0.031%
85	12.683	3619	3621	3623	rBV3	929	474	0.05%	0.007%
86	12.709	3627	3629	3634	rBV6	1422	1019	0.12%	0.014%
87	13.037	3728	3731	3733	rBV3	752	414	0.05%	0.006%
88	13.053	3733	3736	3740	rBV5	1291	1066	0.12%	0.015%
89	13.146	3762	3765	3767	rVB4	1479	838	0.10%	0.012%
90	13.210	3777	3785	3796	rVB3	30816	47812	5.48%	0.666%
91	13.477	3866	3868	3872	rBV4	1273	1194	0.14%	0.017%
92	13.622	3911	3913	3914	rBV2	1078	433	0.05%	0.006%
93	13.692	3929	3935	3947	rVB7	11326	18220	2.09%	0.254%
94	13.737	3947	3949	3951	rBV3	932	477	0.05%	0.007%
95	13.750	3951	3953	3954	rBV2	919	427	0.05%	0.006%
96	14.188	4087	4089	4093	rBV4	921	579	0.07%	0.008%
97	14.236	4102	4104	4107	rBV4	1311	555	0.06%	0.008%
98	14.622	4221	4224	4226	rVB4	1116	599	0.07%	0.008%
99	14.667	4236	4238	4240	rBV2	1936	856	0.10%	0.012%
100	15.027	4347	4350	4352	rBV3	1972	1499	0.17%	0.021%




Sum of corrected areas: 7176763

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
Data File : VV030803.D
Acq On : 24 Apr 2023 19:21
Operator : SY/MD
Sample : 02398-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMN4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

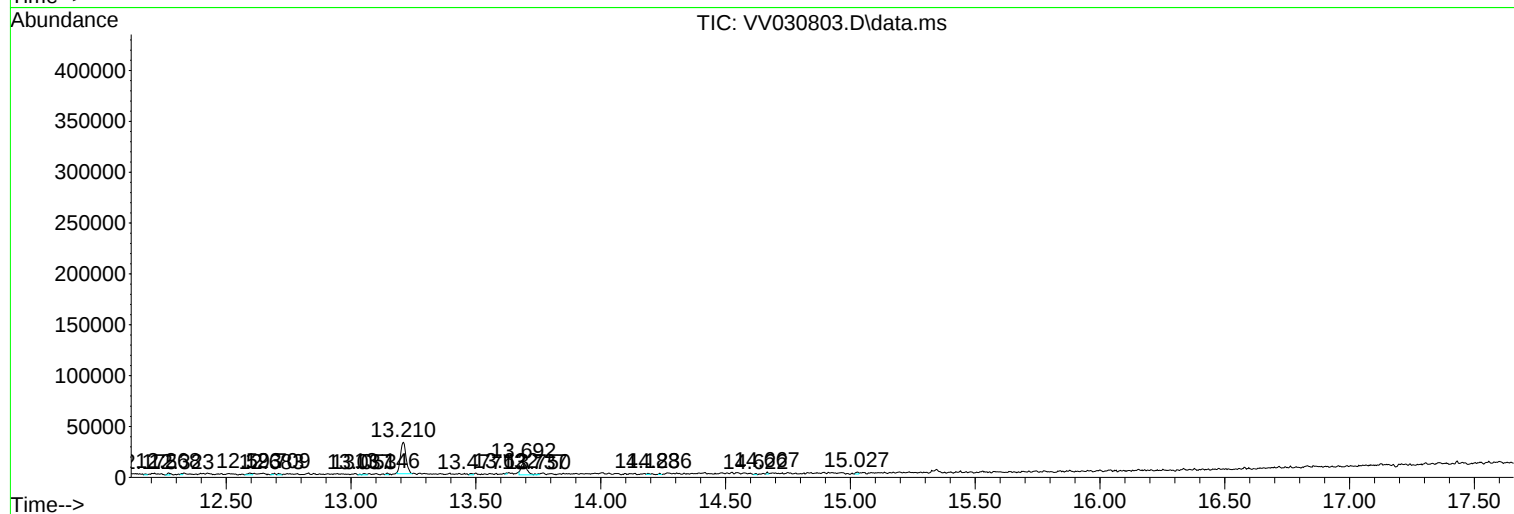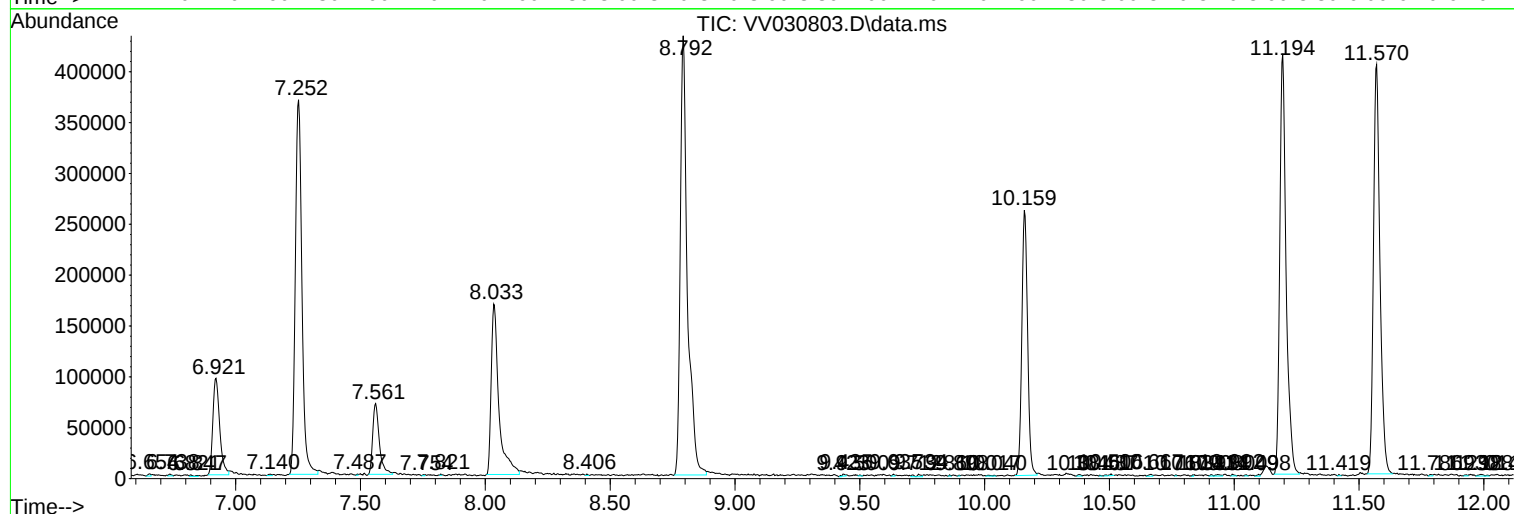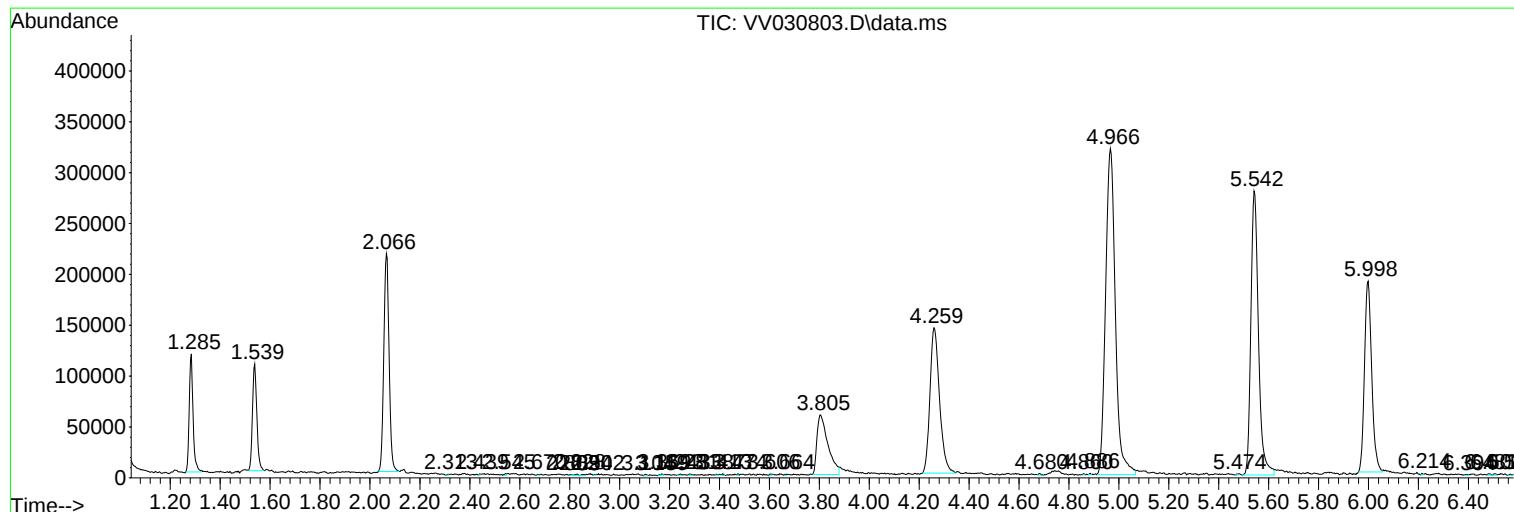

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
Data File : VV030803.D
Acq On : 24 Apr 2023 19:21
Operator : SY/MD
Sample : 02398-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMN4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
Data File : VV030803.D
Acq On : 24 Apr 2023 19:21
Operator : SY/MD
Sample : 02398-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMN4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------