

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
 Data File : VV030805.D
 Acq On : 24 Apr 2023 20:09
 Operator : SY/MD
 Sample : 02398-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030805.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.285	69	76	87	rVB	111912	122831	13.89%	1.789%
2	1.539	148	155	165	rBV	107093	124908	14.13%	1.820%
3	2.066	310	319	337	rVB	221751	321159	36.33%	4.678%
4	2.297	390	391	396	rVB6	1271	874	0.10%	0.013%
5	2.381	415	417	422	rVB5	1728	1254	0.14%	0.018%
6	2.555	468	471	473	rBV4	1345	824	0.09%	0.012%
7	2.786	540	543	546	rBV5	1723	1086	0.12%	0.016%
8	2.969	596	600	602	rBV5	1359	1022	0.12%	0.015%
9	2.989	602	606	607	rVV3	1052	700	0.08%	0.010%
10	3.111	641	644	648	rBV5	1939	1854	0.21%	0.027%
11	3.188	663	668	672	rBV6	1793	2135	0.24%	0.031%
12	3.330	710	712	718	rBV6	1458	1391	0.16%	0.020%
13	3.391	726	731	734	rBV5	1305	1081	0.12%	0.016%
14	3.416	736	739	741	rBV4	1011	670	0.08%	0.010%
15	3.635	805	807	808	rBV2	1465	716	0.08%	0.010%
16	3.667	812	817	820	rBV6	1840	1507	0.17%	0.022%
17	3.747	837	842	843	rBV5	1737	1202	0.14%	0.018%
18	3.809	850	861	885	rBV2	51785	165458	18.72%	2.410%
19	4.111	953	955	959	rBV4	1980	1056	0.12%	0.015%
20	4.262	989	1002	1019	rVB2	140276	345344	39.07%	5.031%
21	4.558	1091	1094	1096	rBV4	1666	897	0.10%	0.013%
22	4.638	1117	1119	1124	rVB5	2017	1524	0.17%	0.022%
23	4.712	1140	1142	1145	rVB4	1068	683	0.08%	0.010%
24	4.783	1160	1164	1168	rBV6	1626	1316	0.15%	0.019%
25	4.876	1191	1193	1196	rVB3	2040	1043	0.12%	0.015%
26	4.902	1196	1201	1202	rBV5	1041	755	0.09%	0.011%
27	4.966	1204	1221	1242	rBV2	332558	884005	100.00%	12.877%
28	5.259	1309	1312	1315	rBV4	1670	1016	0.11%	0.015%
29	5.542	1388	1400	1422	rBV	276017	575593	65.11%	8.385%
30	5.915	1514	1516	1520	rVB5	1294	830	0.09%	0.012%
31	5.998	1526	1542	1563	rBV	198927	414555	46.90%	6.039%
32	6.262	1621	1624	1625	rBV3	1253	703	0.08%	0.010%
33	6.362	1650	1655	1658	rBV6	1933	1476	0.17%	0.022%
34	6.413	1669	1671	1675	rBV5	980	689	0.08%	0.010%
35	6.471	1685	1689	1690	rBV4	1568	1083	0.12%	0.016%
36	6.513	1698	1702	1705	rBV4	1057	708	0.08%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042423\
 Data File : VW030805.D
 Acq On : 24 Apr 2023 20:09
 Operator : SY/MD
 Sample : 02398-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	6.558	1713	1716	1718	rBV4	1495	908	0.10%	0.013%
38	6.683	1753	1755	1759	rBV6	978	718	0.08%	0.010%
39	6.786	1786	1787	1792	rVB4	1237	620	0.07%	0.009%
40	6.841	1802	1804	1813	rVB9	1574	1826	0.21%	0.027%
41	6.921	1817	1829	1848	rBV	100519	195665	22.13%	2.850%
42	7.252	1920	1932	1961	rBV	381401	685640	77.56%	9.988%
43	7.561	2016	2028	2052	rBV	76046	145176	16.42%	2.115%
44	7.741	2082	2084	2087	rBV4	1701	943	0.11%	0.014%
45	7.796	2095	2101	2104	rBV7	1920	1839	0.21%	0.027%
46	7.841	2113	2115	2120	rVB6	1696	1392	0.16%	0.020%
47	7.866	2120	2123	2126	rBV4	1297	1052	0.12%	0.015%
48	8.037	2166	2176	2205	rBV	169530	364592	41.24%	5.311%
49	8.336	2266	2269	2270	rBV3	1330	697	0.08%	0.010%
50	8.506	2320	2322	2325	rBV4	1079	706	0.08%	0.010%
51	8.587	2342	2347	2350	rBV6	1480	1260	0.14%	0.018%
52	8.657	2367	2369	2374	rBV4	1685	821	0.09%	0.012%
53	8.792	2400	2411	2435	rBV	423213	710035	80.32%	10.343%
54	9.381	2592	2594	2596	rVB3	1455	688	0.08%	0.010%
55	9.394	2596	2598	2601	rBV3	1079	785	0.09%	0.011%
56	9.413	2601	2604	2606	rBV4	1060	657	0.07%	0.010%
57	9.519	2635	2637	2639	rBV3	1520	946	0.11%	0.014%
58	9.596	2659	2661	2665	rBV3	846	690	0.08%	0.010%
59	9.677	2683	2686	2690	rBV4	1026	864	0.10%	0.013%
60	9.705	2693	2695	2700	rBV6	955	651	0.07%	0.009%
61	9.805	2723	2726	2728	rBV4	913	648	0.07%	0.009%
62	9.918	2759	2761	2762	rBV2	1274	631	0.07%	0.009%
63	9.959	2771	2774	2776	rBV3	1755	1129	0.13%	0.016%
64	10.159	2825	2836	2858	rBV	270378	430547	48.70%	6.272%
65	10.467	2925	2932	2934	rBV7	1824	1814	0.21%	0.026%
66	10.789	3029	3032	3034	rBV3	1889	1075	0.12%	0.016%
67	10.802	3034	3036	3041	rVB4	1312	1007	0.11%	0.015%
68	10.853	3049	3052	3055	rBV4	1548	1308	0.15%	0.019%
69	11.037	3104	3109	3111	rBV6	1046	1130	0.13%	0.016%
70	11.049	3111	3113	3119	rVB7	1536	1137	0.13%	0.017%
71	11.094	3125	3127	3129	rBV3	1343	651	0.07%	0.009%
72	11.194	3146	3158	3181	rBV	408517	660443	74.71%	9.621%
73	11.567	3264	3274	3293	rVB	395819	631146	71.40%	9.194%
74	11.766	3334	3336	3340	rBV4	980	663	0.07%	0.010%
75	11.940	3387	3390	3391	rBV2	1229	673	0.08%	0.010%
76	12.094	3435	3438	3441	rBV5	752	637	0.07%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
 Data File : VV030805.D
 Acq On : 24 Apr 2023 20:09
 Operator : SY/MD
 Sample : 02398-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	12.403	3531	3534	3535	rBV3	1487	759	0.09%	0.011%
78	12.487	3558	3560	3565	rVB6	1512	1234	0.14%	0.018%
79	12.516	3565	3569	3573	rBV6	2030	1701	0.19%	0.025%
80	12.545	3573	3578	3582	rBV5	1058	1238	0.14%	0.018%
81	12.612	3596	3599	3600	rBV3	1661	1063	0.12%	0.015%
82	12.760	3641	3645	3646	rBV4	1178	866	0.10%	0.013%
83	12.873	3678	3680	3682	rBV3	993	647	0.07%	0.009%
84	13.107	3750	3753	3755	rBV4	980	718	0.08%	0.010%
85	13.162	3768	3770	3773	rBV3	822	604	0.07%	0.009%
86	13.265	3799	3802	3804	rBV3	1687	904	0.10%	0.013%
87	13.686	3931	3933	3945	rVB10	2586	3338	0.38%	0.049%
88	13.750	3951	3953	3957	rVB4	1493	785	0.09%	0.011%
89	13.773	3957	3960	3963	rBV5	2050	1438	0.16%	0.021%
90	13.898	3998	3999	4001	rVB2	1865	626	0.07%	0.009%
91	13.914	4001	4004	4010	rVB7	2045	1602	0.18%	0.023%
92	13.953	4010	4016	4018	rBV7	1807	1439	0.16%	0.021%
93	14.085	4052	4057	4058	rBV4	2066	1413	0.16%	0.021%
94	14.200	4089	4093	4094	rBV4	1176	733	0.08%	0.011%
95	14.268	4112	4114	4118	rBV5	1380	946	0.11%	0.014%
96	14.557	4202	4204	4205	rBV2	1883	699	0.08%	0.010%
97	14.609	4214	4220	4221	rBV5	1512	1316	0.15%	0.019%
98	14.699	4246	4248	4250	rBV3	1444	822	0.09%	0.012%
99	14.930	4317	4320	4321	rBV3	1707	949	0.11%	0.014%
100	15.098	4369	4372	4375	rBV4	1681	1315	0.15%	0.019%




Sum of corrected areas: 6864913

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
Data File : VV030805.D
Acq On : 24 Apr 2023 20:09
Operator : SY/MD
Sample : 02398-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

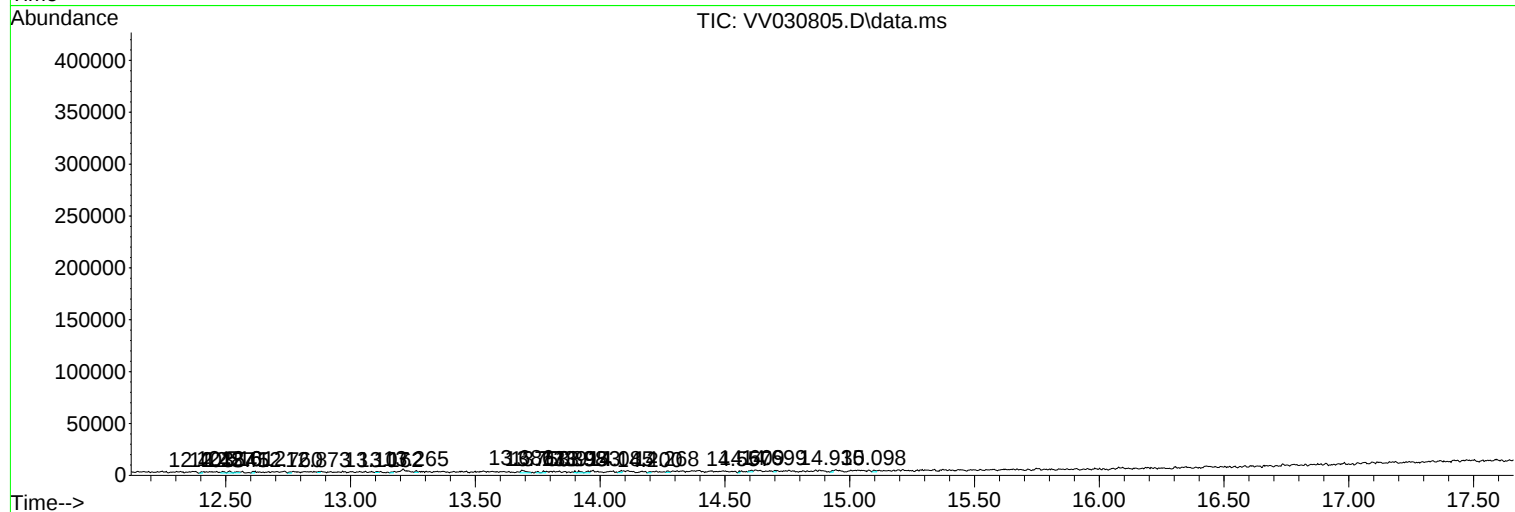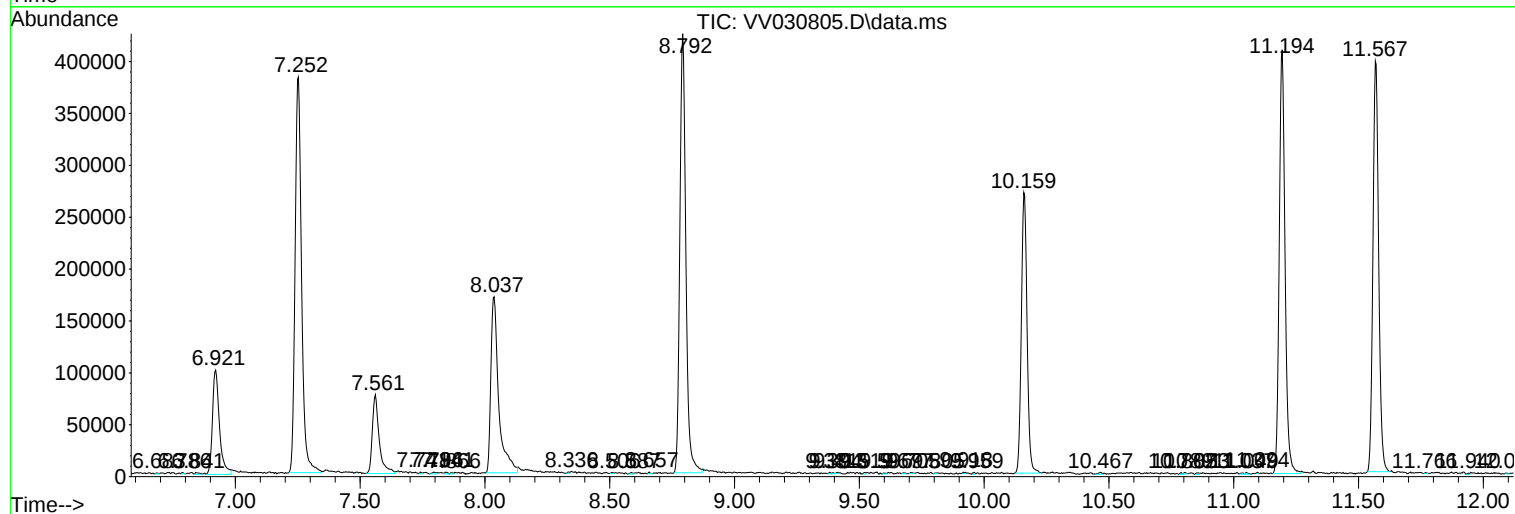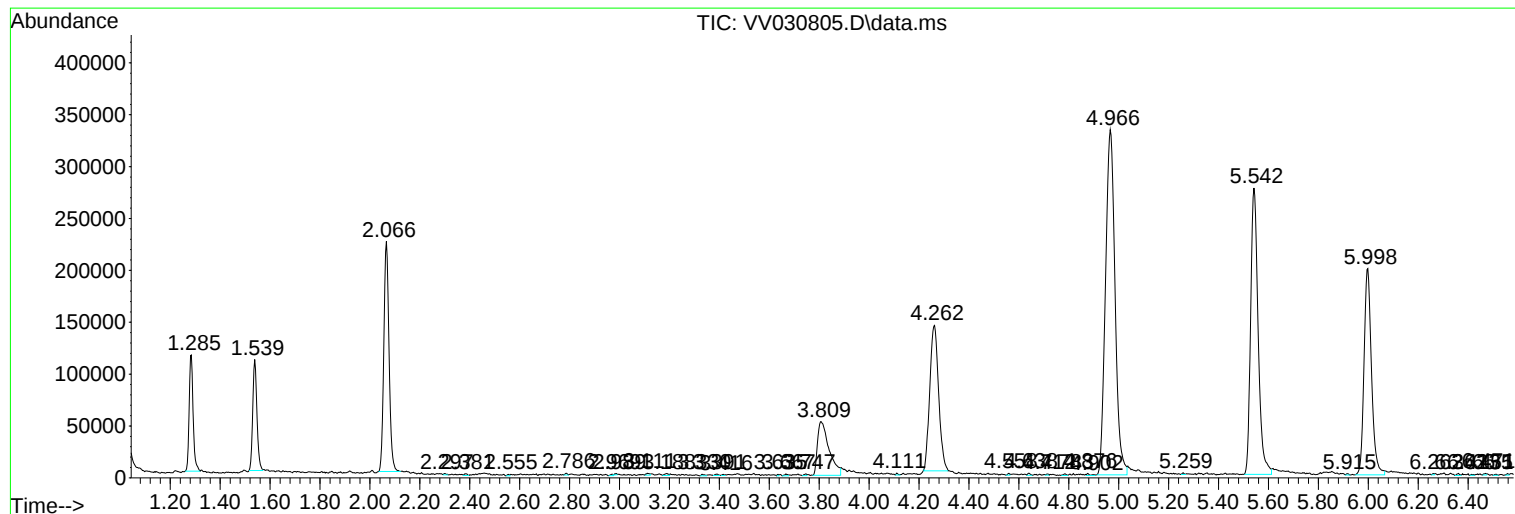

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
Data File : VV030805.D
Acq On : 24 Apr 2023 20:09
Operator : SY/MD
Sample : 02398-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
Data File : VV030805.D
Acq On : 24 Apr 2023 20:09
Operator : SY/MD
Sample : 02398-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------