

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
 Data File : VV030806.D
 Acq On : 24 Apr 2023 20:33
 Operator : SY/MD
 Sample : 02440-19
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030806.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	69	75	86	rBV	110665	120765	13.82%	1.797%
2	1.539	148	155	166	rVB	109230	123606	14.14%	1.839%
3	2.066	310	319	334	rBV	213250	308504	35.29%	4.591%
4	2.211	362	364	368	rBV5	1834	1389	0.16%	0.021%
5	2.397	420	422	423	rBV	1387	650	0.07%	0.010%
6	2.429	430	432	434	rBV3	1326	502	0.06%	0.007%
7	2.519	458	460	464	rBV5	906	579	0.07%	0.009%
8	2.597	482	484	487	rBV3	750	516	0.06%	0.008%
9	2.658	501	503	505	rBV3	1453	812	0.09%	0.012%
10	2.770	536	538	541	rBV4	906	477	0.05%	0.007%
11	2.790	541	544	549	rBV7	984	894	0.10%	0.013%
12	2.896	574	577	579	rBV5	1314	889	0.10%	0.013%
13	3.040	620	622	625	rBV4	799	457	0.05%	0.007%
14	3.137	649	652	655	rBV4	1419	1108	0.13%	0.016%
15	3.163	659	660	664	rVB3	1354	527	0.06%	0.008%
16	3.191	664	669	670	rBV4	1239	790	0.09%	0.012%
17	3.211	670	675	680	rBV7	1379	1735	0.20%	0.026%
18	3.246	684	686	688	rVB3	1100	423	0.05%	0.006%
19	3.262	688	691	695	rBV6	1523	1189	0.14%	0.018%
20	3.397	730	733	739	rBV6	1679	1692	0.19%	0.025%
21	3.507	763	767	772	rBV7	1370	1434	0.16%	0.021%
22	3.564	782	785	788	rBV5	1461	1049	0.12%	0.016%
23	3.648	807	811	814	rBV6	1127	995	0.11%	0.015%
24	3.664	814	816	817	rBV2	1495	520	0.06%	0.008%
25	3.722	832	834	836	rBV3	1055	575	0.07%	0.009%
26	3.806	850	860	882	rBV	53835	151741	17.36%	2.258%
27	4.259	986	1001	1020	rBV	140106	354822	40.59%	5.280%
28	4.532	1083	1086	1089	rVB6	2242	1346	0.15%	0.020%
29	4.683	1128	1133	1138	rBV8	1835	1950	0.22%	0.029%
30	4.783	1160	1164	1171	rVB10	1819	2111	0.24%	0.031%
31	4.889	1194	1197	1198	rBV3	1743	877	0.10%	0.013%
32	4.966	1201	1221	1242	rBV2	326242	874111	100.00%	13.007%
33	5.542	1388	1400	1423	rBV	270098	561105	64.19%	8.350%
34	5.928	1519	1520	1523	rBV2	1083	454	0.05%	0.007%
35	5.998	1530	1542	1567	rVB	189988	398063	45.54%	5.924%
36	6.352	1649	1652	1655	rBV5	1110	779	0.09%	0.012%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
 Data File : VV030806.D
 Acq On : 24 Apr 2023 20:33
 Operator : SY/MD
 Sample : 02440-19
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	6.384	1661	1662	1667	rVB5	1287	628	0.07%	0.009%
38	6.503	1694	1699	1702	rBV6	1178	1134	0.13%	0.017%
39	6.548	1710	1713	1716	rBV5	1153	1056	0.12%	0.016%
40	6.584	1722	1724	1727	rBV4	1154	750	0.09%	0.011%
41	6.741	1768	1773	1774	rBV5	1167	982	0.11%	0.015%
42	6.786	1784	1787	1790	rBV3	1102	813	0.09%	0.012%
43	6.812	1790	1795	1796	rBV5	1475	1296	0.15%	0.019%
44	6.860	1808	1810	1813	rBV4	1036	684	0.08%	0.010%
45	6.921	1818	1829	1846	rBV	98145	185537	21.23%	2.761%
46	7.252	1920	1932	1950	rBV	374391	668305	76.46%	9.945%
47	7.558	2019	2027	2044	rBV	70852	130504	14.93%	1.942%
48	7.815	2105	2107	2110	rVB4	1533	728	0.08%	0.011%
49	7.873	2122	2125	2129	rVB5	1347	1123	0.13%	0.017%
50	7.895	2129	2132	2133	rBV3	974	490	0.06%	0.007%
51	8.034	2165	2175	2201	rBV	169713	359308	41.11%	5.347%
52	8.558	2334	2338	2340	rBV3	1408	1104	0.13%	0.016%
53	8.793	2399	2411	2434	rBV	411031	701367	80.24%	10.437%
54	8.982	2468	2470	2471	rBV2	1079	430	0.05%	0.006%
55	9.030	2483	2485	2486	rBV2	1294	519	0.06%	0.008%
56	9.227	2542	2546	2547	rBV3	951	659	0.08%	0.010%
57	9.265	2556	2558	2561	rBV4	1273	618	0.07%	0.009%
58	9.722	2695	2700	2702	rBV6	1099	872	0.10%	0.013%
59	9.780	2716	2718	2720	rBV3	787	415	0.05%	0.006%
60	9.815	2728	2729	2731	rBV2	1013	436	0.05%	0.006%
61	9.831	2731	2734	2736	rVV5	1588	782	0.09%	0.012%
62	9.841	2736	2737	2740	rVB3	924	460	0.05%	0.007%
63	9.915	2758	2760	2763	rBV3	1166	608	0.07%	0.009%
64	10.104	2816	2819	2821	rBV4	1293	706	0.08%	0.011%
65	10.159	2821	2836	2855	rVV	264001	430914	49.30%	6.412%
66	10.323	2884	2887	2888	rBV3	1182	755	0.09%	0.011%
67	10.407	2909	2913	2914	rBV4	1095	730	0.08%	0.011%
68	10.474	2931	2934	2936	rBV4	1050	646	0.07%	0.010%
69	10.683	2998	2999	3001	rBV2	1174	487	0.06%	0.007%
70	10.783	3027	3030	3032	rBV4	1343	872	0.10%	0.013%
71	10.828	3038	3044	3046	rBV6	1659	1391	0.16%	0.021%
72	10.918	3070	3072	3075	rBV4	809	553	0.06%	0.008%
73	11.194	3146	3158	3177	rBV	411402	648151	74.15%	9.645%
74	11.407	3222	3224	3229	rVB6	1819	1380	0.16%	0.021%
75	11.519	3257	3259	3262	rBV4	1095	619	0.07%	0.009%
76	11.567	3262	3274	3291	rBV	387420	627404	71.78%	9.336%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
 Data File : VV030806.D
 Acq On : 24 Apr 2023 20:33
 Operator : SY/MD
 Sample : 02440-19
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	11.757	3330	3333	3336	rBV5	1319	1012	0.12%	0.015%
78	11.905	3377	3379	3381	rBV3	1166	614	0.07%	0.009%
79	12.001	3407	3409	3411	rBV3	971	511	0.06%	0.008%
80	12.088	3433	3436	3439	rBV4	1390	1374	0.16%	0.020%
81	12.394	3529	3531	3536	rVB5	1752	1010	0.12%	0.015%
82	12.606	3595	3597	3599	rVB3	1100	509	0.06%	0.008%
83	12.667	3613	3616	3620	rBV5	849	535	0.06%	0.008%
84	12.712	3628	3630	3633	rVB4	972	477	0.05%	0.007%
85	12.751	3639	3642	3644	rBV5	1170	822	0.09%	0.012%
86	12.773	3647	3649	3650	rBV2	1274	662	0.08%	0.010%
87	13.069	3739	3741	3746	rBV5	1580	1088	0.12%	0.016%
88	13.140	3760	3763	3767	rVV5	1588	1242	0.14%	0.018%
89	13.294	3806	3811	3816	rBV8	1909	1888	0.22%	0.028%
90	13.326	3818	3821	3822	rBV2	1660	829	0.09%	0.012%
91	13.509	3873	3878	3883	rBV6	2254	2807	0.32%	0.042%
92	13.741	3947	3950	3951	rBV3	1453	912	0.10%	0.014%
93	13.921	4004	4006	4009	rBV4	1804	1439	0.16%	0.021%
94	13.960	4017	4018	4021	rVB3	2026	728	0.08%	0.011%
95	13.982	4021	4025	4028	rBV6	1982	1546	0.18%	0.023%
96	14.114	4064	4066	4069	rVB4	1574	613	0.07%	0.009%
97	14.165	4079	4082	4086	rBV6	1206	1007	0.12%	0.015%
98	14.259	4108	4111	4114	rBV4	1281	990	0.11%	0.015%
99	14.969	4329	4332	4333	rBV3	1662	946	0.11%	0.014%
100	15.046	4354	4356	4358	rBV3	1541	845	0.10%	0.013%




Sum of corrected areas: 6720058

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
Data File : VV030806.D
Acq On : 24 Apr 2023 20:33
Operator : SY/MD
Sample : 02440-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

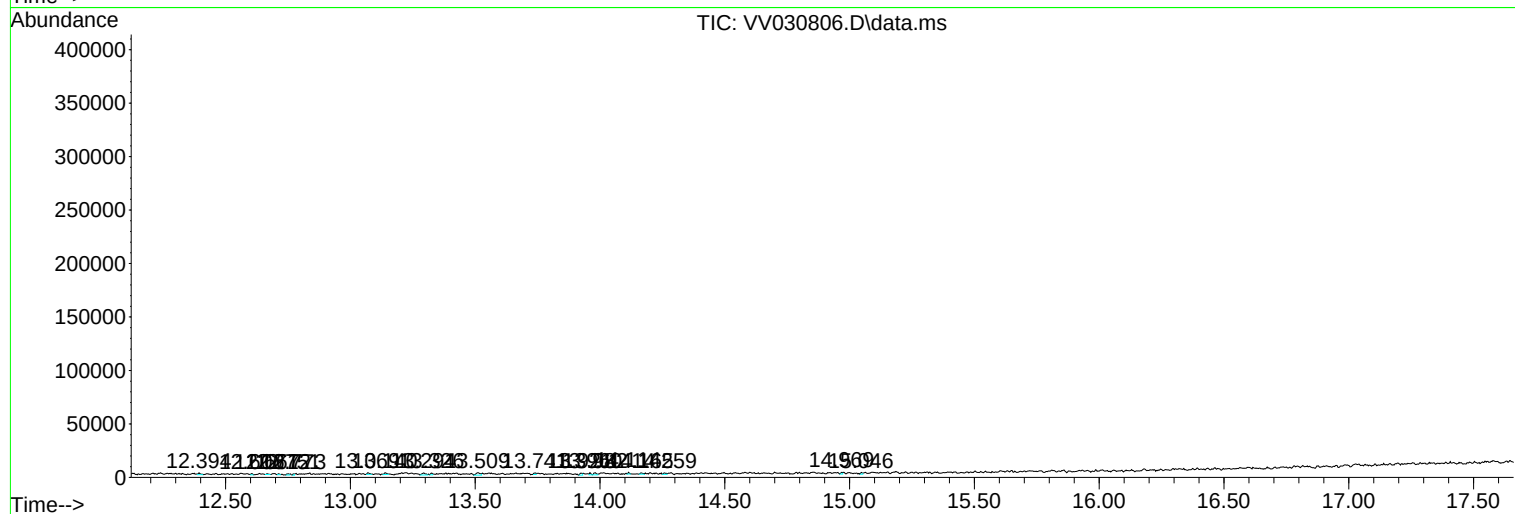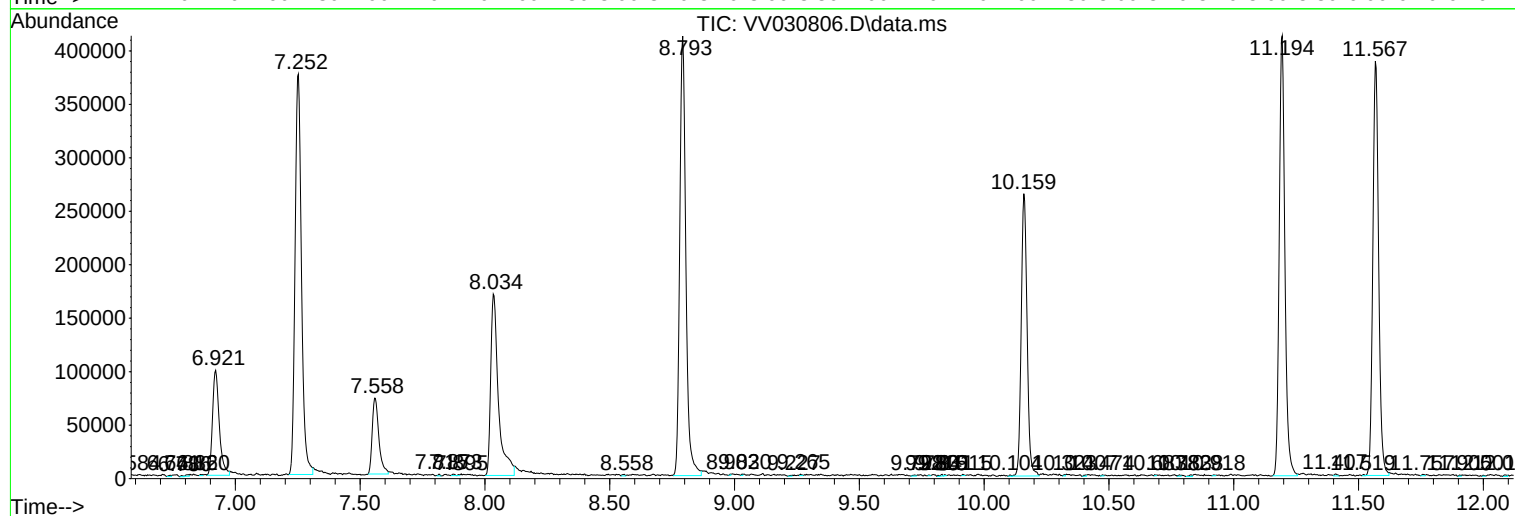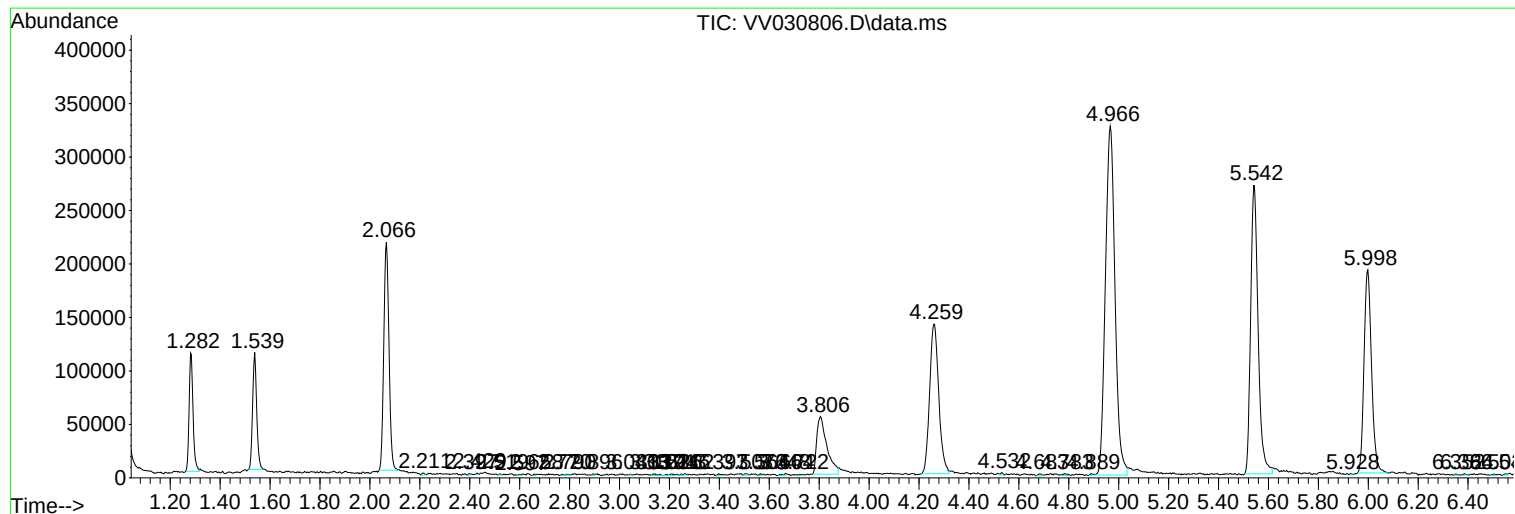

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
Data File : VV030806.D
Acq On : 24 Apr 2023 20:33
Operator : SY/MD
Sample : 02440-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
Data File : VV030806.D
Acq On : 24 Apr 2023 20:33
Operator : SY/MD
Sample : 02440-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc