

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
 Data File : VV030814.D
 Acq On : 25 Apr 2023 00:20
 Operator : SY/MD
 Sample : 02418-16ME
 Misc : 4.22g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW900ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030814.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.191	41	47	51	rBV	36414	35453	3.97%	0.508%
2	1.220	52	56	69	rVV	29499	37844	4.24%	0.542%
3	1.282	69	75	91	rVB	92454	115009	12.89%	1.647%
4	1.536	149	154	165	rVB	101687	114480	12.83%	1.640%
5	2.053	305	315	328	rBV	210880	316115	35.43%	4.528%
6	2.767	531	537	540	rBV8	1291	1348	0.15%	0.019%
7	2.783	540	542	545	rVB3	1978	1078	0.12%	0.015%
8	2.799	545	547	549	rBV3	1062	545	0.06%	0.008%
9	2.818	551	553	557	rVB4	1363	632	0.07%	0.009%
10	2.847	557	562	564	rBV4	1069	903	0.10%	0.013%
11	2.892	574	576	579	rBV5	841	298	0.03%	0.004%
12	2.953	591	595	596	rBV4	1461	814	0.09%	0.012%
13	3.092	633	638	640	rBV5	1128	812	0.09%	0.012%
14	3.130	647	650	653	rBV5	969	684	0.08%	0.010%
15	3.220	675	678	681	rVB5	1159	674	0.08%	0.010%
16	3.240	681	684	685	rBV3	473	240	0.03%	0.003%
17	3.278	694	696	700	rVB4	1982	1157	0.13%	0.017%
18	3.294	700	701	703	rBV	915	414	0.05%	0.006%
19	3.310	703	706	707	rBV2	737	471	0.05%	0.007%
20	3.404	730	735	737	rVB6	1070	797	0.09%	0.011%
21	3.490	761	762	765	rBV2	863	408	0.05%	0.006%
22	3.516	766	770	773	rVV5	1124	747	0.08%	0.011%
23	3.539	775	777	778	rBV2	611	197	0.02%	0.003%
24	3.574	786	788	789	rBV	837	319	0.04%	0.005%
25	3.635	802	807	808	rBV4	1480	1165	0.13%	0.017%
26	3.661	812	815	816	rBV2	459	248	0.03%	0.004%
27	3.670	816	818	819	rBV2	1551	596	0.07%	0.009%
28	3.722	829	834	837	rBV6	1533	1340	0.15%	0.019%
29	3.822	854	865	893	rBV2	32837	133142	14.92%	1.907%
30	4.259	988	1001	1021	rVB	137179	339998	38.11%	4.870%
31	4.516	1079	1081	1085	rVB5	1040	597	0.07%	0.009%
32	4.632	1115	1117	1118	rBV2	779	274	0.03%	0.004%
33	4.674	1128	1130	1131	rVB2	755	166	0.02%	0.002%
34	4.709	1140	1141	1143	rBV2	864	392	0.04%	0.006%
35	4.802	1168	1170	1171	rBV2	560	194	0.02%	0.003%
36	4.812	1171	1173	1176	rVB4	1060	638	0.07%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042423\
 Data File : VW030814.D
 Acq On : 25 Apr 2023 00:20
 Operator : SY/MD
 Sample : 02418-16ME
 Misc : 4.22g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW900ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	4.828	1176	1178	1179	rBV2	1067	578	0.06%	0.008%
38	4.854	1184	1186	1187	rBV3	711	292	0.03%	0.004%
39	4.963	1203	1220	1244	rBV3	348831	892236	100.00%	12.779%
40	5.268	1309	1315	1317	rBV7	2241	2418	0.27%	0.035%
41	5.542	1386	1400	1421	rBV	328642	690430	77.38%	9.889%
42	5.998	1530	1542	1564	rVB	188469	392979	44.04%	5.628%
43	6.278	1626	1629	1630	rBV3	1036	639	0.07%	0.009%
44	6.384	1660	1662	1664	rBV2	1246	634	0.07%	0.009%
45	6.539	1705	1710	1714	rBV6	1450	1635	0.18%	0.023%
46	6.793	1787	1789	1792	rBV3	1010	835	0.09%	0.012%
47	6.921	1816	1829	1850	rBV2	98643	202820	22.73%	2.905%
48	7.249	1919	1931	1949	rBV	386037	691074	77.45%	9.898%
49	7.561	2019	2028	2049	rBV	65941	142816	16.01%	2.045%
50	7.892	2129	2131	2135	rBV5	1226	1087	0.12%	0.016%
51	8.043	2169	2178	2180	rBV	57629	72730	8.15%	1.042%
52	8.645	2363	2365	2366	rBV2	1056	416	0.05%	0.006%
53	8.699	2380	2382	2385	rBV3	801	477	0.05%	0.007%
54	8.792	2400	2411	2435	rBV	473426	848302	95.08%	12.150%
55	9.204	2533	2539	2542	rBV6	1982	1934	0.22%	0.028%
56	9.255	2552	2555	2558	rBV5	1374	1357	0.15%	0.019%
57	9.317	2572	2574	2575	rBV	422	133	0.01%	0.002%
58	9.516	2633	2636	2638	rBV3	1693	1151	0.13%	0.016%
59	9.567	2649	2652	2654	rBV3	1801	925	0.10%	0.013%
60	9.609	2661	2665	2667	rBV4	1410	977	0.11%	0.014%
61	9.712	2694	2697	2698	rBV3	1281	754	0.08%	0.011%
62	9.860	2741	2743	2746	rVB4	1308	555	0.06%	0.008%
63	9.915	2758	2760	2761	rBV2	989	391	0.04%	0.006%
64	10.101	2816	2818	2819	rBV2	648	189	0.02%	0.003%
65	10.172	2828	2840	2856	rVB	222534	402239	45.08%	5.761%
66	10.374	2901	2903	2906	rBV2	1325	842	0.09%	0.012%
67	10.390	2906	2908	2911	rVV3	1645	957	0.11%	0.014%
68	10.603	2972	2974	2975	rBV2	1045	470	0.05%	0.007%
69	10.763	3020	3024	3025	rBV3	1331	973	0.11%	0.014%
70	10.947	3079	3081	3084	rVB4	1300	554	0.06%	0.008%
71	10.976	3086	3090	3092	rBV5	1638	1389	0.16%	0.020%
72	11.043	3108	3111	3112	rBV3	2913	1836	0.21%	0.026%
73	11.198	3147	3159	3176	rBV	528296	840531	94.21%	12.039%
74	11.574	3266	3276	3294	rVB	418940	669083	74.99%	9.583%
75	12.535	3573	3575	3580	rVB5	1773	1179	0.13%	0.017%
76	13.249	3795	3797	3802	rBV6	1349	994	0.11%	0.014%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
Data File : VV030814.D
Acq On : 25 Apr 2023 00:20
Operator : SY/MD
Sample : 02418-16ME
Misc : 4.22g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW900ME

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Title : VOC Analysis




Sum of corrected areas: 6982000

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
Data File : VV030814.D
Acq On : 25 Apr 2023 00:20
Operator : SY/MD
Sample : 02418-16ME
Misc : 4.22g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW900ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

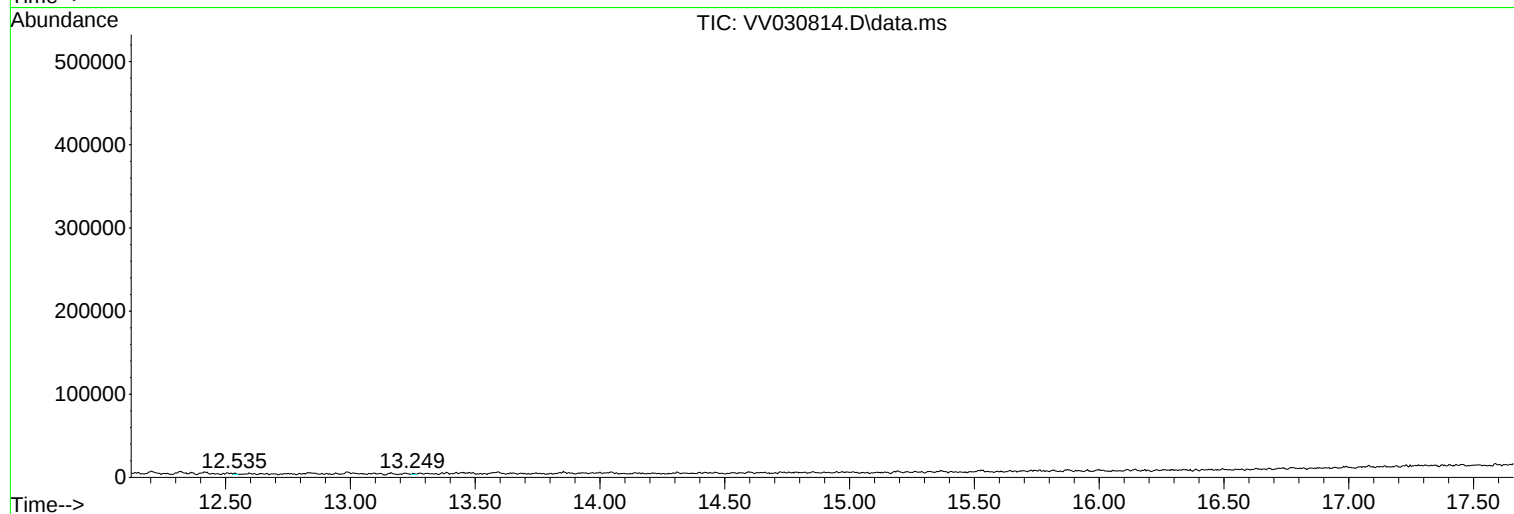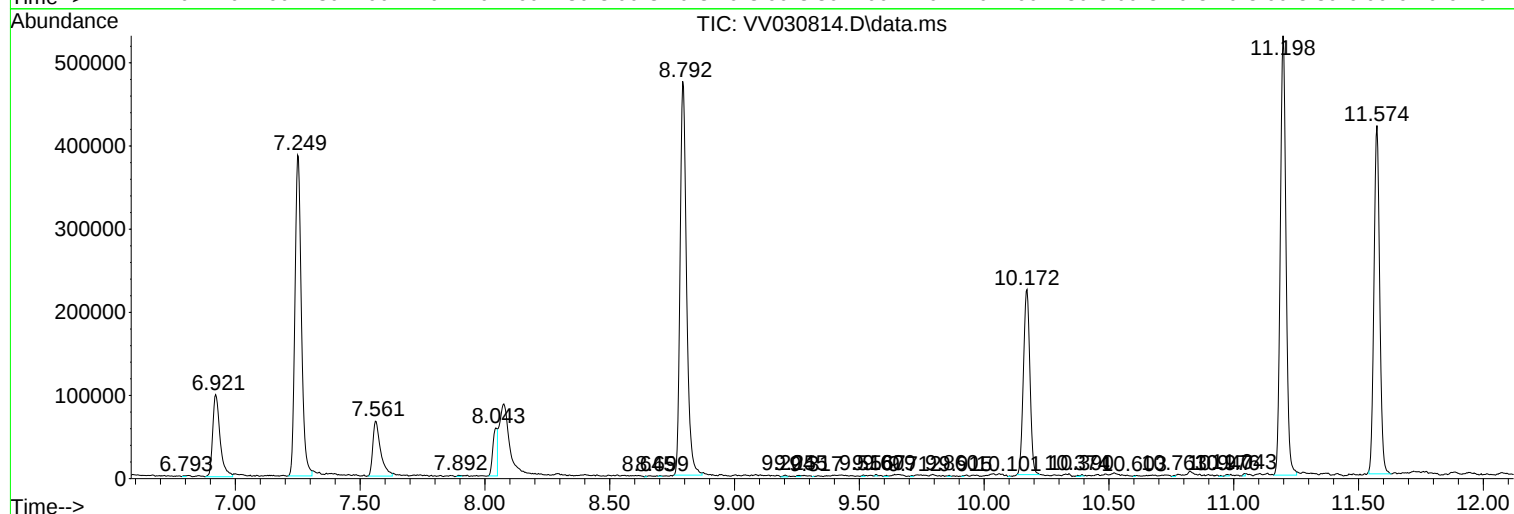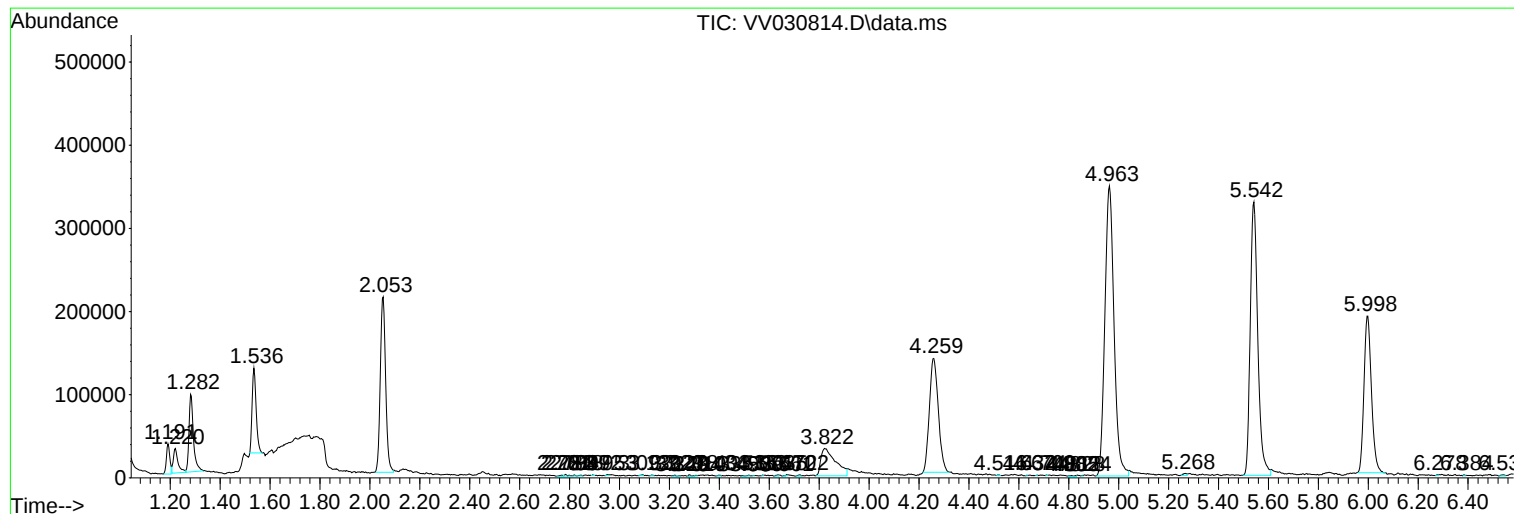

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
Data File : VV030814.D
Acq On : 25 Apr 2023 00:20
Operator : SY/MD
Sample : 02418-16ME
Misc : 4.22g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW900ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042423\
Data File : VV030814.D
Acq On : 25 Apr 2023 00:20
Operator : SY/MD
Sample : 02418-16ME
Misc : 4.22g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW900ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------