
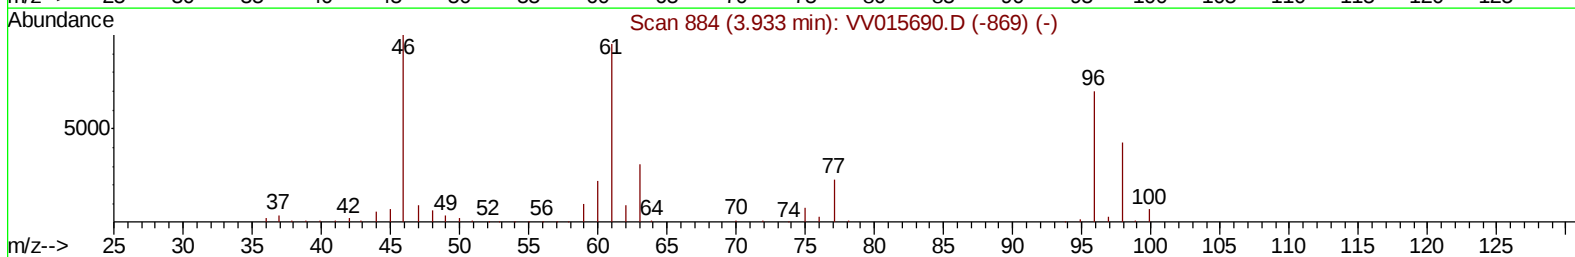
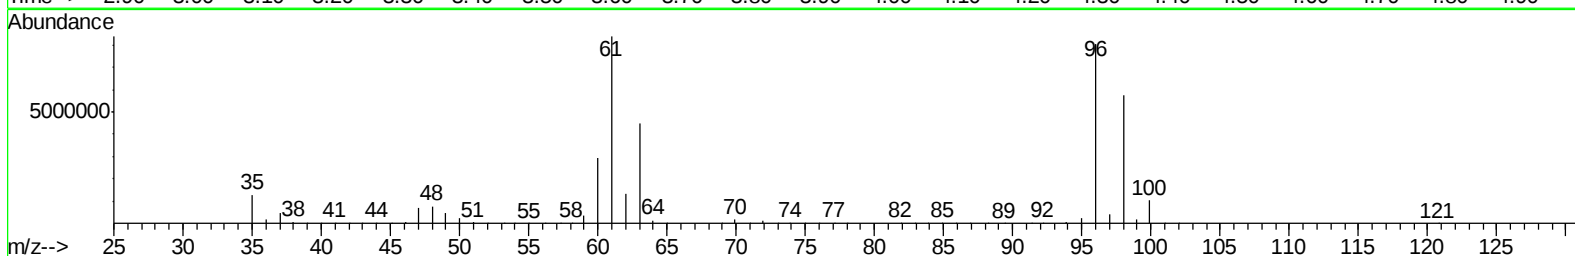


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV042520\
Data File : VV015706.D
Acq On : 25 Apr 2020 20:11
Operator : SY/MD
Sample : L2413-13
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Apr 27 01:17:42 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR042220WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Mon Apr 27 01:12:28 2020
Response via : Initial Calibration

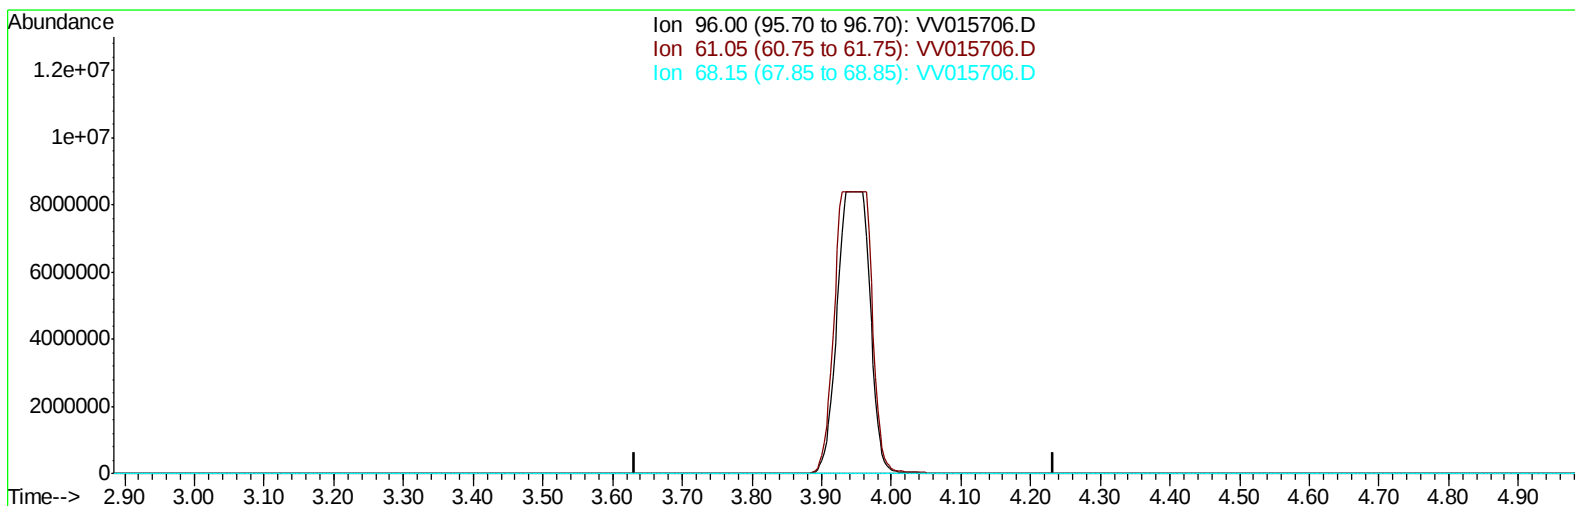

TIC: VV015706.D

(22) cis-1,2-Dichloroethene (T)

3.933min (-3.933) 0.00ug/L




response 0

Ion	Exp%	Act%
96.00	100	0.00
61.05	137.70	0.00#
68.15	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV042520\
 Data File : VV015706.D
 Acq On : 25 Apr 2020 20:11
 Operator : SY/MD
 Sample : L2413-13
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Apr 27 01:17:42 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR042220WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Mon Apr 27 01:12:28 2020
 Response via : Initial Calibration

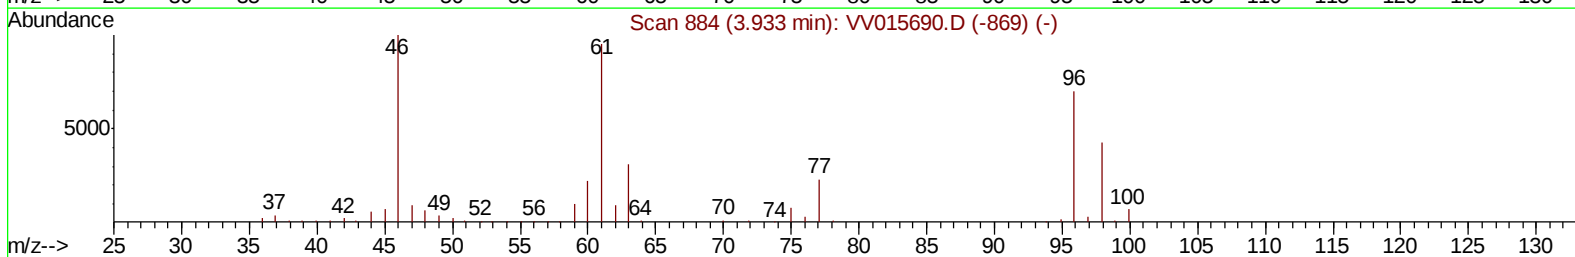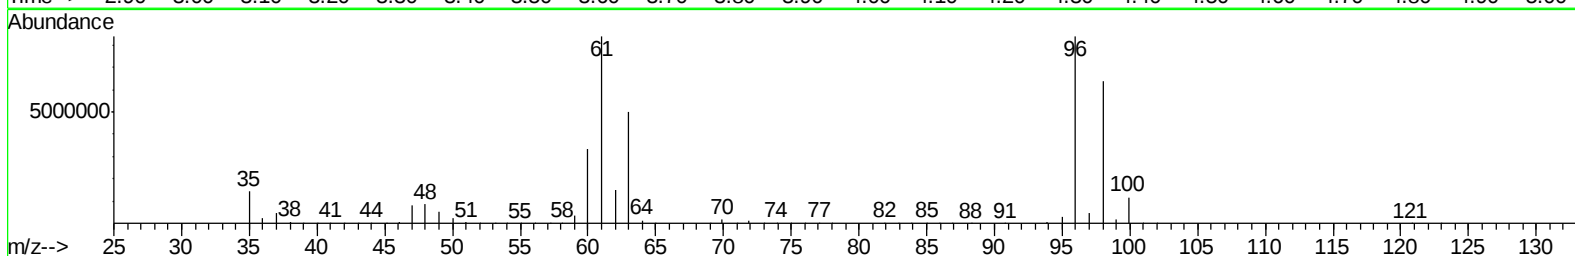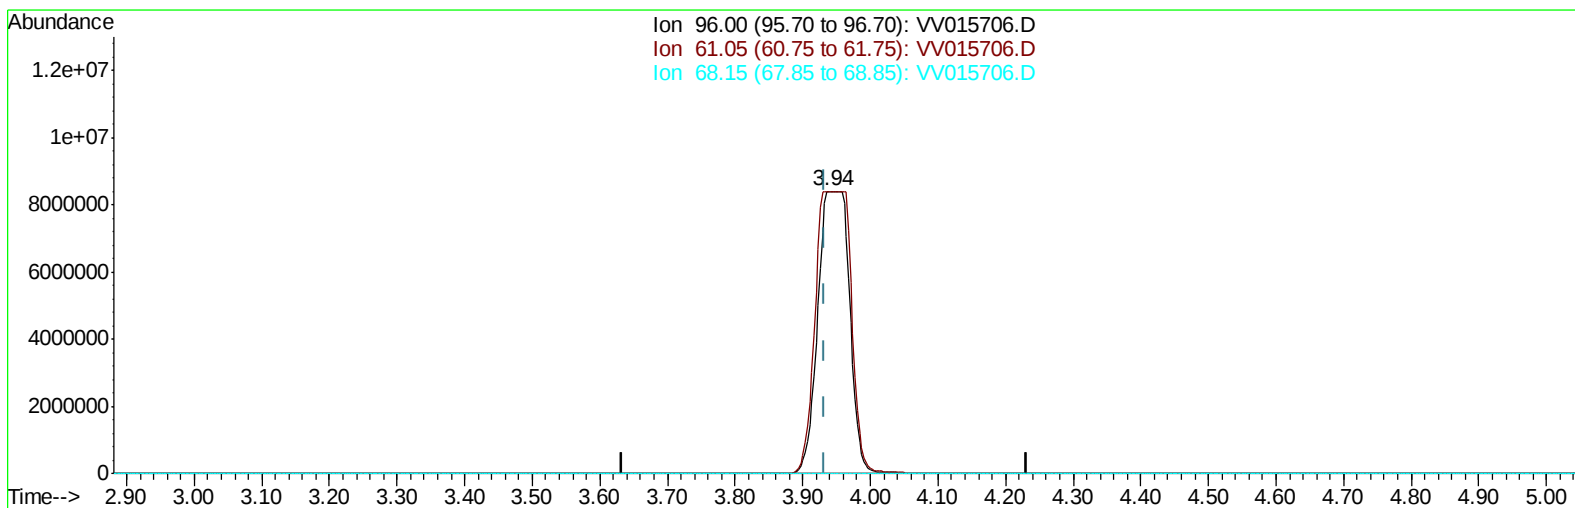

TIC: VV015706.D

(22) cis-1,2-Dichloroethene (T)

3.936min (+0.003) 2955.65ug/L m

response 27263060

Ion	Exp%	Act%
96.00	100	100
61.05	137.70	100.00
68.15	0.00	0.00
0.00	0.00	0.00