

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV042520\
 Data File : VV015696.D
 Acq On : 25 Apr 2020 15:55
 Operator : SY/MD
 Sample : L2413-02
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETKLO

Quant Time: Apr 27 02:41:36 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR042220WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Mon Apr 27 01:12:28 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	124439	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	122304	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	57312	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.31	65	25706	3.95	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	79.00%
7) Chloroethane-d5	1.57	69	26793	4.28	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	85.60%
11) 1,1-Dichloroethene-d2	2.11	63	42100	2.96	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	59.20%#
20) 2-Butanone-d5	3.94	46	101667	48.69	ug/L	0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	97.38%
24) Chloroform-d	4.38	84	66640	4.40	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.00%
26) 1,2-Dichloroethane-d4	5.06	65	40755	4.81	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.20%
32) Benzene-d6	5.07	84	128379	4.40	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.00%
36) 1,2-Dichloropropane-d6	6.09	67	42603	4.57	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	91.40%
41) Toluene-d8	7.34	98	114943	4.15	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	83.00%
43) trans-1,3-Dichloropropene-	7.65	79	11831	3.28	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	65.60%
46) 2-Hexanone-d5	8.11	63	73689	41.89	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	83.78%
57) 1,1,2,2-Tetrachloroethane-	10.24	84	30340	4.37	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	87.40%
64) 1,2-Dichlorobenzene-d4	11.65	152	45823	4.70	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	94.00%


Target Compounds				Ovalue
25) Chloroform	4.40	83	2796	0.165 ug/L 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV042520\
Data File : VV015696.D
Acq On : 25 Apr 2020 15:55
Operator : SY/MD
Sample : L2413-02
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETKL0

Quant Time: Apr 27 02:41:36 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR042220WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Mon Apr 27 01:12:28 2020
Response via : Initial Calibration

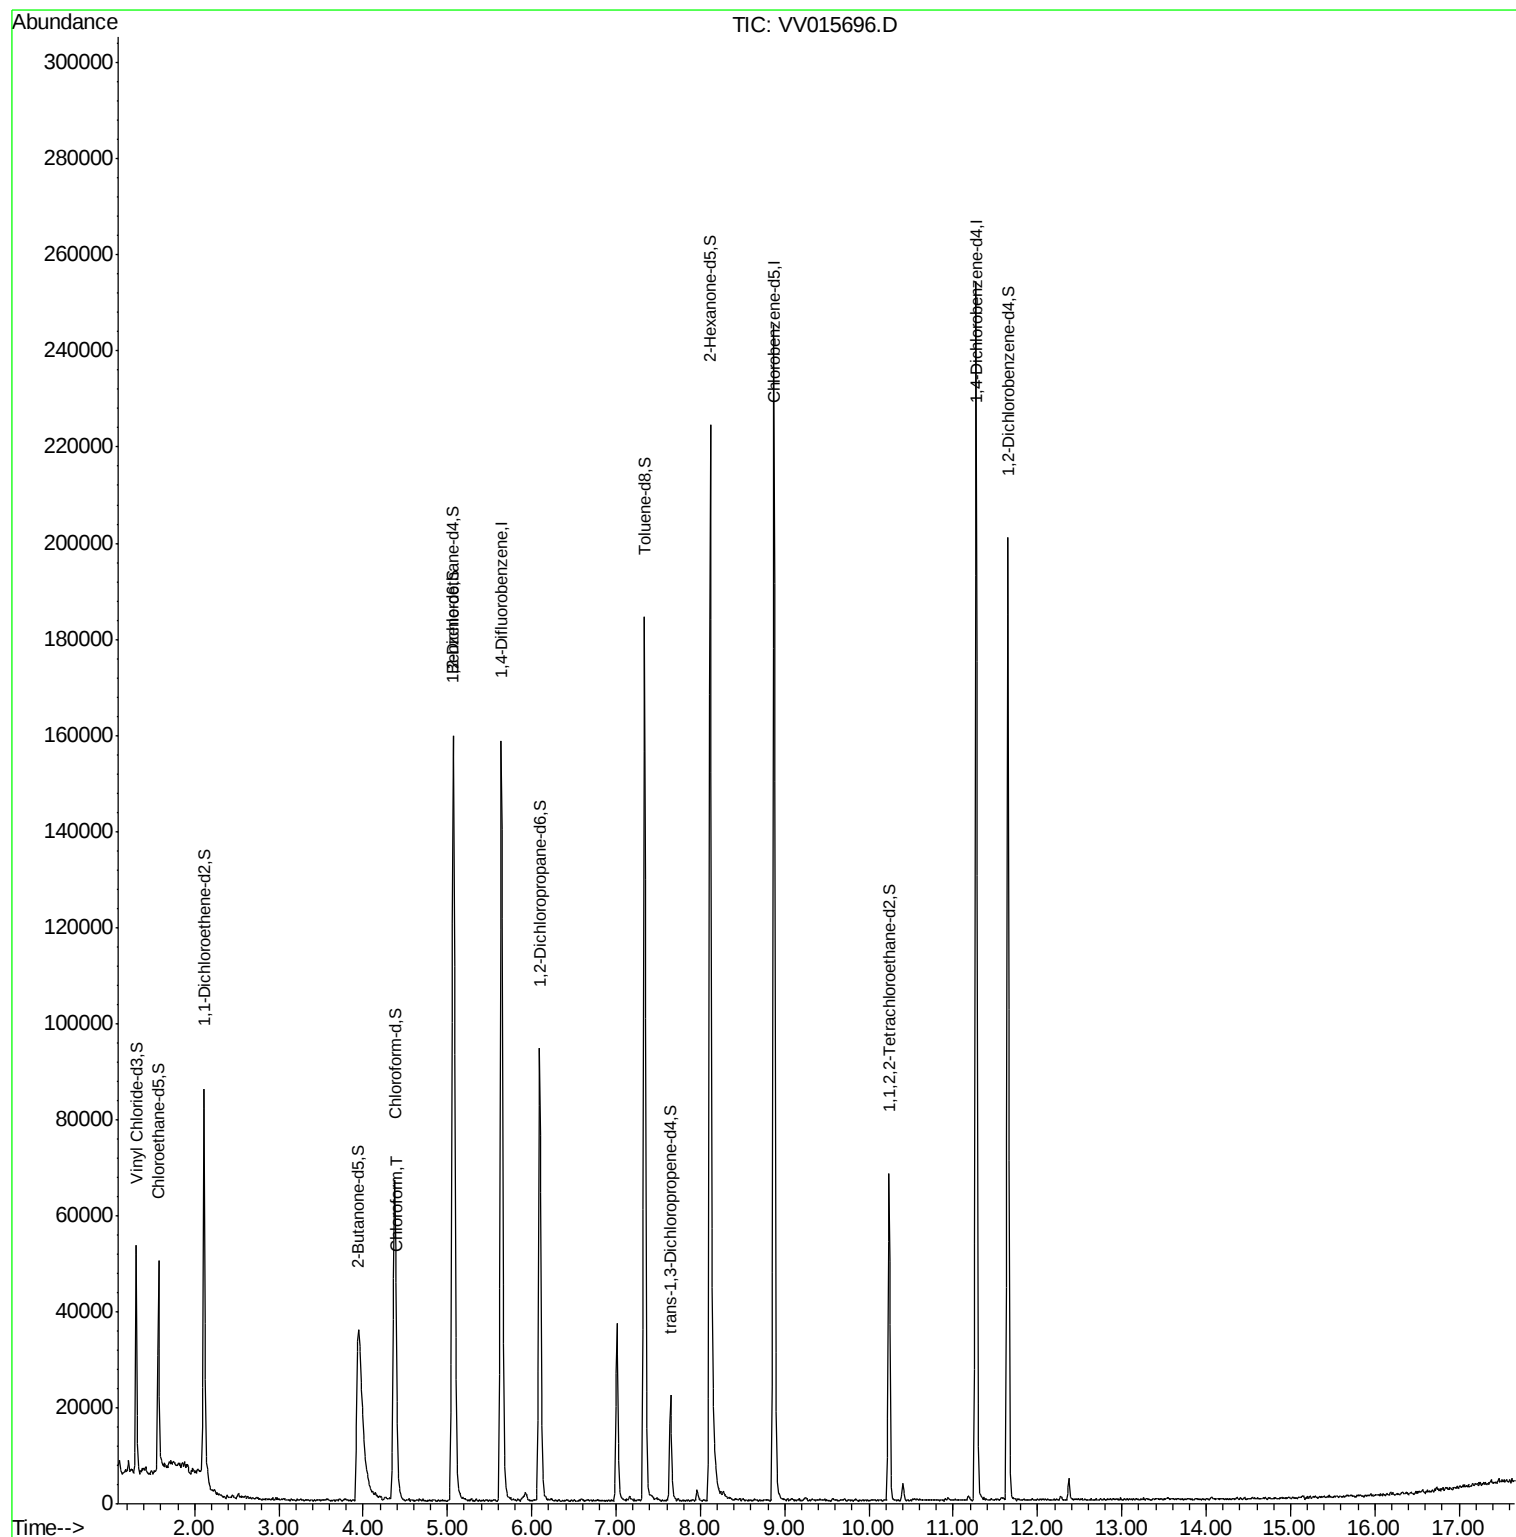

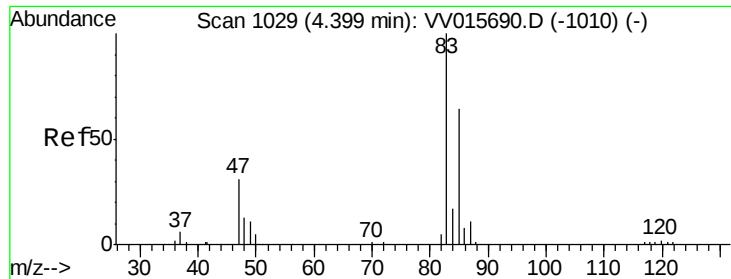

#25
 Chloroform
 Concen: 0.165 ug/L
 RT: 4.40 min Scan# 1030
 Delta R.T. 0.00 min
 Lab File: VV015696.D
 Acq: 25 Apr 2020 15:55

Instrument :
 MSVOA_V
 ClientSampleId :
 ETKL0

Tot Ion: 83 Resp: 2796
 Ion Ratio Lower Upper
 83 100
 85 68.7 46.1 85.5

