

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV042520\
 Data File : VV015705.D
 Acq On : 25 Apr 2020 19:47
 Operator : SY/MD
 Sample : L2413-12
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETKM1

Quant Time: Apr 27 04:14:40 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR042220WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Mon Apr 27 01:12:28 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	121607	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	120048	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	56590	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.31	65	25820	4.06	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	81.20%
7) Chloroethane-d5	1.58	69	28299	4.62	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	92.40%
11) 1,1-Dichloroethene-d2	2.12	63	44696	3.21	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	64.20%
20) 2-Butanone-d5	3.91	46	98973	48.50	ug/L	-0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	97.00%
24) Chloroform-d	4.38	84	70936	4.79	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.80%
26) 1,2-Dichloroethane-d4	5.06	65	42140	5.08	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	101.60%
32) Benzene-d6	5.08	84	133303	4.65	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.00%
36) 1,2-Dichloropropane-d6	6.09	67	43264	4.73	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	94.60%
41) Toluene-d8	7.34	98	118681	4.36	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	87.20%
43) trans-1,3-Dichloropropene-	7.65	79	10862	3.07	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	61.40%
46) 2-Hexanone-d5	8.11	63	75573	43.77	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	87.54%
57) 1,1,2,2-Tetrachloroethane-	10.24	84	31875	4.68	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	93.60%
64) 1,2-Dichlorobenzene-d4	11.65	152	47022	4.89	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	97.80%


Target Compounds					Ovalue
13) Acetone	2.19	43	1689	1.192 ug/L	93
22) cis-1,2-Dichloroethene	3.95	96	1171	0.134 ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV042520\
Data File : VV015705.D
Acq On : 25 Apr 2020 19:47
Operator : SY/MD
Sample : L2413-12
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETKM1

Quant Time: Apr 27 04:14:40 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR042220WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Mon Apr 27 01:12:28 2020
Response via : Initial Calibration

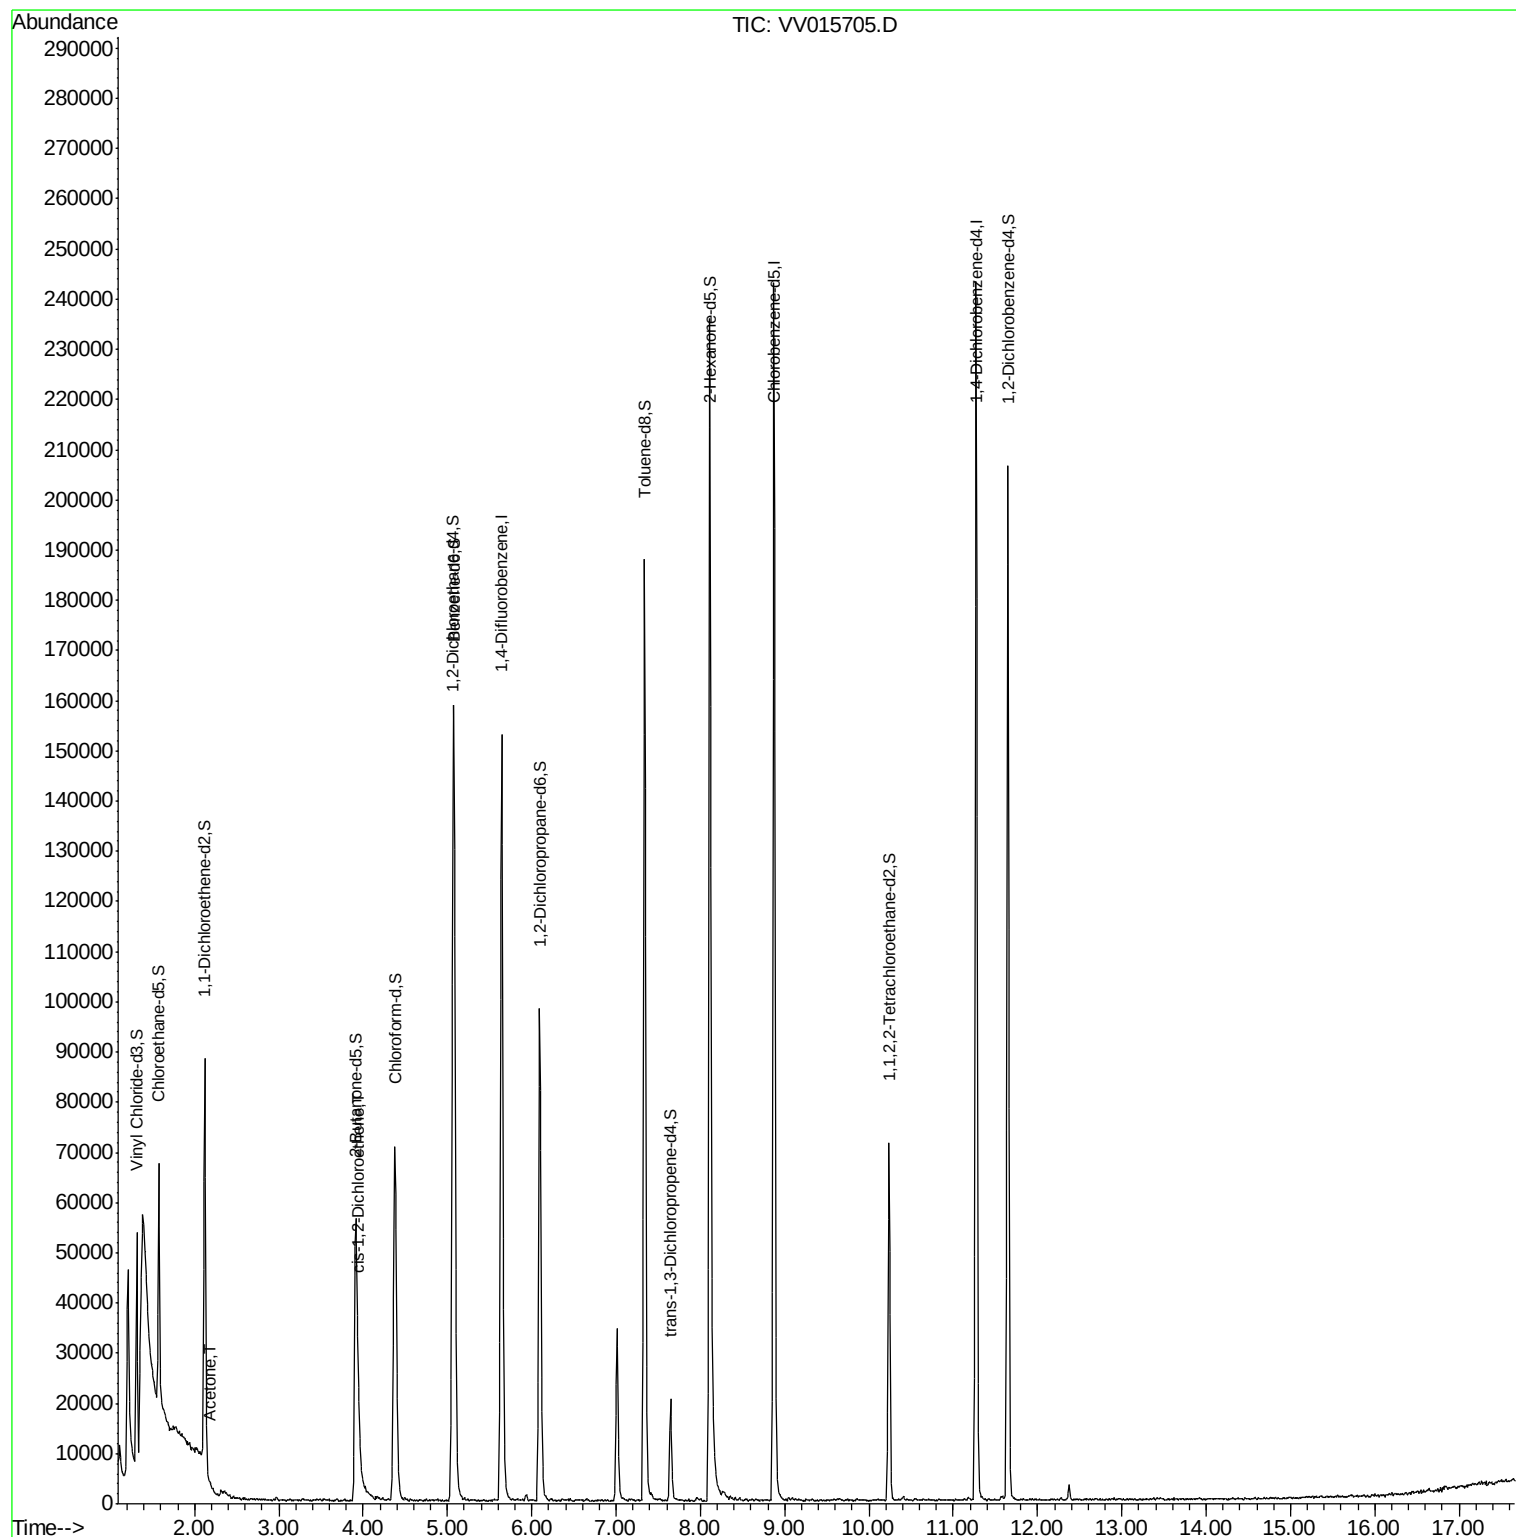

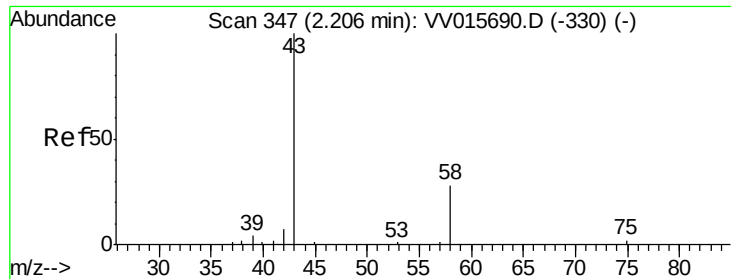

#13

Acetone

Concen: 1.192 ug/L

RT: 2.19 min Scan# 341

Delta R.T. -0.02 min

Lab File: VV015705.D

Acq: 25 Apr 2020 19:47

Instrument :

MSVOA_V

ClientSampled :





ETKM1

Tot Ion: 43 Resp: 1689

Ion Ratio Lower Upper

43 100

58 24.8 0.0 57.6

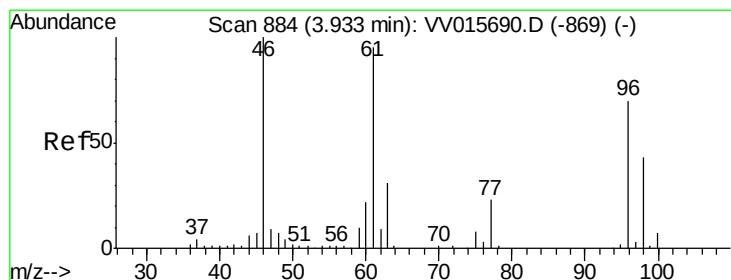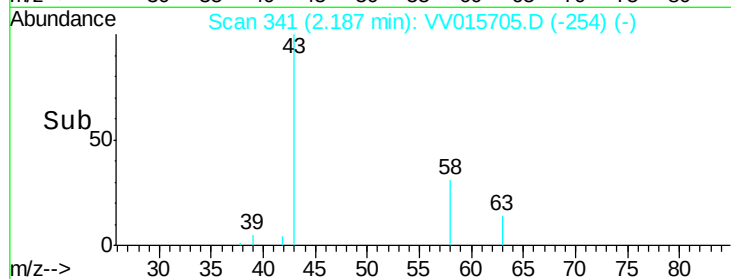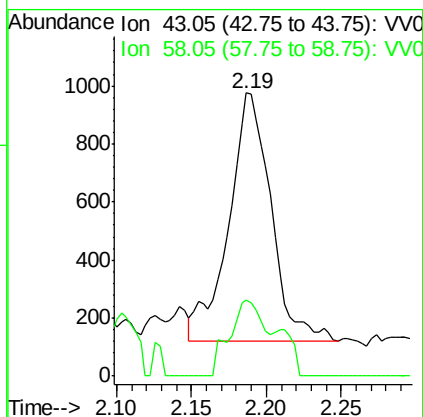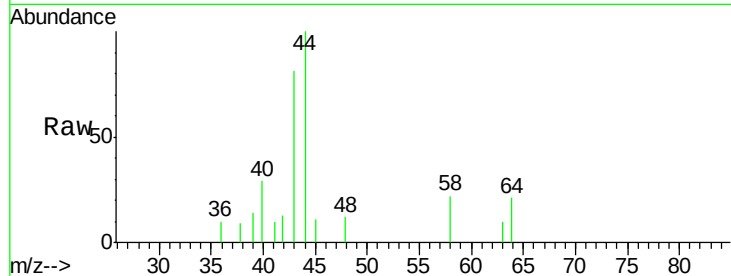

#22

cis-1,2-Dichloroethene

Concen: 0.134 ug/L

RT: 3.95 min Scan# 888

Delta R.T. 0.01 min

Lab File: VV015705.D

Acq: 25 Apr 2020 19:47

Tgt Ion: 96 Resp: 1171

Ion Ratio Lower Upper

96 100

61 142.2 96.4 179.0

68 0.0 0.0 0.0

