


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV042520\
 Data File : VV015689.D
 Acq On : 25 Apr 2020 12:06
 Operator : SY/MD
 Sample : BFB43
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB43

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR042220WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Mon Apr 27 01:12:28 2020

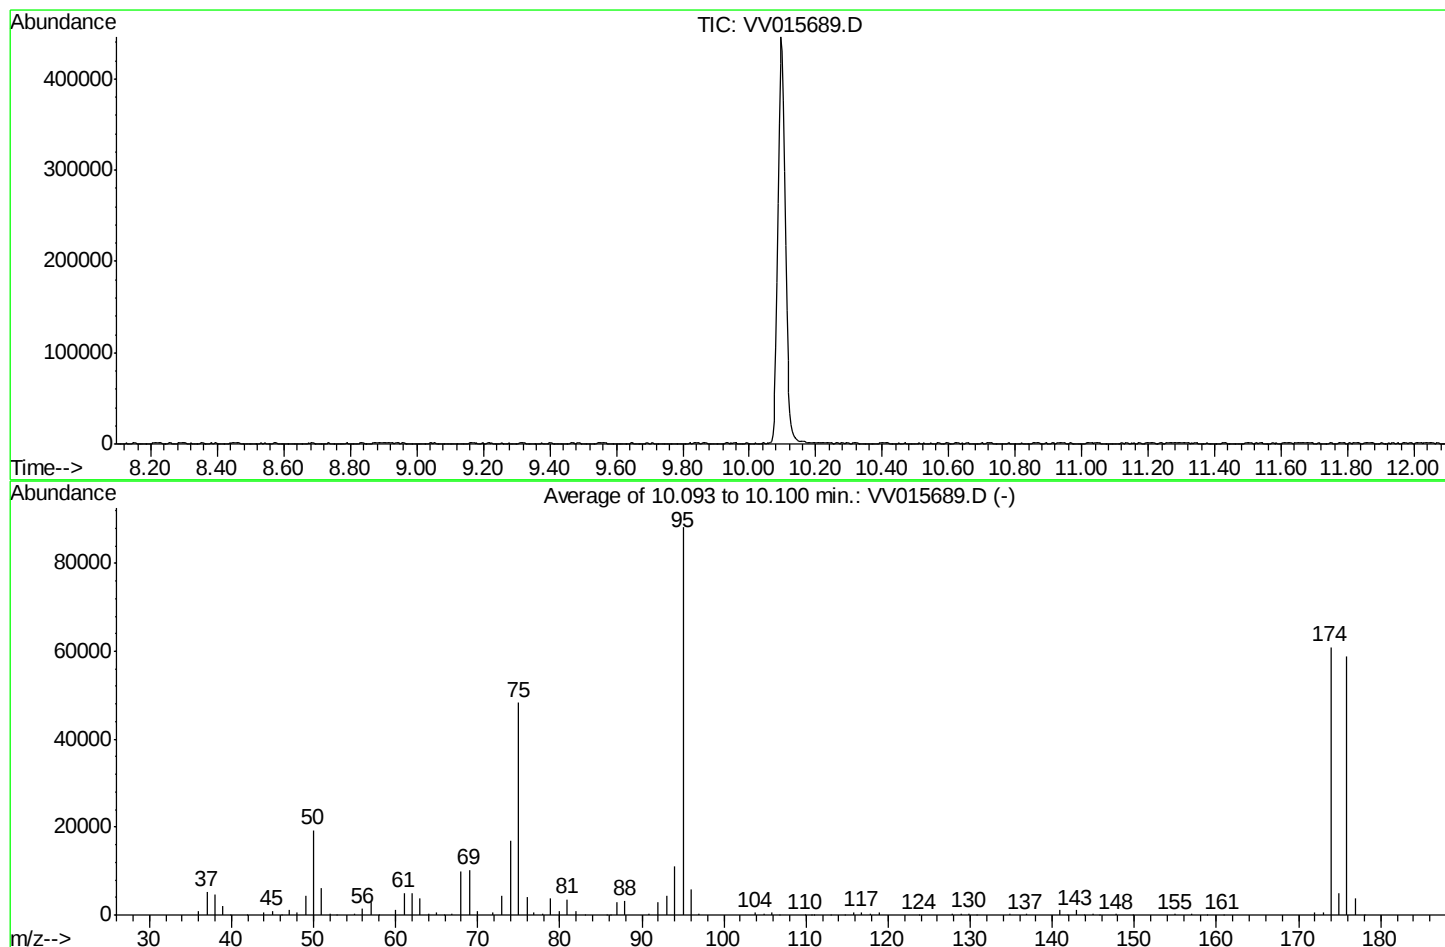

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2788

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.9	19349	PASS
75	95	30	80	54.7	48218	PASS
95	95	100	100	100.0	88202	PASS
96	95	5	9	6.6	5791	PASS
173	174	0.00	2	1.0	593	PASS
174	95	50	120	69.1	60989	PASS
175	174	5	9	8.0	4880	PASS
176	174	95	101	96.5	58853	PASS
177	176	5	9	6.3	3694	PASS

m/z	Abundance
36.00	903.0
37.00	5280.0
38.00	4548.0
39.00	2068.0
39.90	343.0
44.00	871.0
44.90	953.0
46.00	140.0
47.00	1034.0
47.90	627.0
49.00	4277.0
50.00	19312.0
51.00	5904.0
52.00	277.0
52.80	105.0
54.90	278.0
56.00	1366.0
57.00	2774.0
58.00	170.0
60.00	1005.0
61.00	5006.0
62.00	4955.0
63.00	3726.0
64.00	497.0
64.90	474.0
66.90	281.0
68.00	9712.0
69.00	10135.0
70.00	809.0
71.90	612.0
73.00	4428.0
74.00	16424.0
75.00	46568.0
76.00	4160.0
76.90	497.0
77.90	359.0
78.90	3622.0
79.90	984.0
80.90	3523.0
81.90	906.0
83.00	114.0
85.70	105.0
86.90	2986.0
88.00	3264.0
90.90	342.0
91.90	2717.0
93.00	4175.0
94.00	10769.0
95.00	86232.0
96.00	5890.0
97.00	142.0
103.90	580.0
104.90	182.0
105.80	465.0
110.70	117.0
114.80	106.0
115.80	478.0
116.80	687.0
117.90	397.0
118.90	562.0
123.80	119.0
127.80	335.0
128.80	149.0
129.80	326.0
130.90	120.0
134.90	161.0
136.80	181.0
140.90	999.0
141.90	155.0
142.90	1063.0
143.80	106.0
144.90	186.0
147.80	199.0
149.80	100.0
154.90	250.0
156.90	160.0
158.80	110.0
171.90	605.0
173.90	57872.0
174.90	4683.0
175.90	55240.0
177.00	3550.0
178.00	130.0

Instrument :
MSVOA_V
ClientSampleId :
BFB43

m/z	Abundance
36.00	967.0
37.00	5507.0
38.00	4709.0
39.00	2177.0
39.90	369.0
44.00	967.0
44.90	962.0
46.10	152.0
47.00	1073.0
47.90	597.0
49.00	4565.0
50.00	19944.0
51.00	6407.0
52.00	295.0
55.00	285.0
56.00	1477.0
57.00	2917.0
58.00	149.0
60.00	1156.0
61.00	5153.0
62.00	5106.0
63.00	4040.0
64.00	441.0
65.00	511.0
65.80	102.0
66.90	294.0
68.00	10165.0
69.00	10523.0
70.00	893.0
71.90	629.0
73.00	4588.0
74.00	17328.0
75.00	49952.0
76.00	4353.0
76.90	565.0
78.00	384.0
78.90	3886.0
79.90	1031.0
80.90	3761.0
81.90	938.0
83.00	147.0
86.90	3102.0
87.90	3389.0
90.90	343.0
92.00	3024.0
93.00	4586.0
94.00	11456.0
95.00	91288.0
96.00	5984.0
97.00	170.0
103.80	567.0
104.90	201.0
105.80	473.0
109.90	125.0
110.90	110.0
113.00	107.0
114.80	115.0
115.80	504.0
116.80	748.0
117.90	446.0
118.90	567.0
127.80	339.0
128.90	179.0
129.80	353.0
130.90	135.0
134.90	179.0
136.80	285.0
140.90	1119.0
141.90	152.0
142.90	1189.0
145.00	167.0
145.70	127.0
147.80	228.0
149.80	106.0
155.00	253.0
156.90	185.0
160.80	102.0
171.90	670.0
173.00	894.0
173.90	63008.0
174.90	5038.0
175.90	60736.0
176.90	3830.0
178.00	114.0

Instrument :
MSVOA_V
ClientSampleId :
BFB43

m/z	Abundance
36.00	962.0
37.00	5279.0
38.00	4495.0
39.00	2008.0
39.90	336.0
41.90	115.0
44.00	964.0
45.00	855.0
46.00	135.0
47.00	1004.0
48.00	574.0
49.00	4345.0
50.00	18792.0
51.00	6111.0
52.00	301.0
55.00	289.0
56.00	1483.0
57.00	2852.0
58.00	143.0
60.00	1091.0
61.00	4914.0
62.00	4765.0
63.00	3787.0
64.00	359.0
65.00	492.0
65.90	107.0
66.90	289.0
68.00	9476.0
69.00	9980.0
70.00	843.0
71.90	615.0
73.00	4362.0
74.00	16600.0
75.00	48136.0
76.00	4171.0
76.90	549.0
77.90	332.0
78.90	3665.0
79.90	1004.0
80.90	3628.0
81.90	878.0
83.00	140.0
86.20	140.0
86.90	3064.0
88.00	3254.0
90.90	334.0
92.00	2940.0
93.00	4396.0
94.00	11022.0
95.00	87088.0
96.00	5501.0
97.00	187.0
103.80	497.0
104.80	169.0
105.80	429.0
106.80	105.0
109.90	123.0
111.00	112.0
114.70	109.0
115.80	444.0
116.80	735.0
117.80	454.0
118.90	509.0
127.80	315.0
128.90	178.0
129.90	348.0
130.80	140.0
134.90	186.0
136.80	314.0
140.90	1079.0
141.90	142.0
142.90	1134.0
145.00	143.0
145.70	144.0
147.80	240.0
149.90	117.0
155.00	206.0
156.90	201.0
160.80	102.0
171.90	645.0
173.00	886.0
173.90	62088.0
174.90	4919.0
175.90	60584.0
176.90	3702.0

Instrument :
MSVOA_V
ClientSampleId :
BFB43

Scan 2788 (10.055 min): VV015689.D
BFB43

m/z	Abundance
39.00	107.0
39.90	307.0
43.90	399.0

Instrument :
MSVOA_V
ClientSampleId :
BFB43