

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042523\
 Data File : VW030832.D
 Acq On : 25 Apr 2023 13:17
 Operator : SY/MD
 Sample : 02418-09ME
 Misc : 4.16g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW8Z5ME

Quant Time: Apr 26 01:30:48 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Apr 22 00:43:23 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.542	114	210515	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.792	117	203113	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152	103597	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.281	65	66054	42.802	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	85.600%		
7) Chloroethane-d5	1.535	69	56950	44.037	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	88.080%		
11) 1,1-Dichloroethene-d2	2.066	65	33516	45.796	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	91.600%		
21) 2-Butanone-d5	3.796	46	96052	113.317	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	113.320%		
24) Chloroform-d	4.259	84	136418	48.778	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	97.560%		
26) 1,2-Dichloroethane-d4	4.950	65	101433	56.413	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	112.820%		
32) Benzene-d6	4.969	84	255307	53.165	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	106.320%		
36) 1,2-Dichloropropane-d6	5.998	67	79551	53.330	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	106.660%		
41) Toluene-d8	7.252	98	227317	50.417	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	100.840%		
43) trans-1,3-Dichloroprop...	7.561	79	36930	49.120	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	98.240%		
47) 2-Hexanone-d5	8.034	63	55205	93.945	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	93.950%		
56) 1,1,2,2-Tetrachloroeth...	10.159	84	112850	52.137	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	104.280%		
66) 1,2-Dichlorobenzene-d4	11.570	152	93482	56.771	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	113.540%		
Target Compounds						Qvalue
44) trans-1,3-Dichloropropene	7.558	75	2328	0.951	ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
Data File : VV030832.D
Acq On : 25 Apr 2023 13:17
Operator : SY/MD
Sample : 02418-09ME
Misc : 4.16g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW8Z5ME

Quant Time: Apr 26 01:30:48 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Apr 22 00:43:23 2023
Response via : Initial Calibration

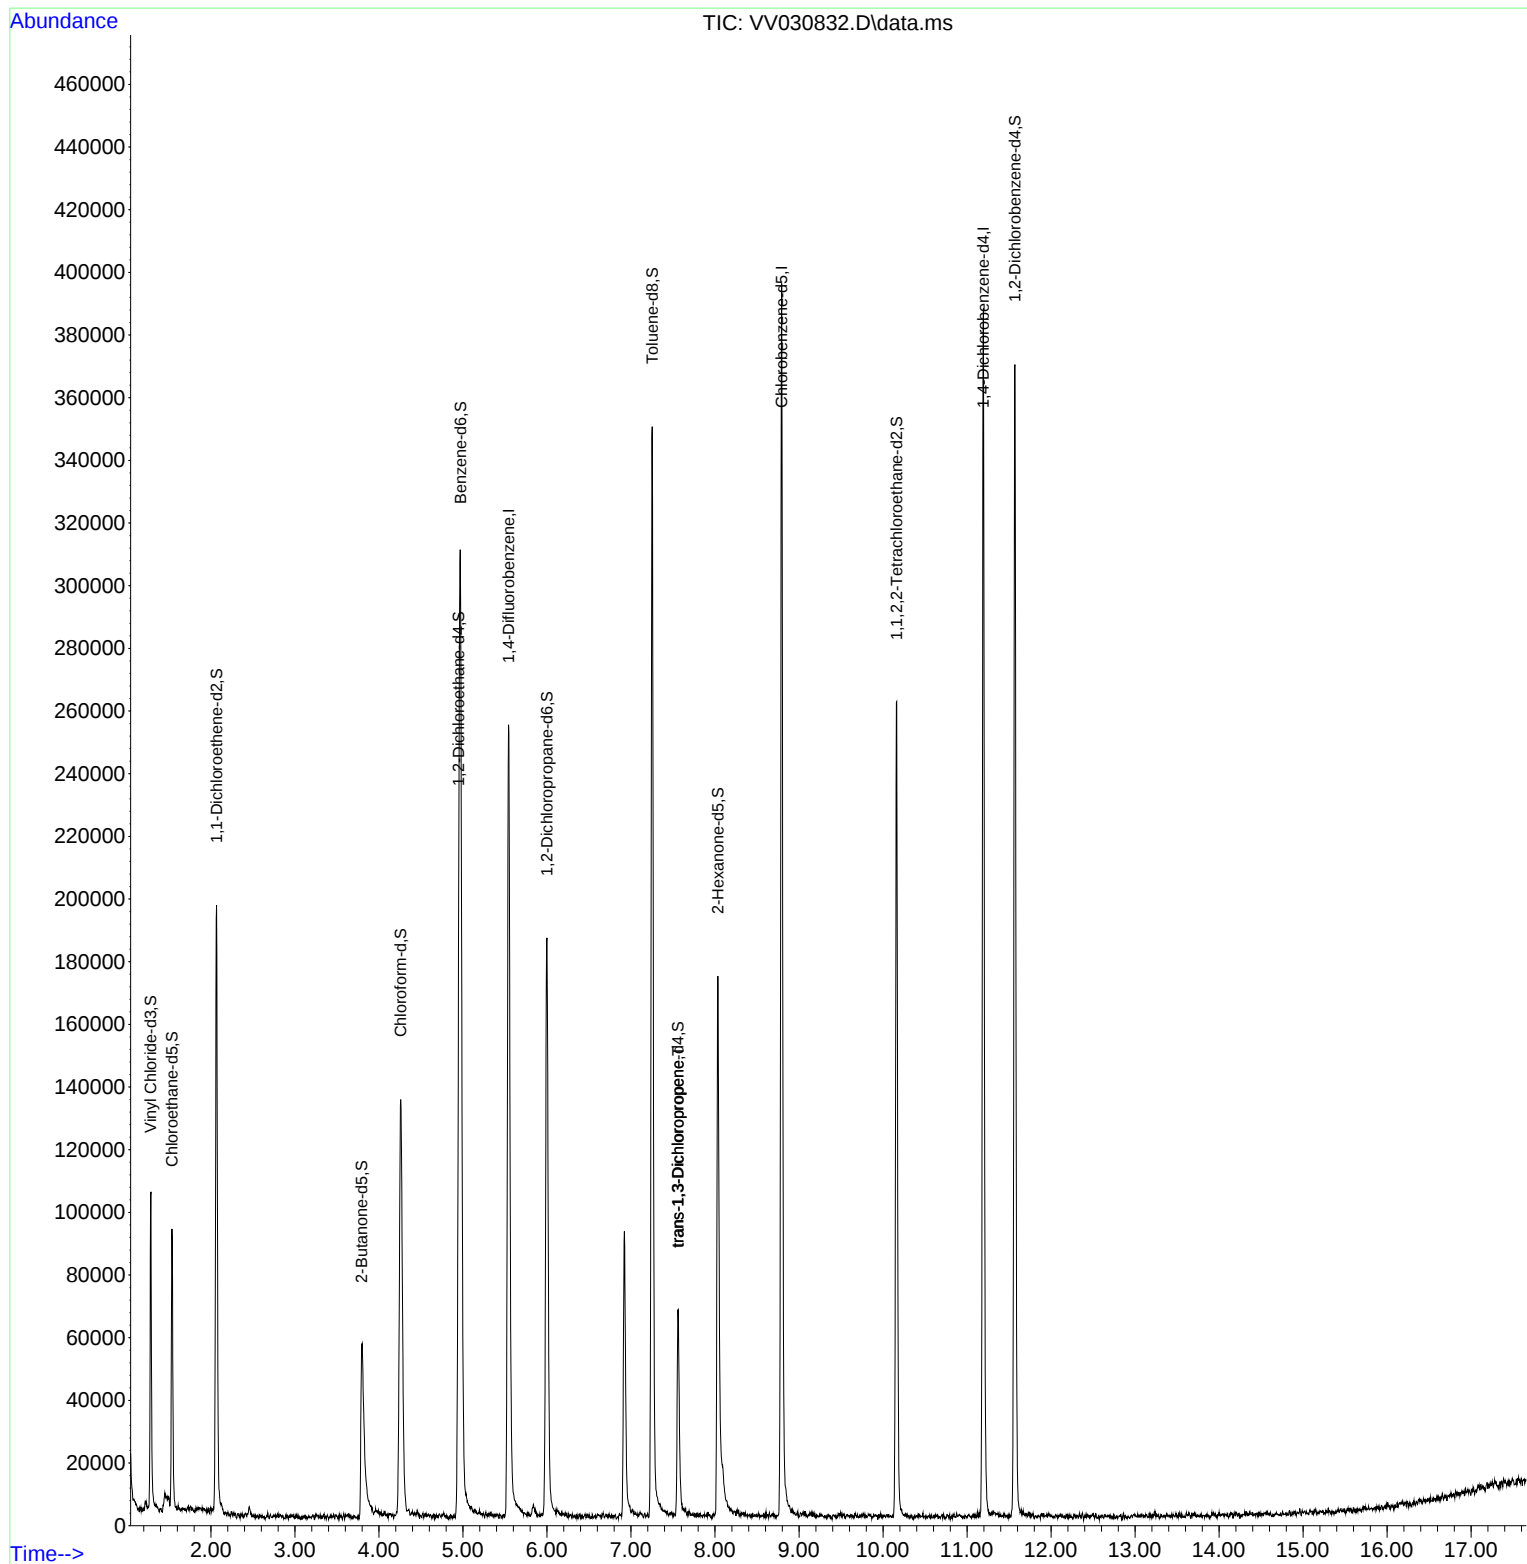

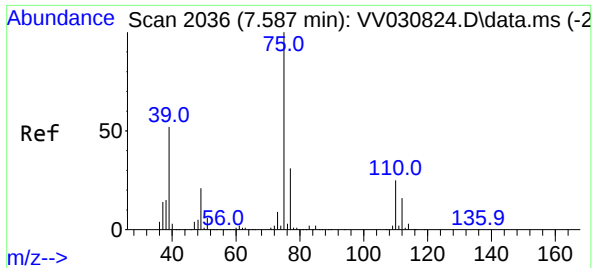

#44
 trans-1,3-Dichloropropene
 Concen: 0.951 ug/L
 RT: 7.558 min Scan# 20
 Delta R.T. -0.029 min
 Lab File: VV030832.D
 Acq: 25 Apr 2023 13:17

Instrument :
 MSVOA_V
 ClientSampleId :
 EW8Z5ME

Tgt Ion: 75 Resp: 2328
 Ion Ratio Lower Upper
 75 100
 77 35.5 22.1 41.1

