

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042523\
 Data File : VW030833.D
 Acq On : 25 Apr 2023 13:41
 Operator : SY/MD
 Sample : 02418-14ME
 Misc : 5.36g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW8Z8ME

Quant Time: Apr 26 01:30:56 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Apr 22 00:43:23 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.542	114	237614	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.793	117	231336	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152	117865	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.282	65	70328	40.374	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	80.740%		
7) Chloroethane-d5	1.536	69	58545	40.107	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	80.220%		
11) 1,1-Dichloroethene-d2	2.066	65	34966	42.329	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	84.660%		
21) 2-Butanone-d5	3.799	46	91683	95.827	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	95.830%		
24) Chloroform-d	4.259	84	143554	45.476	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	90.960%		
26) 1,2-Dichloroethane-d4	4.950	65	100529	49.533	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	99.060%		
32) Benzene-d6	4.970	84	263822	48.236	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	96.480%		
36) 1,2-Dichloropropane-d6	5.998	67	80408	47.328	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	94.660%		
41) Toluene-d8	7.252	98	241063	46.943	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	93.880%		
43) trans-1,3-Dichloroprop...	7.558	79	40489	47.284	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	94.560%		
47) 2-Hexanone-d5	8.034	63	55057	82.263	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	82.260%		
56) 1,1,2,2-Tetrachloroeth...	10.159	84	110428	44.794	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	89.580%		
66) 1,2-Dichlorobenzene-d4	11.567	152	97787	52.197	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	104.400%		
Target Compounds						Qvalue
44) trans-1,3-Dichloropropene	7.561	75	2336	0.838	ug/L	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
Data File : VV030833.D
Acq On : 25 Apr 2023 13:41
Operator : SY/MD
Sample : 02418-14ME
Misc : 5.36g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW8Z8ME

Quant Time: Apr 26 01:30:56 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Apr 22 00:43:23 2023
Response via : Initial Calibration

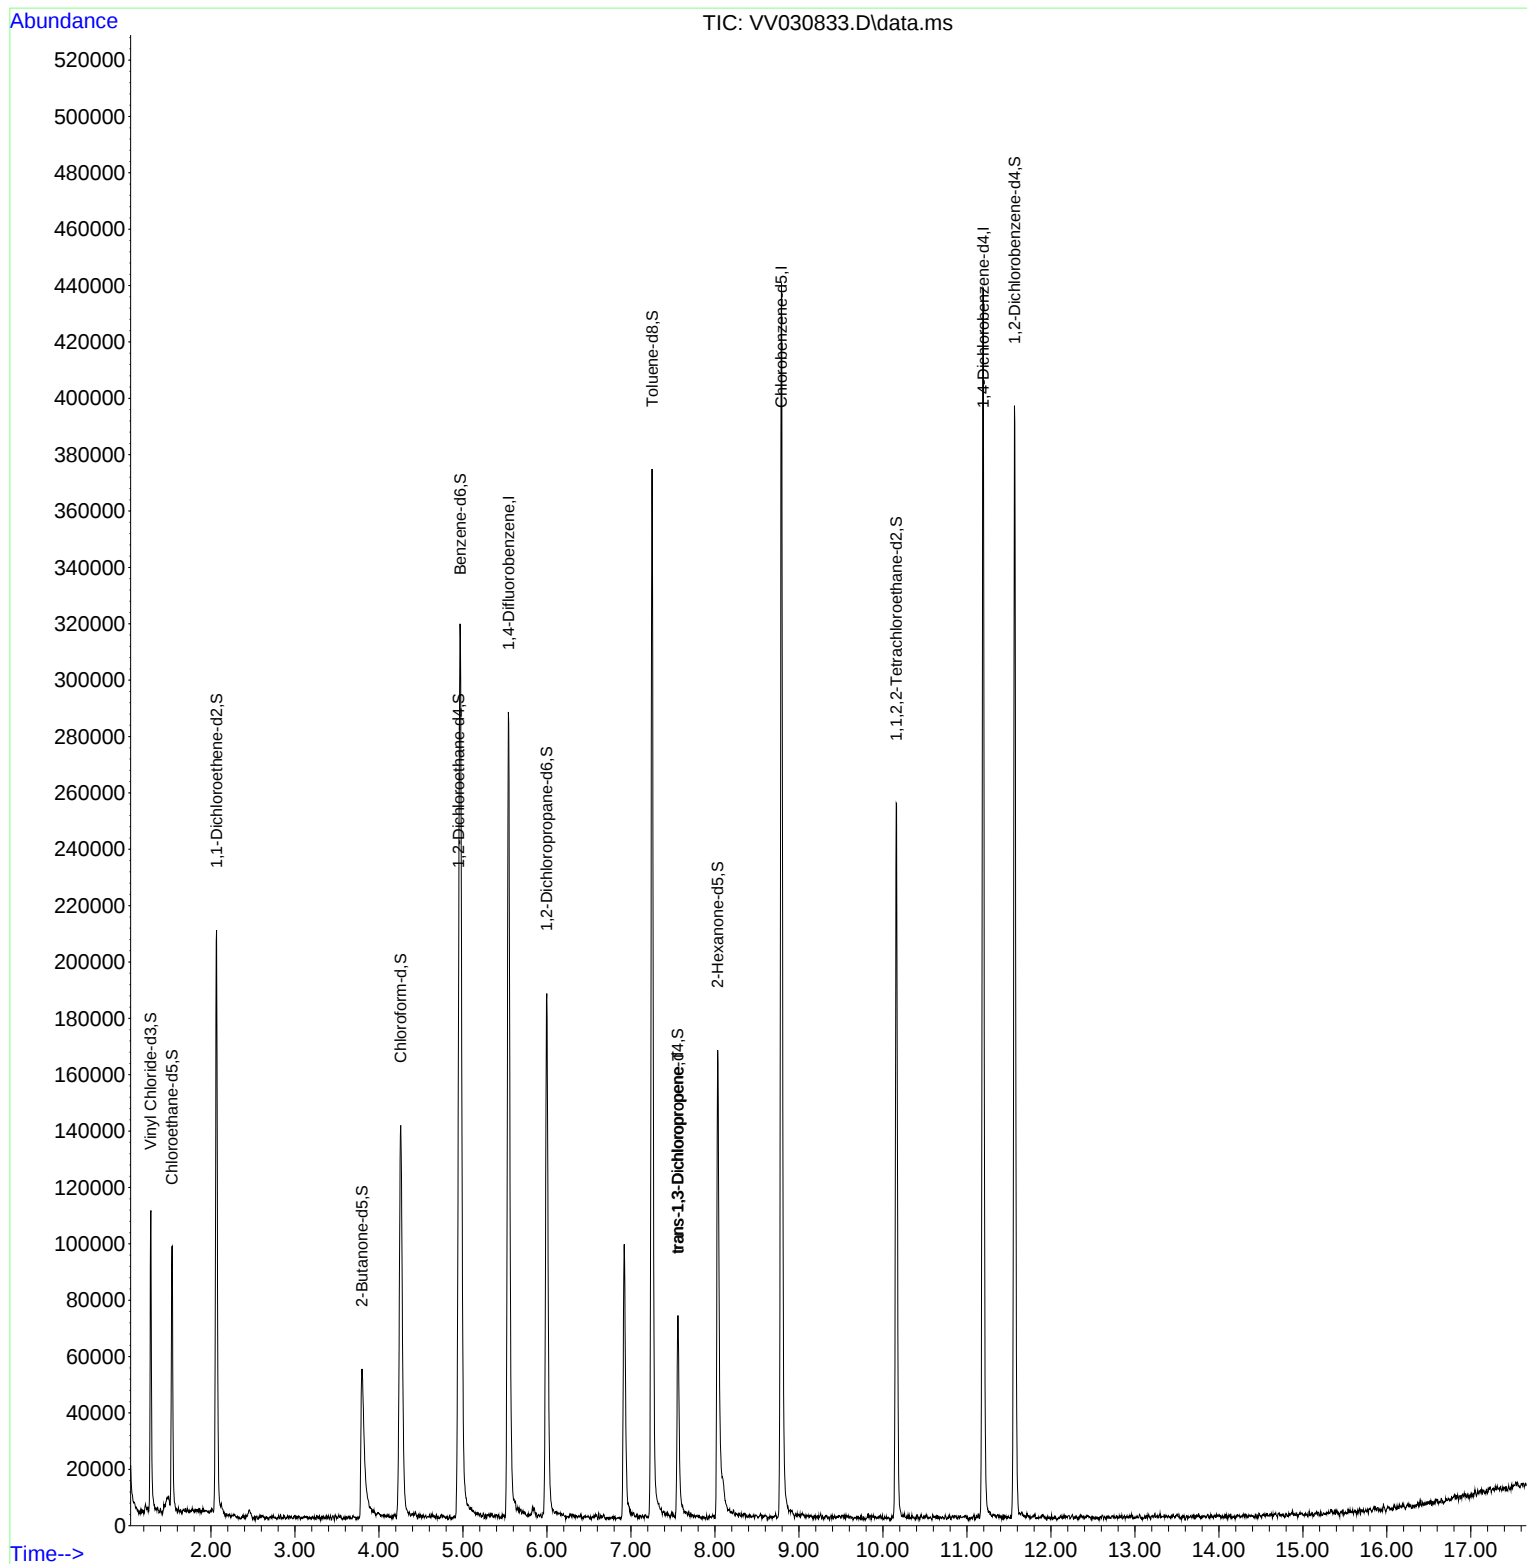

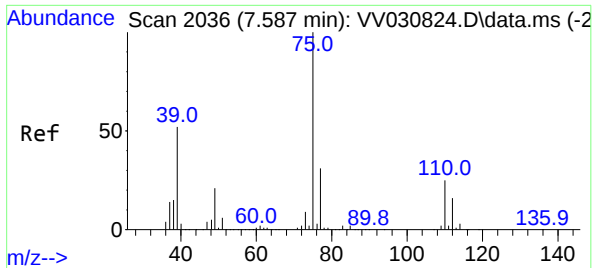

#44
 trans-1,3-Dichloropropene
 Concen: 0.838 ug/L
 RT: 7.561 min Scan# 2036
 Delta R.T. -0.026 min
 Lab File: VV030833.D
 Acq: 25 Apr 2023 13:41

Instrument :
 MSVOA_V
 ClientSampleId :
 EW8Z8ME

Tgt Ion: 75 Resp: 2336

Ion	Ratio	Lower	Upper
75	100		
77	38.2	22.1	41.1

