

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042523\
 Data File : VW030838.D
 Acq On : 25 Apr 2023 15:41
 Operator : SY/MD
 Sample : 02417-03ME
 Misc : 5.44g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW8W9ME

Quant Time: Apr 26 01:31:32 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Apr 22 00:43:23 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.542	114	209130	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.792	117	206920	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152	103041	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.282	65	63051	41.127	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	82.260%
7) Chloroethane-d5	1.536	69	56060	43.636	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	87.280%
11) 1,1-Dichloroethene-d2	2.066	65	31933	43.922	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	87.840%
21) 2-Butanone-d5	3.799	46	92659	110.038	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	110.040%
24) Chloroform-d	4.262	84	137475	49.481	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	98.960%
26) 1,2-Dichloroethane-d4	4.953	65	100923	56.501	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	113.000%
32) Benzene-d6	4.969	84	247680	50.628	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	101.260%
36) 1,2-Dichloropropane-d6	5.998	67	75873	49.928	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	99.860%
41) Toluene-d8	7.252	98	223020	48.554	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	97.100%
43) trans-1,3-Dichloroprop...	7.561	79	39011	50.933	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	101.860%
47) 2-Hexanone-d5	8.034	63	56244	93.952	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	93.950%
56) 1,1,2,2-Tetrachloroeth...	10.159	84	110235	49.992	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	99.980%
66) 1,2-Dichlorobenzene-d4	11.567	152	94204	57.519	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	115.040%
Target Compounds						Qvalue
44) trans-1,3-Dichloropropene	7.558	75	2151	0.863	ug/L	# 57


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
Data File : VV030838.D
Acq On : 25 Apr 2023 15:41
Operator : SY/MD
Sample : 02417-03ME
Misc : 5.44g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW8W9ME

Quant Time: Apr 26 01:31:32 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Apr 22 00:43:23 2023
Response via : Initial Calibration

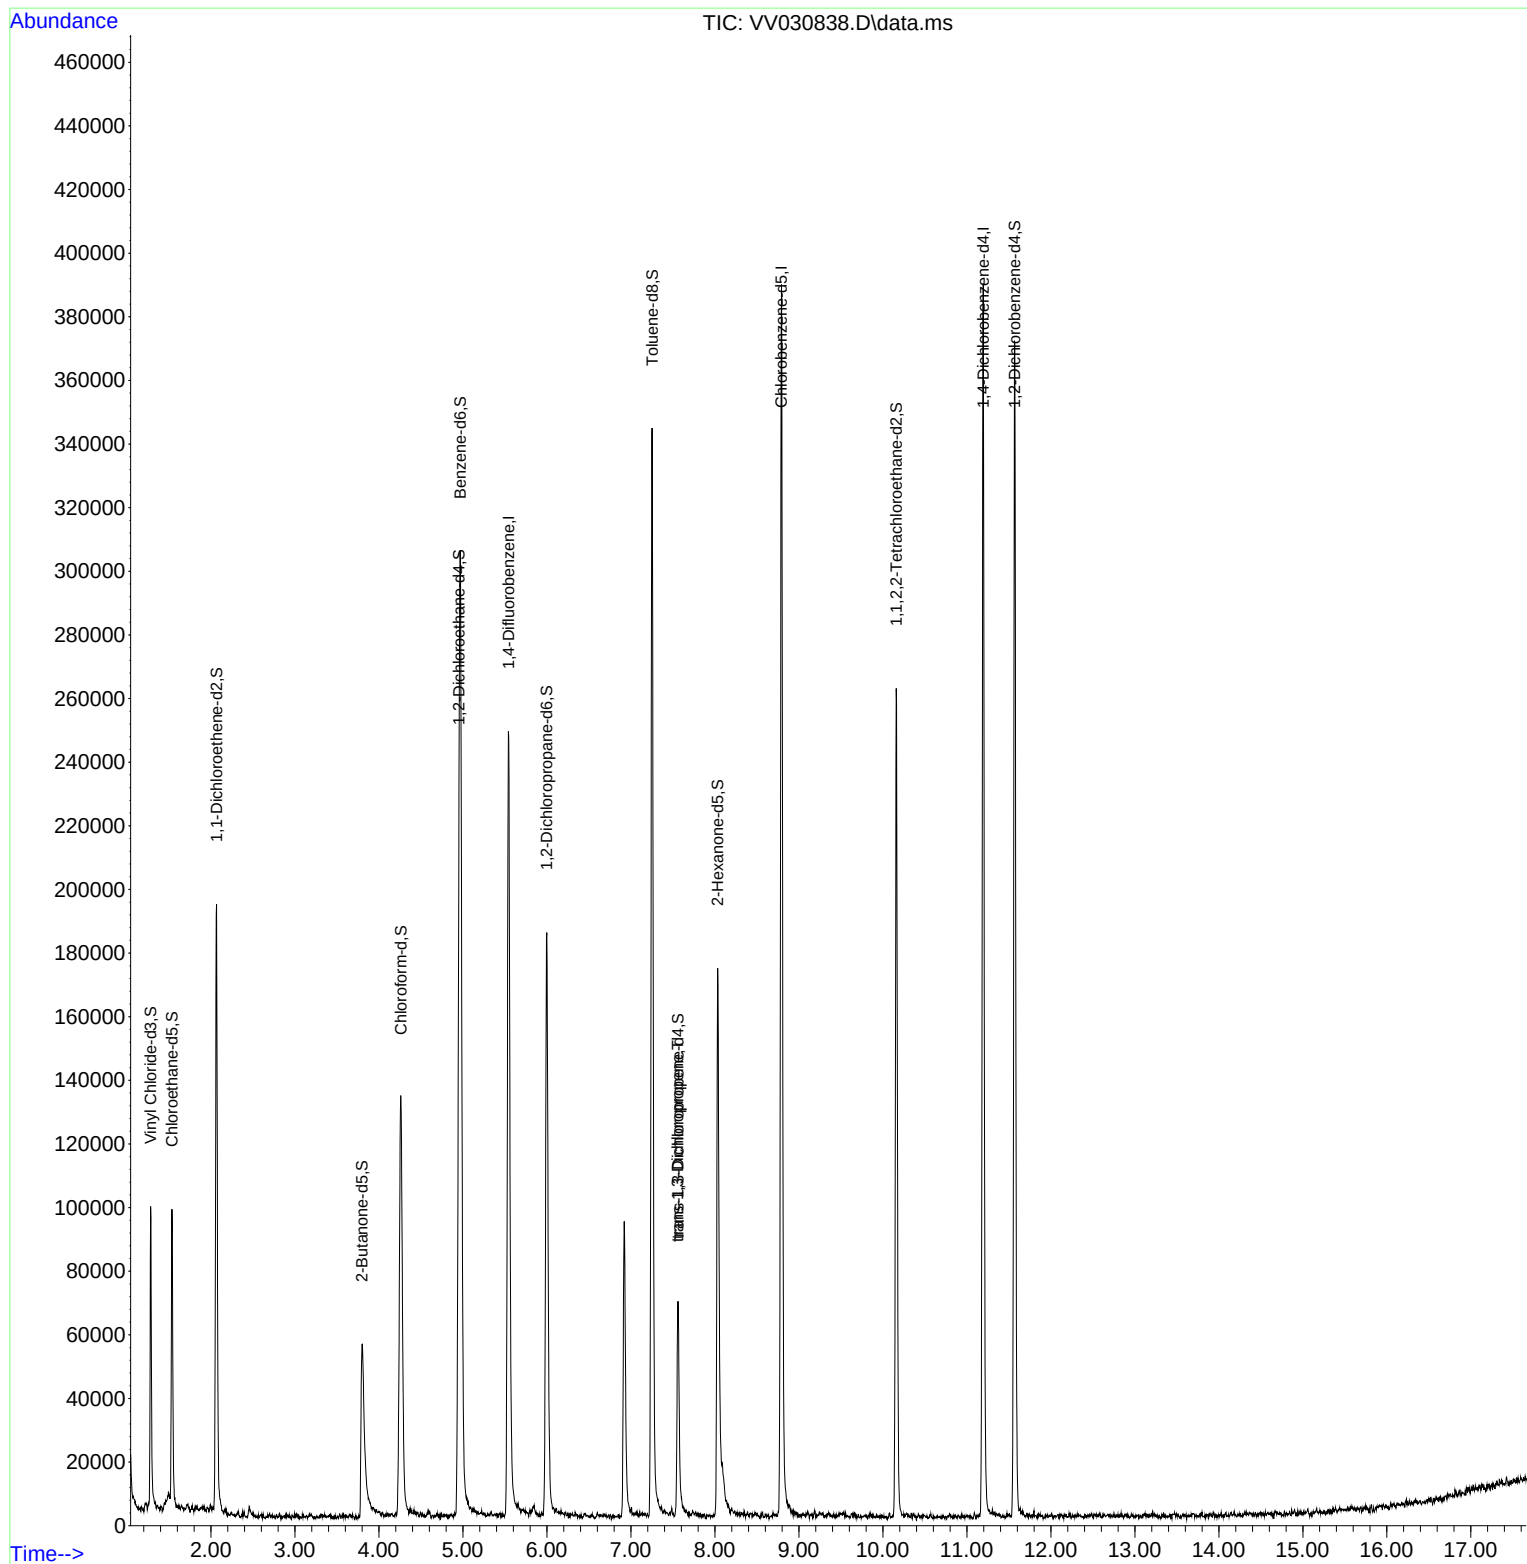

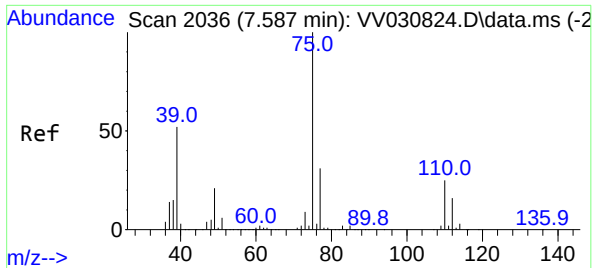

#44
trans-1,3-Dichloropropene
Concen: 0.863 ug/L
RT: 7.558 min Scan# 20
Delta R.T. -0.029 min
Lab File: VV030838.D
Acq: 25 Apr 2023 15:41

Instrument :
MSVOA_V
ClientSampleId :
EW8W9ME

Tgt Ion: 75 Resp: 2151
Ion Ratio Lower Upper
75 100
77 55.6 22.1 41.1#

