

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042523\
 Data File : VW030841.D
 Acq On : 25 Apr 2023 16:52
 Operator : SY/MD
 Sample : 02417-16ME
 Misc : 5.44g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW8Y2ME

Quant Time: Apr 26 01:31:54 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Apr 22 00:43:23 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.542	114	205394	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.792	117	200105	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152	100303	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.281	65	57283	38.044	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	76.080%		
7) Chloroethane-d5	1.535	69	52193	41.365	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	82.720%		
11) 1,1-Dichloroethene-d2	2.063	65	29593	41.444	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	82.880%		
21) 2-Butanone-d5	3.799	46	88205	106.654	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	106.650%		
24) Chloroform-d	4.259	84	126583	46.390	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	92.780%		
26) 1,2-Dichloroethane-d4	4.953	65	94056	53.614	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	107.220%		
32) Benzene-d6	4.969	84	229972	48.609	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	97.220%		
36) 1,2-Dichloropropane-d6	5.998	67	71492	48.648	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	97.300%		
41) Toluene-d8	7.252	98	199515	44.916	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	89.840%		
43) trans-1,3-Dichloroprop...	7.561	79	34383	46.420	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	92.840%		
47) 2-Hexanone-d5	8.034	63	53615	92.611	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	92.610%		
56) 1,1,2,2-Tetrachloroeth...	10.159	84	104550	49.028	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	98.060%		
66) 1,2-Dichlorobenzene-d4	11.570	152	84901	53.254	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	106.500%		
Target Compounds						Qvalue
44) trans-1,3-Dichloropropene	7.561	75	2087	0.865	ug/L	# 79


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
Data File : VV030841.D
Acq On : 25 Apr 2023 16:52
Operator : SY/MD
Sample : 02417-16ME
Misc : 5.44g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW8Y2ME

Quant Time: Apr 26 01:31:54 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Apr 22 00:43:23 2023
Response via : Initial Calibration

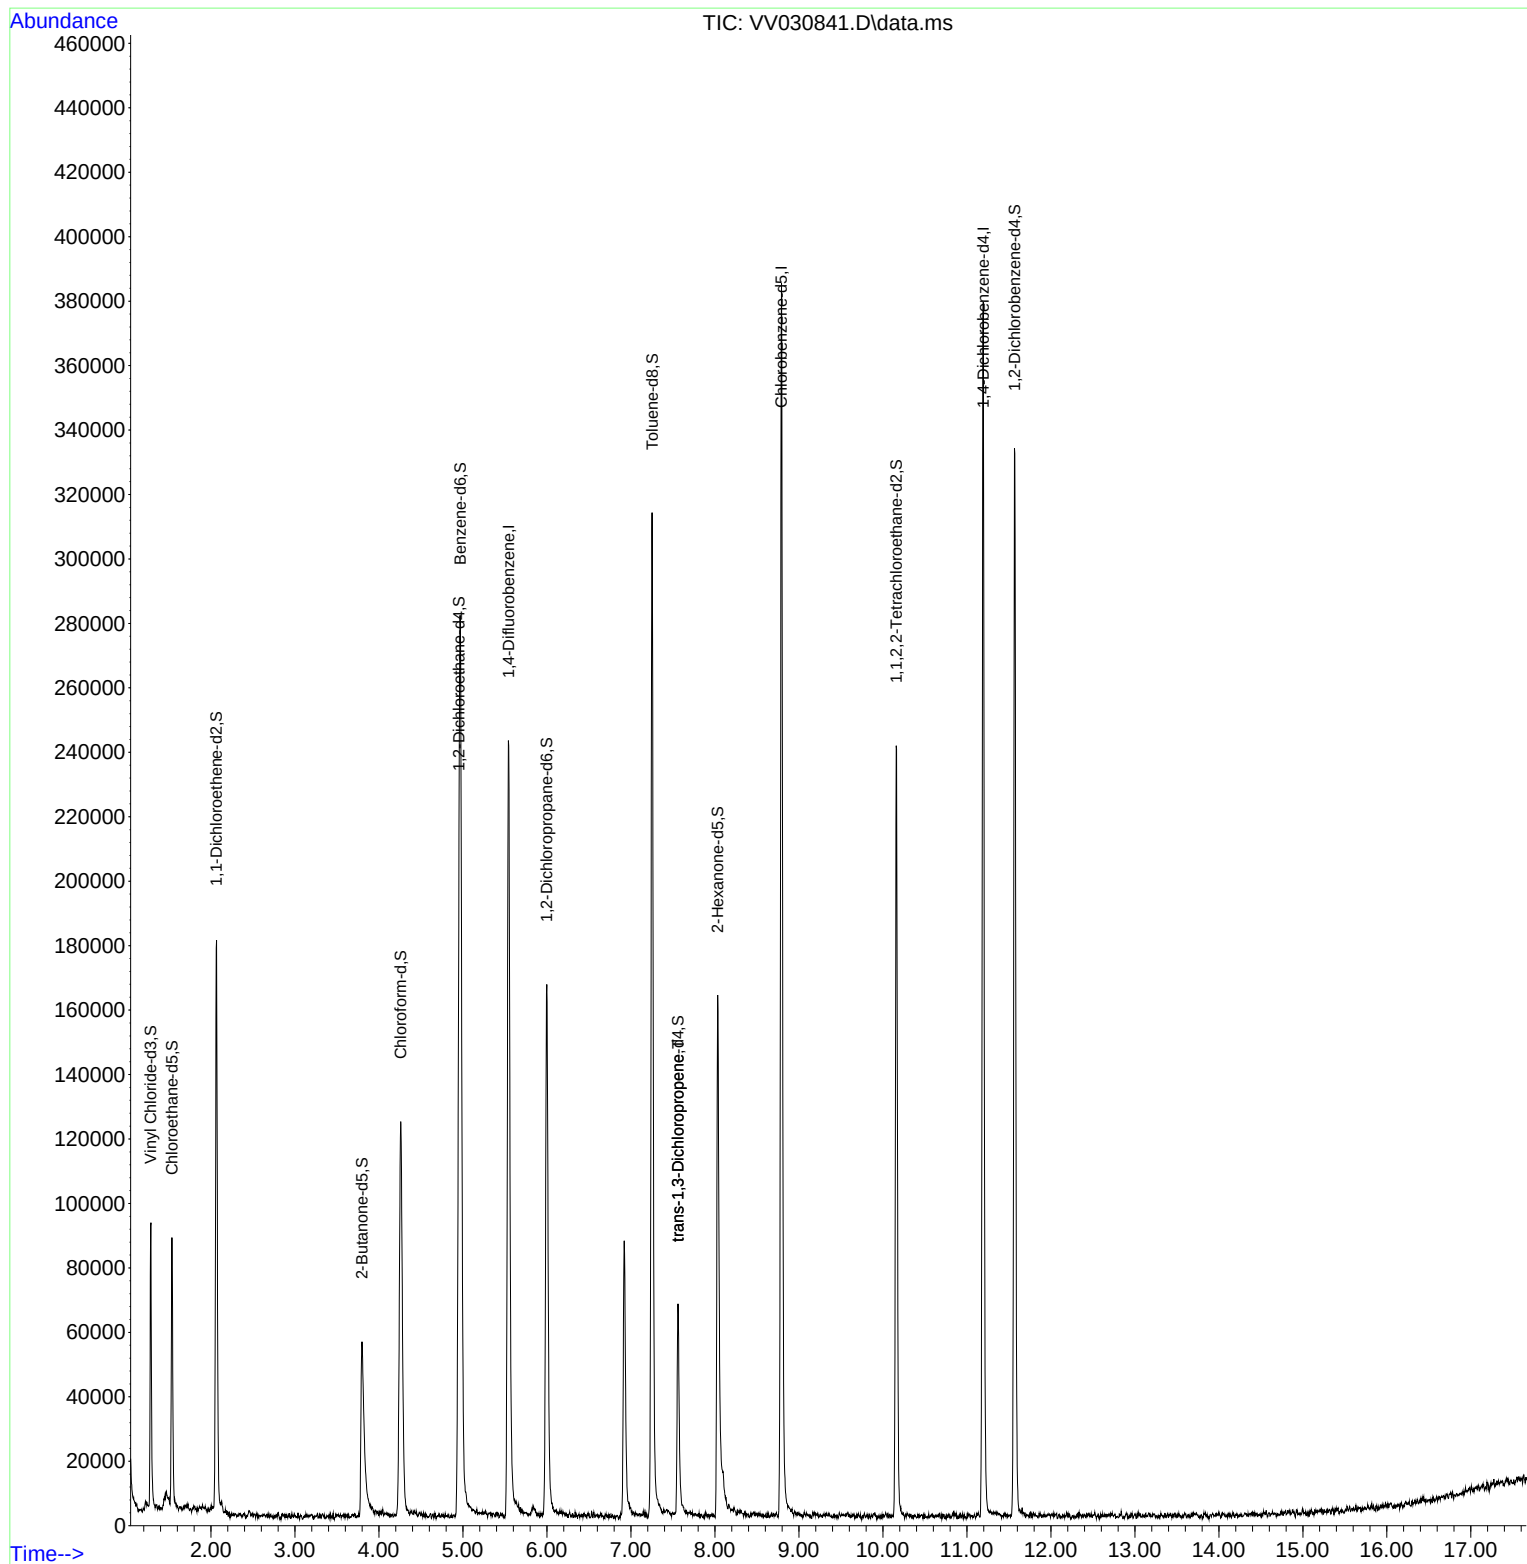

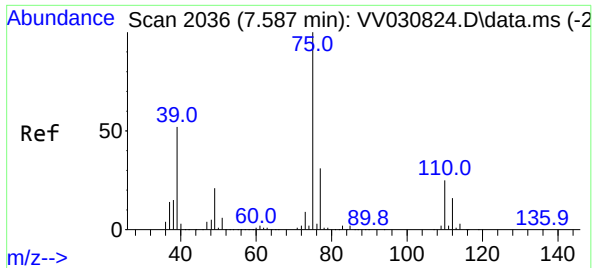

#44
 trans-1,3-Dichloropropene
 Concen: 0.865 ug/L
 RT: 7.561 min Scan# 20
 Delta R.T. -0.026 min
 Lab File: VV030841.D
 Acq: 25 Apr 2023 16:52

Instrument :
 MSVOA_V
 ClientSampleId :
 EW8Y2ME

Tgt Ion: 75 Resp: 2087
 Ion Ratio Lower Upper
 75 100
 77 43.0 22.1 41.1#

