

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042523\
 Data File : VW030842.D
 Acq On : 25 Apr 2023 17:16
 Operator : SY/MD
 Sample : 02475-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AW9

Quant Time: Apr 26 01:32:02 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Apr 22 00:43:23 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.545	114	223863	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.792	117	218337	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152	108461	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.281	65	66167	40.319	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	80.640%		
7) Chloroethane-d5	1.535	69	56951	41.412	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	82.820%		
11) 1,1-Dichloroethene-d2	2.066	65	33653	43.241	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	86.480%		
21) 2-Butanone-d5	3.799	46	86654	96.134	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	96.130%		
24) Chloroform-d	4.262	84	137634	46.278	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	92.560%		
26) 1,2-Dichloroethane-d4	4.950	65	99349	51.959	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	103.920%		
32) Benzene-d6	4.969	84	252376	48.890	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	97.780%		
36) 1,2-Dichloropropane-d6	5.998	67	77806	48.523	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	97.040%		
41) Toluene-d8	7.252	98	227525	46.944	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	93.880%		
43) trans-1,3-Dichloroprop...	7.561	79	38804	48.014	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	96.020%		
47) 2-Hexanone-d5	8.034	63	51483	81.502	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	81.500%		
56) 1,1,2,2-Tetrachloroeth...	10.162	84	108828	46.773	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	93.540%		
66) 1,2-Dichlorobenzene-d4	11.570	152	96025	55.701	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	111.400%		
Target Compounds						Qvalue
44) trans-1,3-Dichloropropene	7.558	75	2357	0.896	ug/L	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
Data File : VV030842.D
Acq On : 25 Apr 2023 17:16
Operator : SY/MD
Sample : 02475-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AW9


Quant Time: Apr 26 01:32:02 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Apr 22 00:43:23 2023
Response via : Initial Calibration

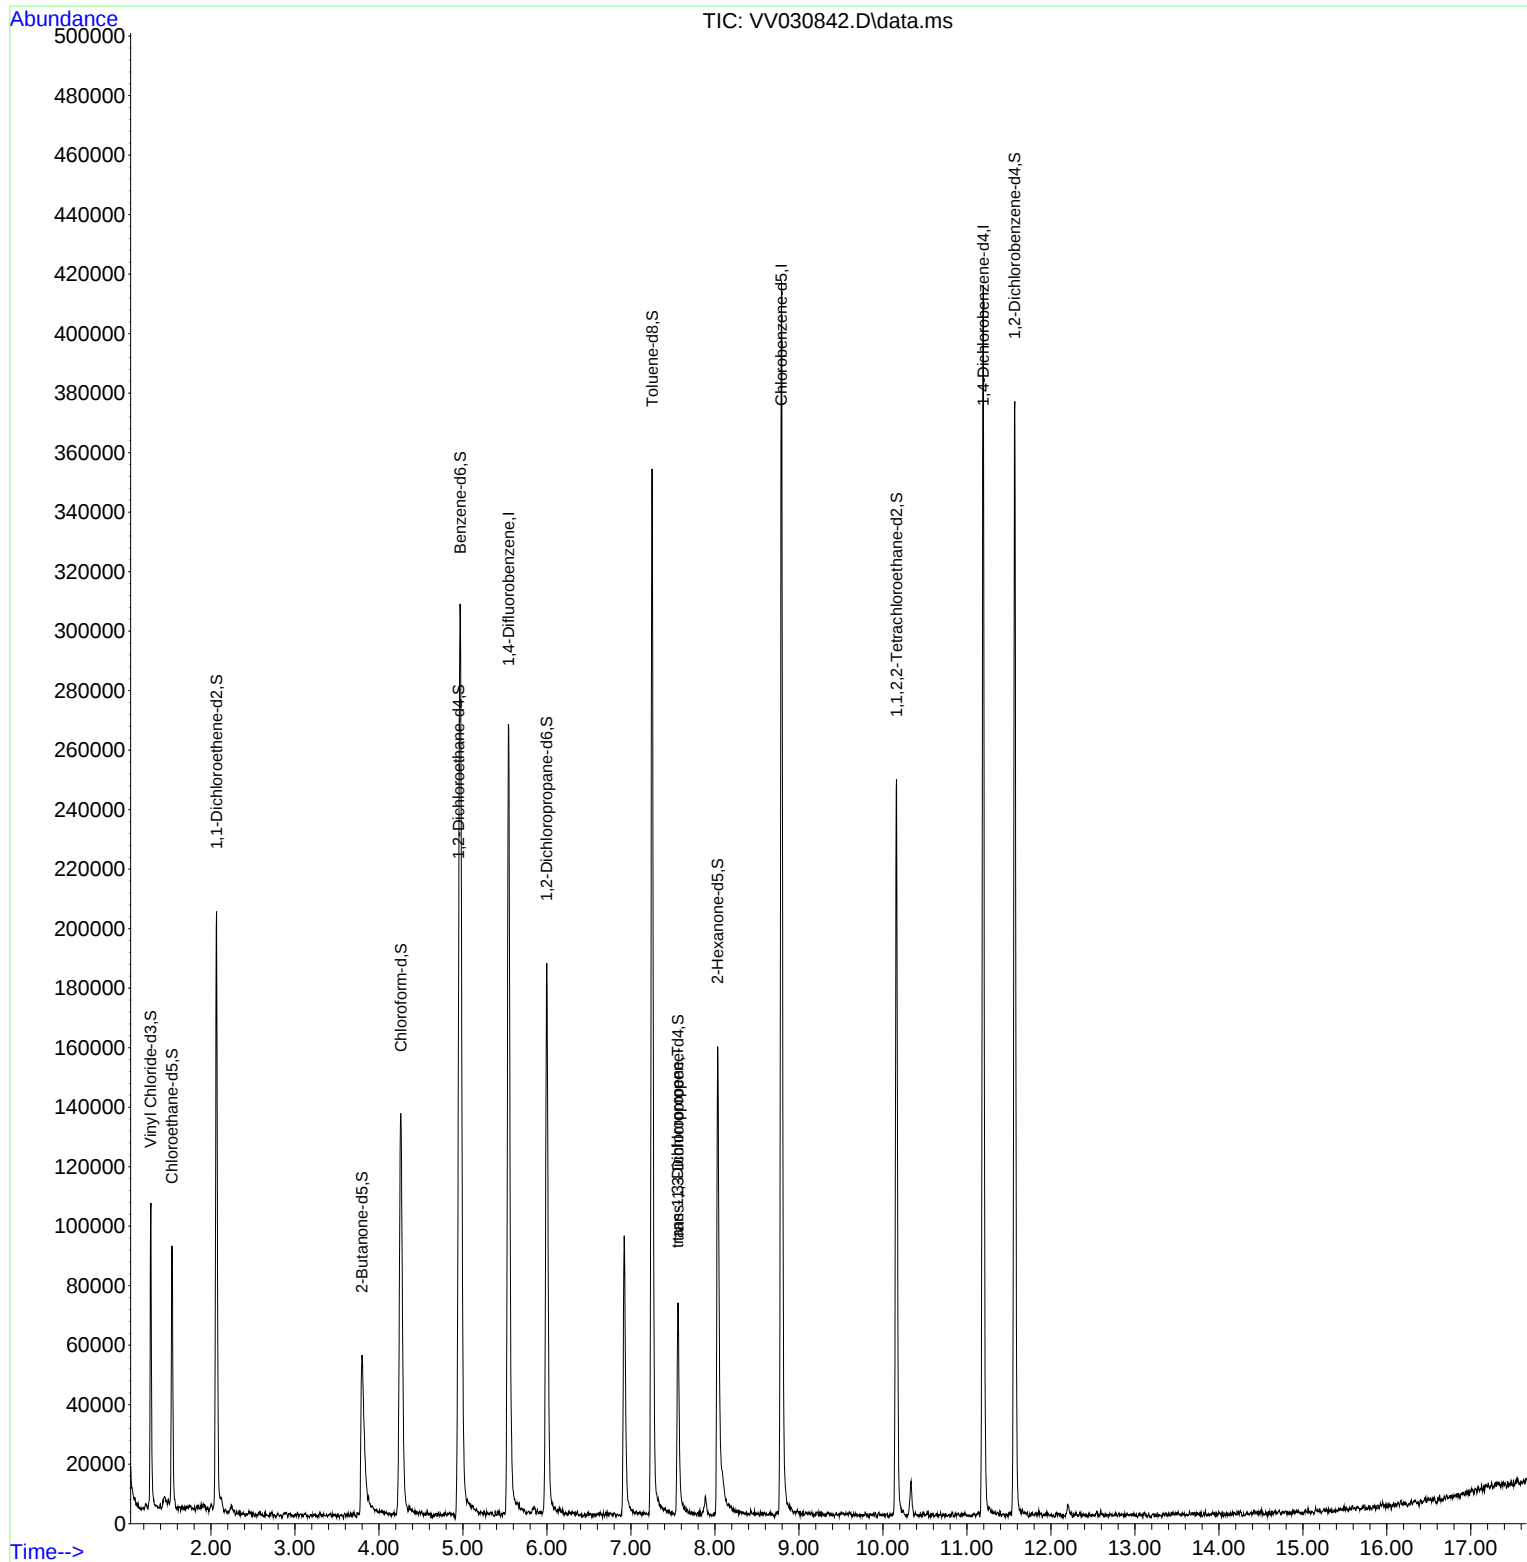

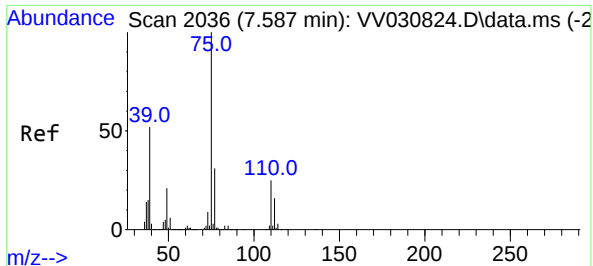

#44
trans-1,3-Dichloropropene
Concen: 0.896 ug/L
RT: 7.558 min Scan# 2036
Delta R.T. -0.029 min
Lab File: VV030842.D
Acq: 25 Apr 2023 17:16

Instrument :
MSVOA_V
ClientSampleId :
C0AW9

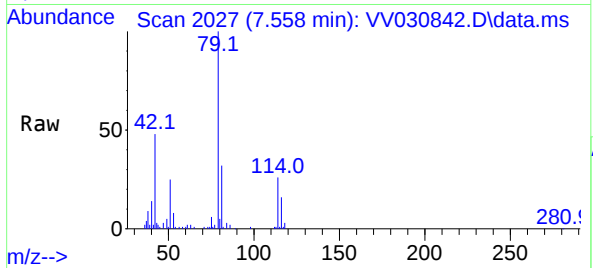

Tgt Ion: 75 Resp: 2357
Ion Ratio Lower Upper
75 100
77 38.8 22.1 41.1

