

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042523\
 Data File : VW030843.D
 Acq On : 25 Apr 2023 17:40
 Operator : SY/MD
 Sample : 02475-01 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AW3

Quant Time: Apr 26 01:32:09 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Apr 22 00:43:23 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.542	114	197196	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.793	117	193676	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152	94527	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.282	65	54398	37.630	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	75.260%
7) Chloroethane-d5	1.536	69	48502	40.038	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	80.080%
11) 1,1-Dichloroethene-d2	2.066	65	27882	40.671	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	81.340%
21) 2-Butanone-d5	3.806	46	70107	88.295	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	88.300%
24) Chloroform-d	4.259	84	113013	43.139	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	86.280%
26) 1,2-Dichloroethane-d4	4.953	65	80210	47.622	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	95.240%
32) Benzene-d6	4.973	84	205905	44.967	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	89.940%
36) 1,2-Dichloropropane-d6	5.998	67	62043	43.619	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	87.240%
41) Toluene-d8	7.252	98	180570	42.000	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	84.000%
43) trans-1,3-Dichloroprop...	7.561	79	31262	43.607	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	87.220%
47) 2-Hexanone-d5	8.034	63	40697	72.631	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	72.630%
56) 1,1,2,2-Tetrachloroeth...	10.159	84	87540	42.414	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	84.820%
66) 1,2-Dichlorobenzene-d4	11.571	152	77469	51.561	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	103.120%
Target Compounds						
44) trans-1,3-Dichloropropene	7.564	75	1969	0.844	ug/L	Qvalue 87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
Data File : VV030843.D
Acq On : 25 Apr 2023 17:40
Operator : SY/MD
Sample : 02475-01 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AW3

Quant Time: Apr 26 01:32:09 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Apr 22 00:43:23 2023
Response via : Initial Calibration

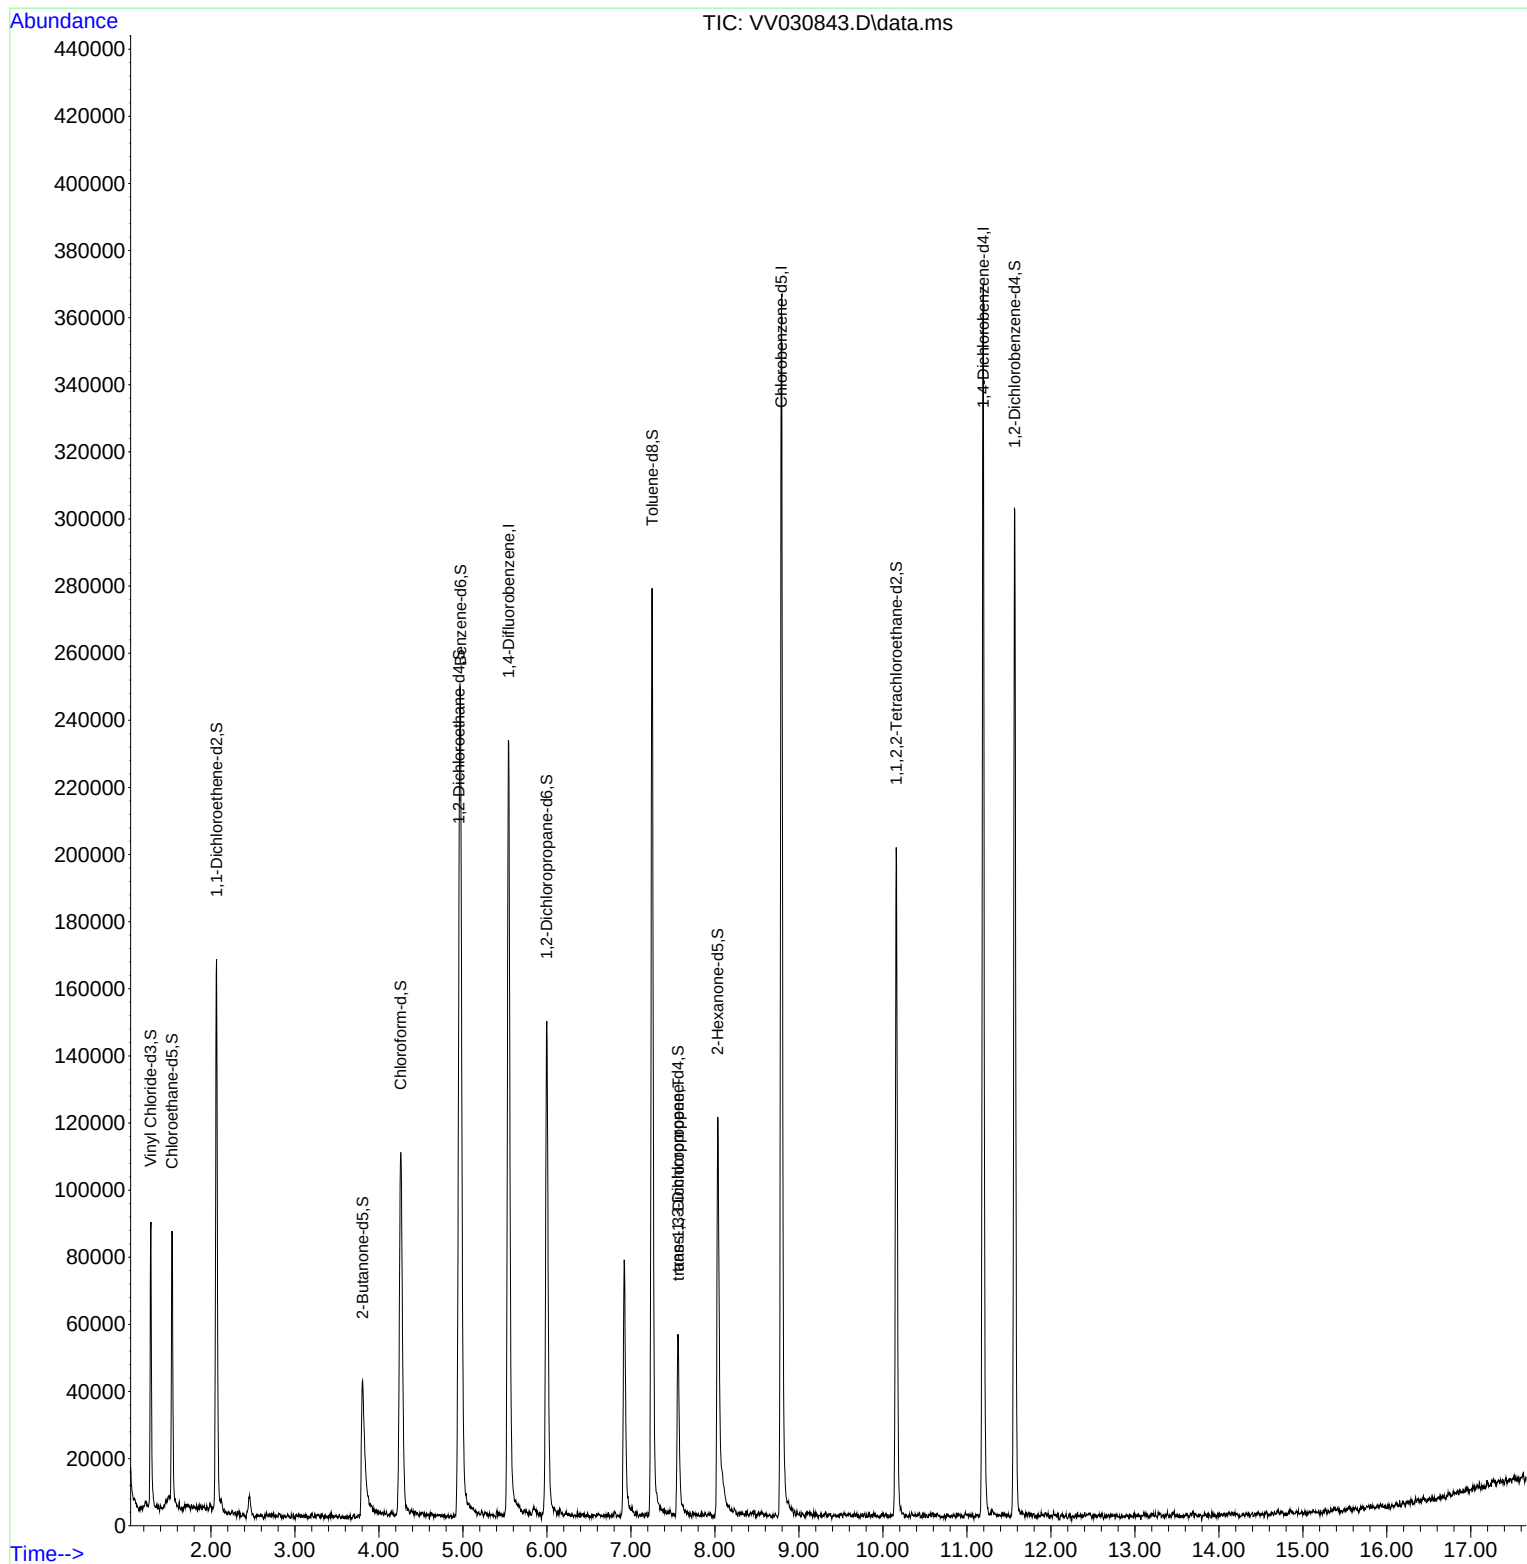

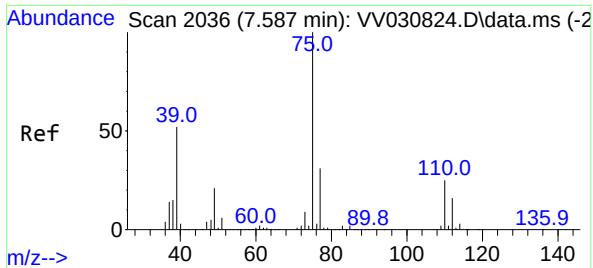

#44
trans-1,3-Dichloropropene
Concen: 0.844 ug/L
RT: 7.564 min Scan# 20
Delta R.T. -0.023 min
Lab File: VV030843.D
Acq: 25 Apr 2023 17:40

Instrument :
MSVOA_V
ClientSampleId :
C0AW3

Tgt Ion: 75 Resp: 1969
Ion Ratio Lower Upper
75 100
77 39.0 22.1 41.1

