

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042523\
 Data File : VW030845.D
 Acq On : 25 Apr 2023 18:28
 Operator : SY/MD
 Sample : 02475-03 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AW5

Quant Time: Apr 26 01:32:23 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Apr 22 00:43:23 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.542	114	225995	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.792	117	222991	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152	109113	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.281	65	66428	40.096	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	80.200%
7) Chloroethane-d5	1.535	69	56517	40.709	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	81.420%
11) 1,1-Dichloroethene-d2	2.066	65	33865	43.103	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	86.200%
21) 2-Butanone-d5	3.796	46	89599	98.464	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	98.460%
24) Chloroform-d	4.262	84	140827	46.905	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.820%
26) 1,2-Dichloroethane-d4	4.950	65	101686	52.680	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	105.360%
32) Benzene-d6	4.969	84	257809	48.900	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	97.800%
36) 1,2-Dichloropropane-d6	5.995	67	77664	47.424	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	94.840%
41) Toluene-d8	7.252	98	229661	46.396	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	92.800%
43) trans-1,3-Dichloroprop...	7.561	79	38437	46.567	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	93.140%
47) 2-Hexanone-d5	8.034	63	53628	83.126	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	83.130%
56) 1,1,2,2-Tetrachloroeth...	10.159	84	108249	45.553	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	91.100%
66) 1,2-Dichlorobenzene-d4	11.567	152	97506	56.222	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	112.440%
Target Compounds						
					Qvalue	
44) trans-1,3-Dichloropropene	7.558	75	2018	0.751	ug/L	# 81


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
Data File : VV030845.D
Acq On : 25 Apr 2023 18:28
Operator : SY/MD
Sample : 02475-03 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AW5

Quant Time: Apr 26 01:32:23 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Apr 22 00:43:23 2023
Response via : Initial Calibration

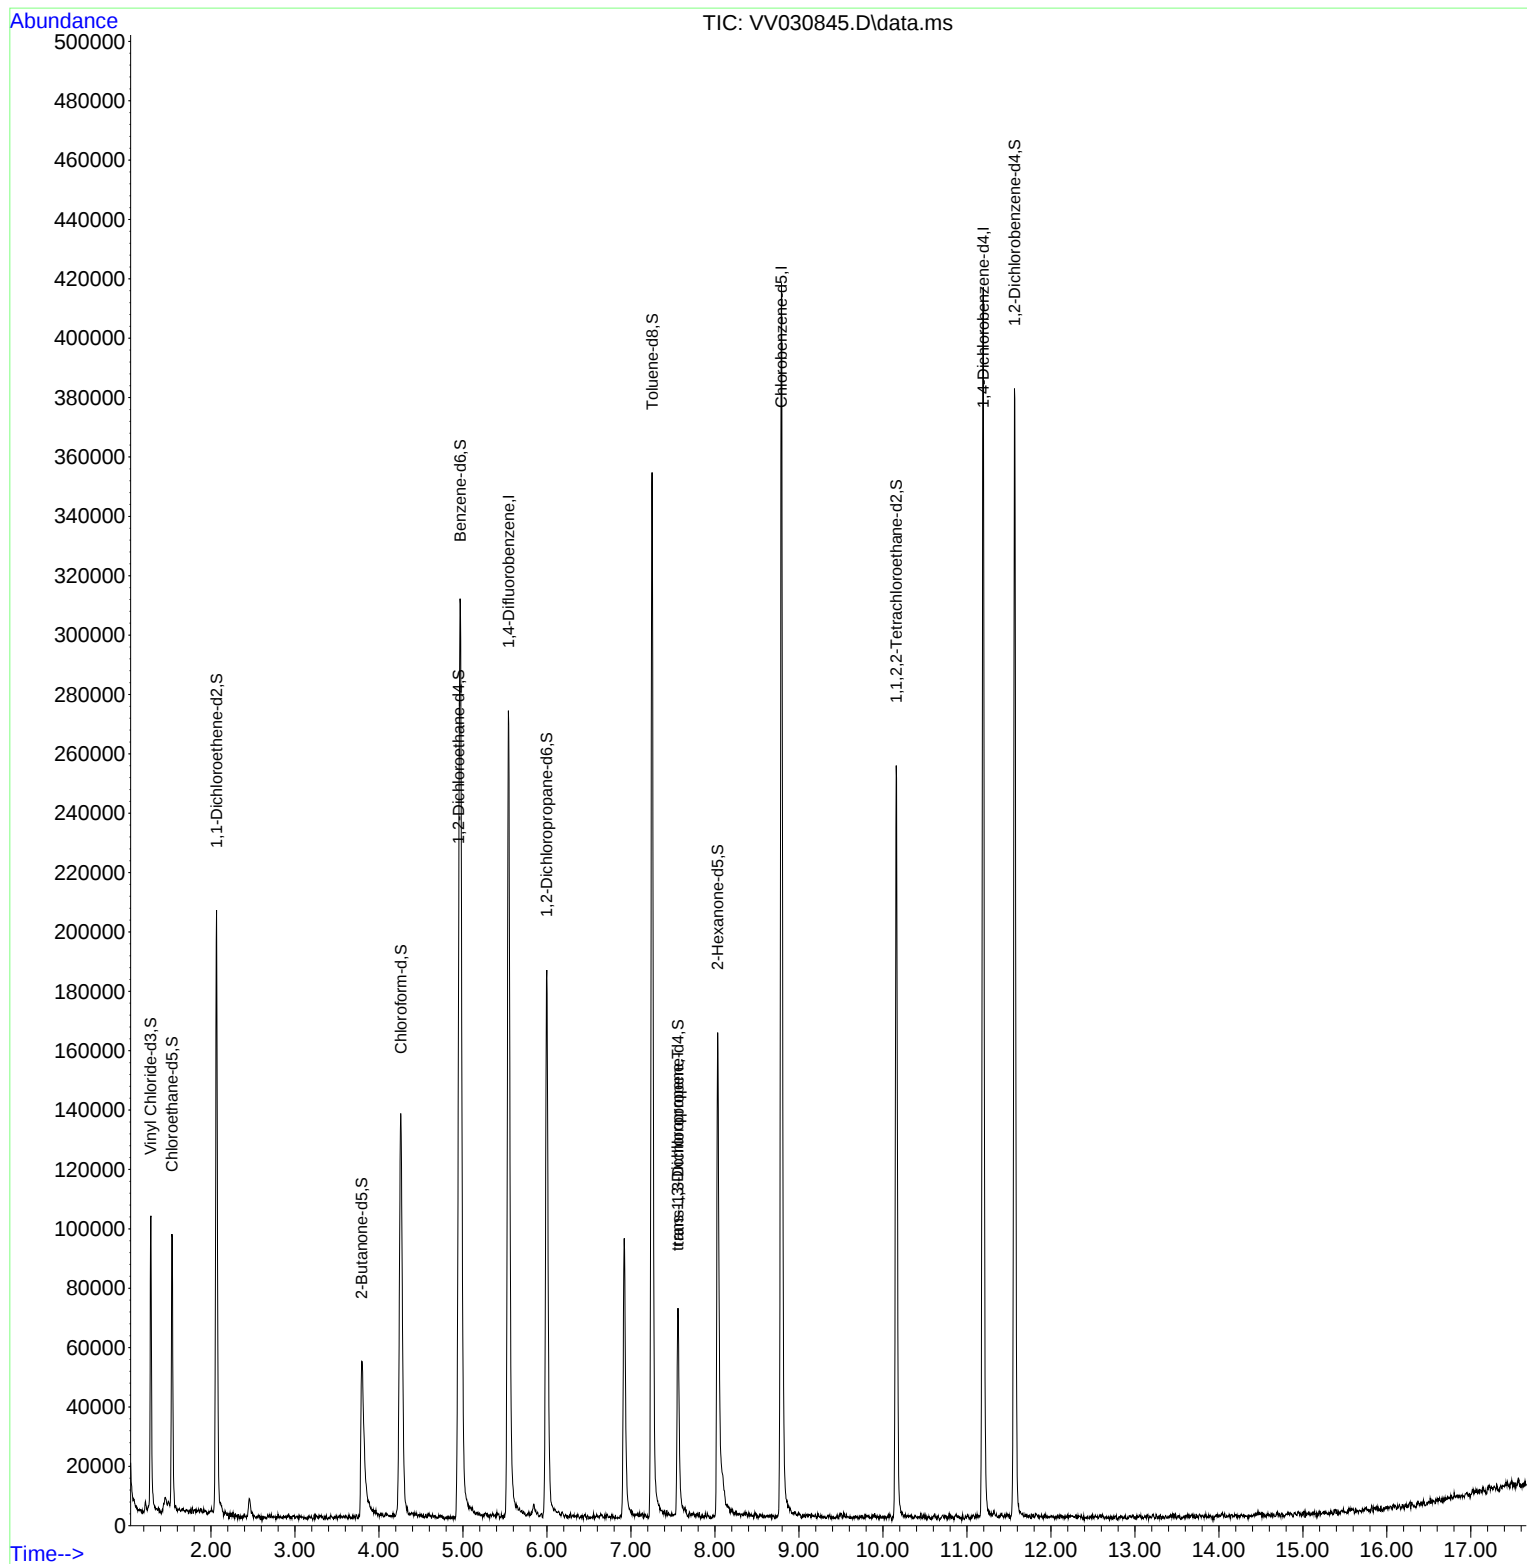

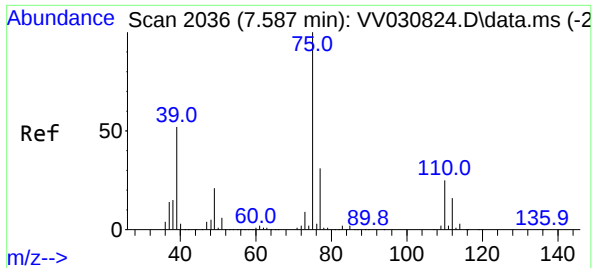

#44
trans-1,3-Dichloropropene
Concen: 0.751 ug/L
RT: 7.558 min Scan# 2018
Delta R.T. -0.029 min
Lab File: VV030845.D
Acq: 25 Apr 2023 18:28

Instrument :
MSVOA_V
ClientSampleId :
C0AW5

Tgt Ion: 75 Resp: 2018
Ion Ratio Lower Upper
75 100
77 42.4 22.1 41.1#

