

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042523\
 Data File : VW030859.D
 Acq On : 26 Apr 2023 00:43
 Operator : SY/MD
 Sample : 02474-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AT2

Quant Time: Apr 26 02:58:38 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Apr 22 00:43:23 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.542	114	213894	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.792	117	210469	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152	105956	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.281	65	60304	38.459	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	76.920%		
7) Chloroethane-d5	1.536	69	54260	41.294	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	82.580%		
11) 1,1-Dichloroethene-d2	2.066	65	31838	42.816	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	85.640%		
21) 2-Butanone-d5	3.799	46	82220	95.467	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	95.470%		
24) Chloroform-d	4.259	84	133930	47.132	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	94.260%		
26) 1,2-Dichloroethane-d4	4.950	65	97055	53.125	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	106.240%		
32) Benzene-d6	4.969	84	241915	48.616	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	97.240%		
36) 1,2-Dichloropropane-d6	5.998	67	74253	48.038	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	96.080%		
41) Toluene-d8	7.252	98	216236	46.283	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	92.560%		
43) trans-1,3-Dichloroprop...	7.561	79	35958	46.155	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	92.320%		
47) 2-Hexanone-d5	8.034	63	48145	79.067	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	79.070%		
56) 1,1,2,2-Tetrachloroeth...	10.159	84	104977	46.804	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	93.600%		
66) 1,2-Dichlorobenzene-d4	11.567	152	91705	54.452	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	108.900%		
Target Compounds					Qvalue	
13) Acetone	2.124	43	6584	4.940	ug/L	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
Data File : VV030859.D
Acq On : 26 Apr 2023 00:43
Operator : SY/MD
Sample : 02474-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AT2

Quant Time: Apr 26 02:58:38 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Apr 22 00:43:23 2023
Response via : Initial Calibration

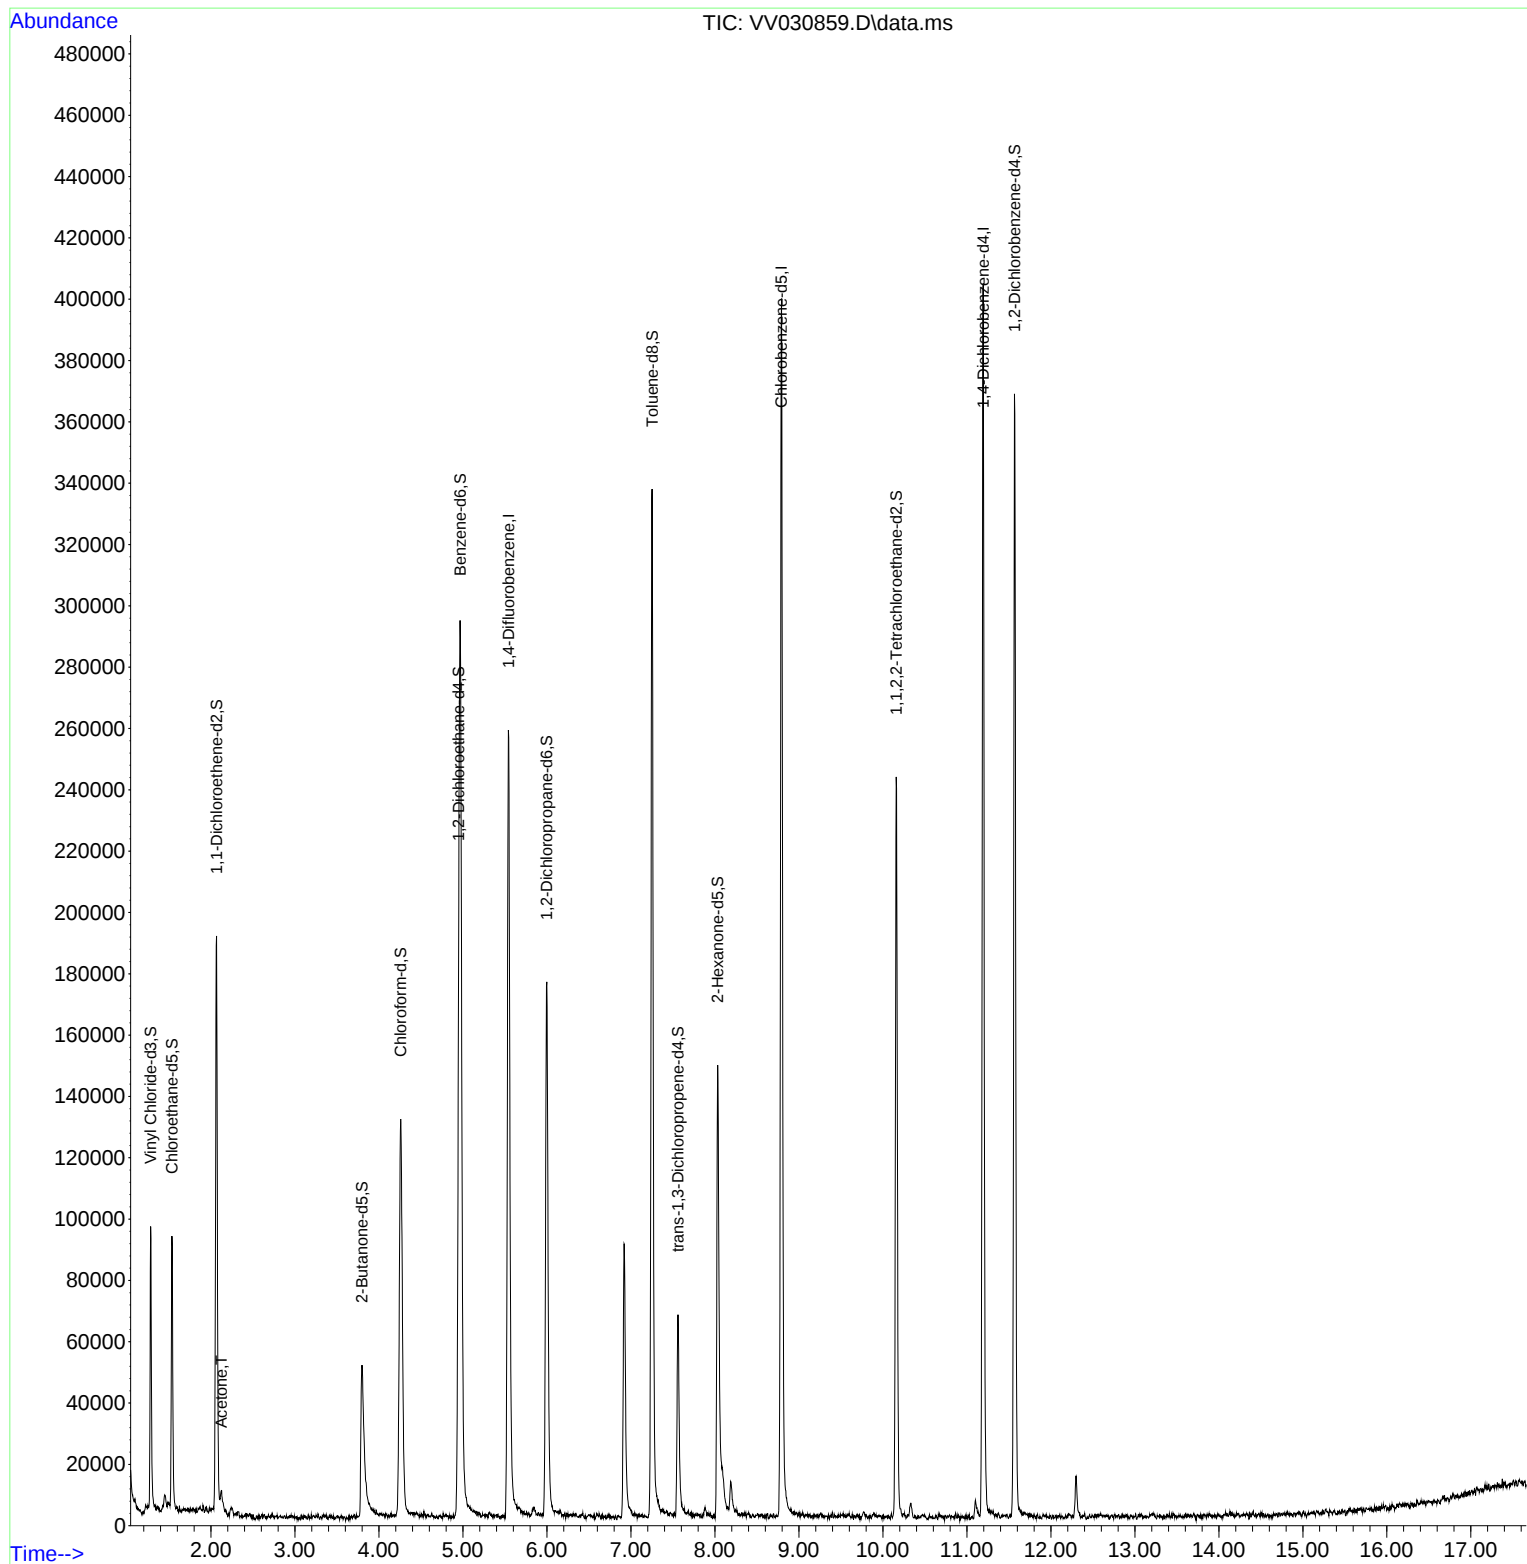

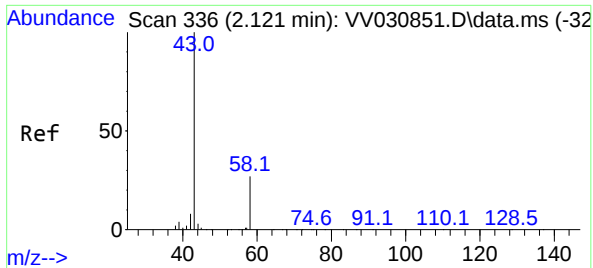

#13
 Acetone
 Concen: 4.940 ug/L
 RT: 2.124 min Scan# 31
 Delta R.T. -0.007 min
 Lab File: VV030859.D
 Acq: 26 Apr 2023 00:43

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AT2

Tgt Ion: 43 Resp: 6584
 Ion Ratio Lower Upper
 43 100
 58 21.7 0.0 52.8

