

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042523\
 Data File : VW030860.D
 Acq On : 26 Apr 2023 01:07
 Operator : SY/MD
 Sample : 02474-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COAT3

Quant Time: Apr 26 02:58:46 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Apr 22 00:43:23 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.542	114	216436	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.793	117	209970	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152	106261	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.282	65	61792	38.945	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	77.900%		
7) Chloroethane-d5	1.536	69	53543	40.270	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	80.540%		
11) 1,1-Dichloroethene-d2	2.063	65	31634	42.042	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	84.080%		
21) 2-Butanone-d5	3.799	46	81654	93.696	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	93.700%		
24) Chloroform-d	4.259	84	135828	47.238	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	94.480%		
26) 1,2-Dichloroethane-d4	4.950	65	96090	51.979	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	103.960%		
32) Benzene-d6	4.970	84	246018	49.558	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	99.120%		
36) 1,2-Dichloropropane-d6	5.995	67	75864	49.197	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	98.400%		
41) Toluene-d8	7.252	98	222199	47.672	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	95.340%		
43) trans-1,3-Dichloroprop...	7.558	79	36393	46.825	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	93.640%		
47) 2-Hexanone-d5	8.034	63	49135	80.885	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	80.880%		
56) 1,1,2,2-Tetrachloroeth...	10.159	84	104028	46.491	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	92.980%		
66) 1,2-Dichlorobenzene-d4	11.567	152	92642	54.851	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	109.700%		
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	6.921	75	2621	1.018	ug/L	# 29


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
Data File : VV030860.D
Acq On : 26 Apr 2023 01:07
Operator : SY/MD
Sample : 02474-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AT3

Quant Time: Apr 26 02:58:46 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Apr 22 00:43:23 2023
Response via : Initial Calibration

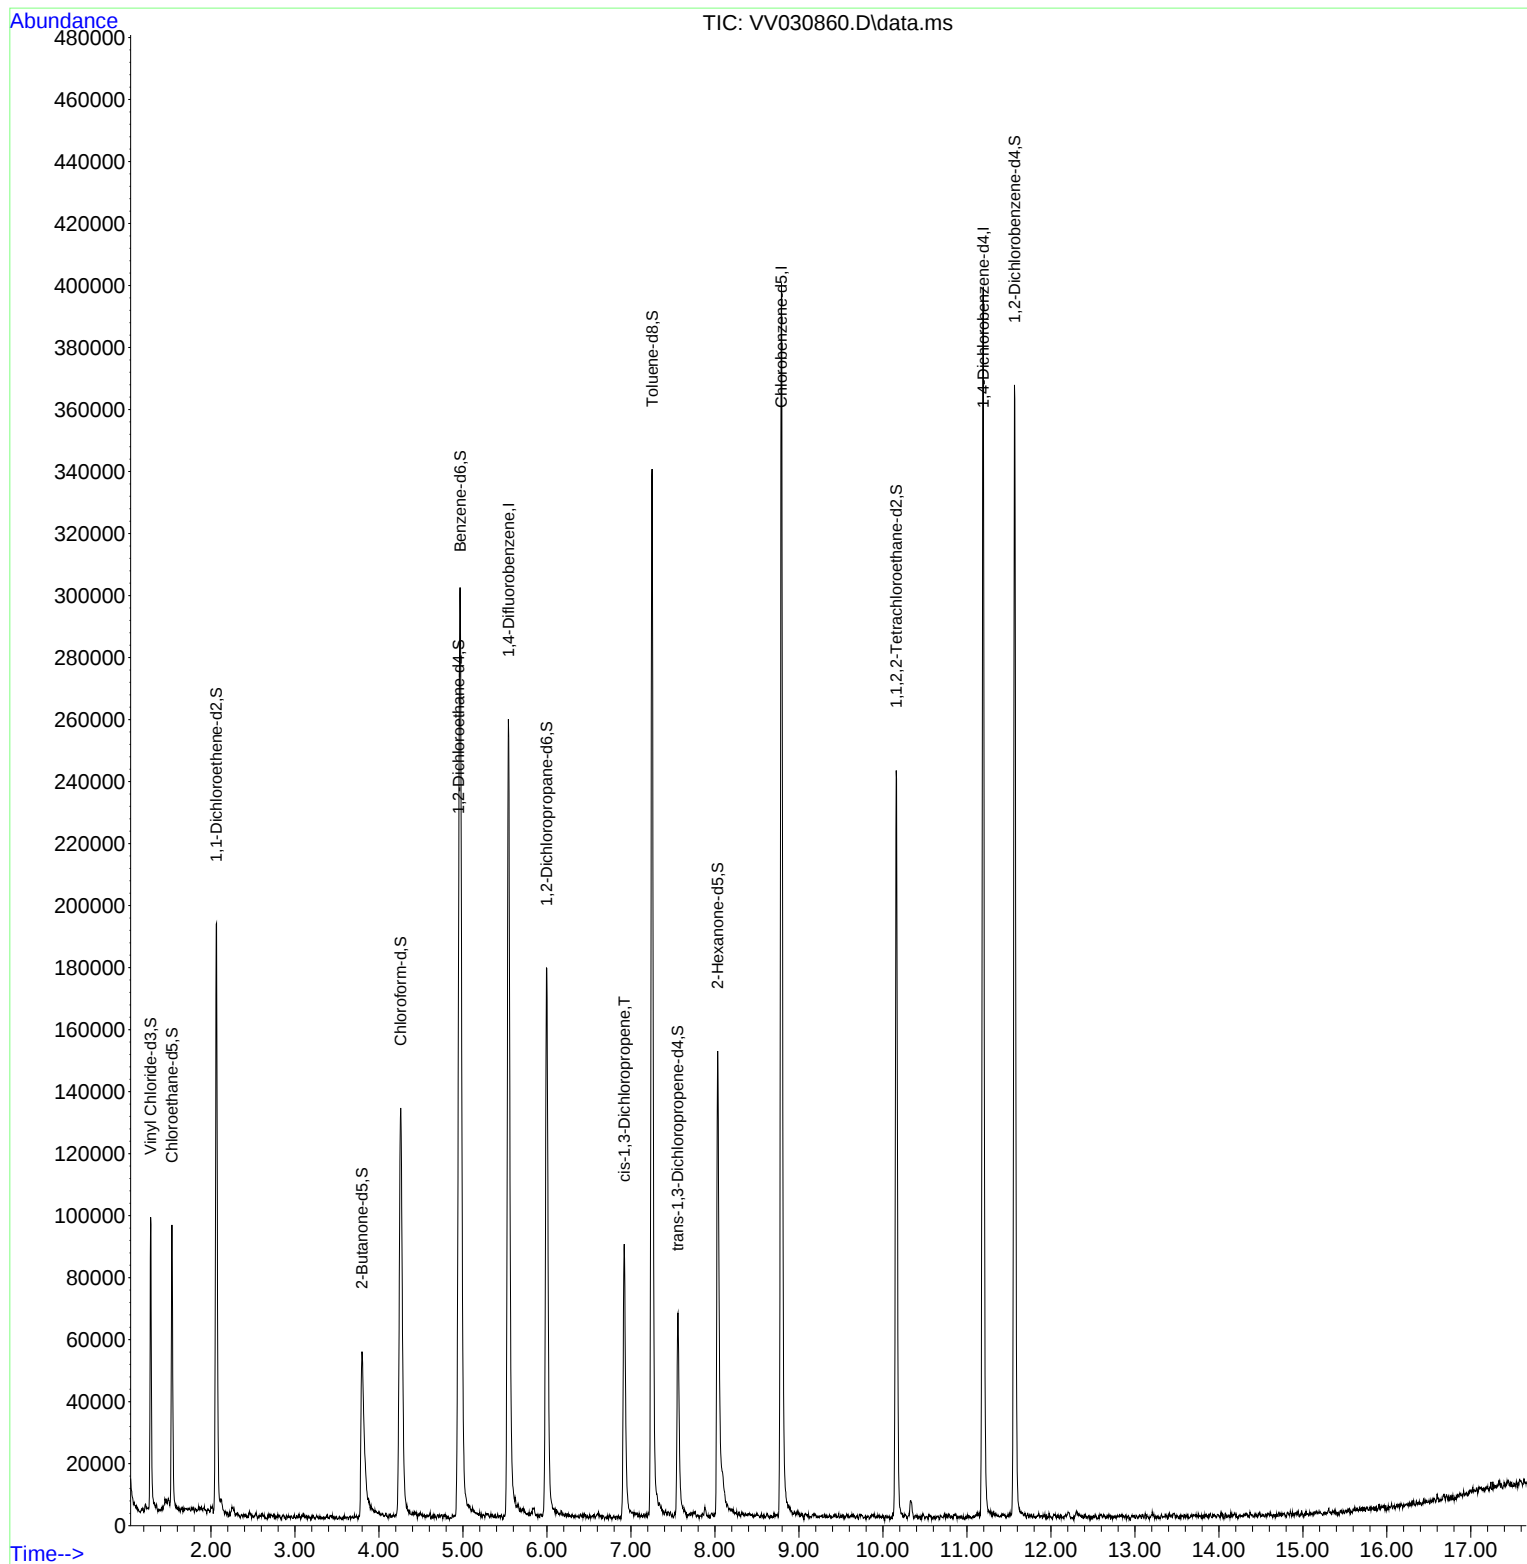

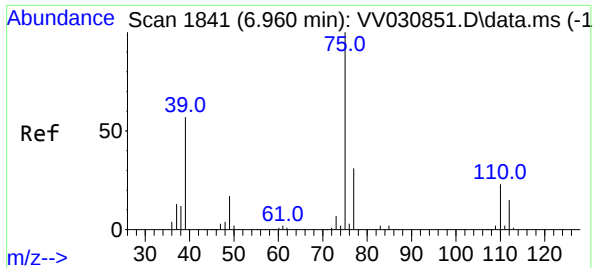

#39
cis-1,3-Dichloropropene
Concen: 1.018 ug/L
RT: 6.921 min Scan# 11
Delta R.T. -0.039 min
Lab File: VV030860.D
Acq: 26 Apr 2023 01:07

Instrument :
MSVOA_V
ClientSampleId :
C0AT3

Tgt Ion: 75 Resp: 2621
Ion Ratio Lower Upper
75 100
77 70.6 22.0 40.8#

