

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042523\
 Data File : VW030862.D
 Acq On : 26 Apr 2023 01:55
 Operator : SY/MD
 Sample : 02474-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AT5

Quant Time: Apr 26 02:59:00 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Apr 22 00:43:23 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.542	114	191691	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.793	117	191275	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152	94334	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.282	65	49971	35.560	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	71.120%
7) Chloroethane-d5	1.536	69	47835	40.621	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	81.240%
11) 1,1-Dichloroethene-d2	2.063	65	26214	39.336	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	78.680%
21) 2-Butanone-d5	3.796	46	83400	108.053	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	108.050%
24) Chloroform-d	4.259	84	122978	48.290	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	96.580%
26) 1,2-Dichloroethane-d4	4.950	65	87917	53.697	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	107.400%
32) Benzene-d6	4.970	84	218191	48.248	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	96.500%
36) 1,2-Dichloropropane-d6	5.998	67	68691	48.899	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	97.800%
41) Toluene-d8	7.252	98	197045	46.407	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	92.820%
43) trans-1,3-Dichloroprop...	7.561	79	33613	47.475	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	94.940%
47) 2-Hexanone-d5	8.034	63	50732	91.676	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	91.680%
56) 1,1,2,2-Tetrachloroeth...	10.159	84	99792	48.957	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	97.920%
66) 1,2-Dichlorobenzene-d4	11.567	152	82008	54.694	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	109.380%
Target Compounds						
39) cis-1,3-Dichloropropene	6.918	75	2675	1.140	ug/L	Qvalue 85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
Data File : VV030862.D
Acq On : 26 Apr 2023 01:55
Operator : SY/MD
Sample : 02474-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COAT5

Quant Time: Apr 26 02:59:00 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Apr 22 00:43:23 2023
Response via : Initial Calibration

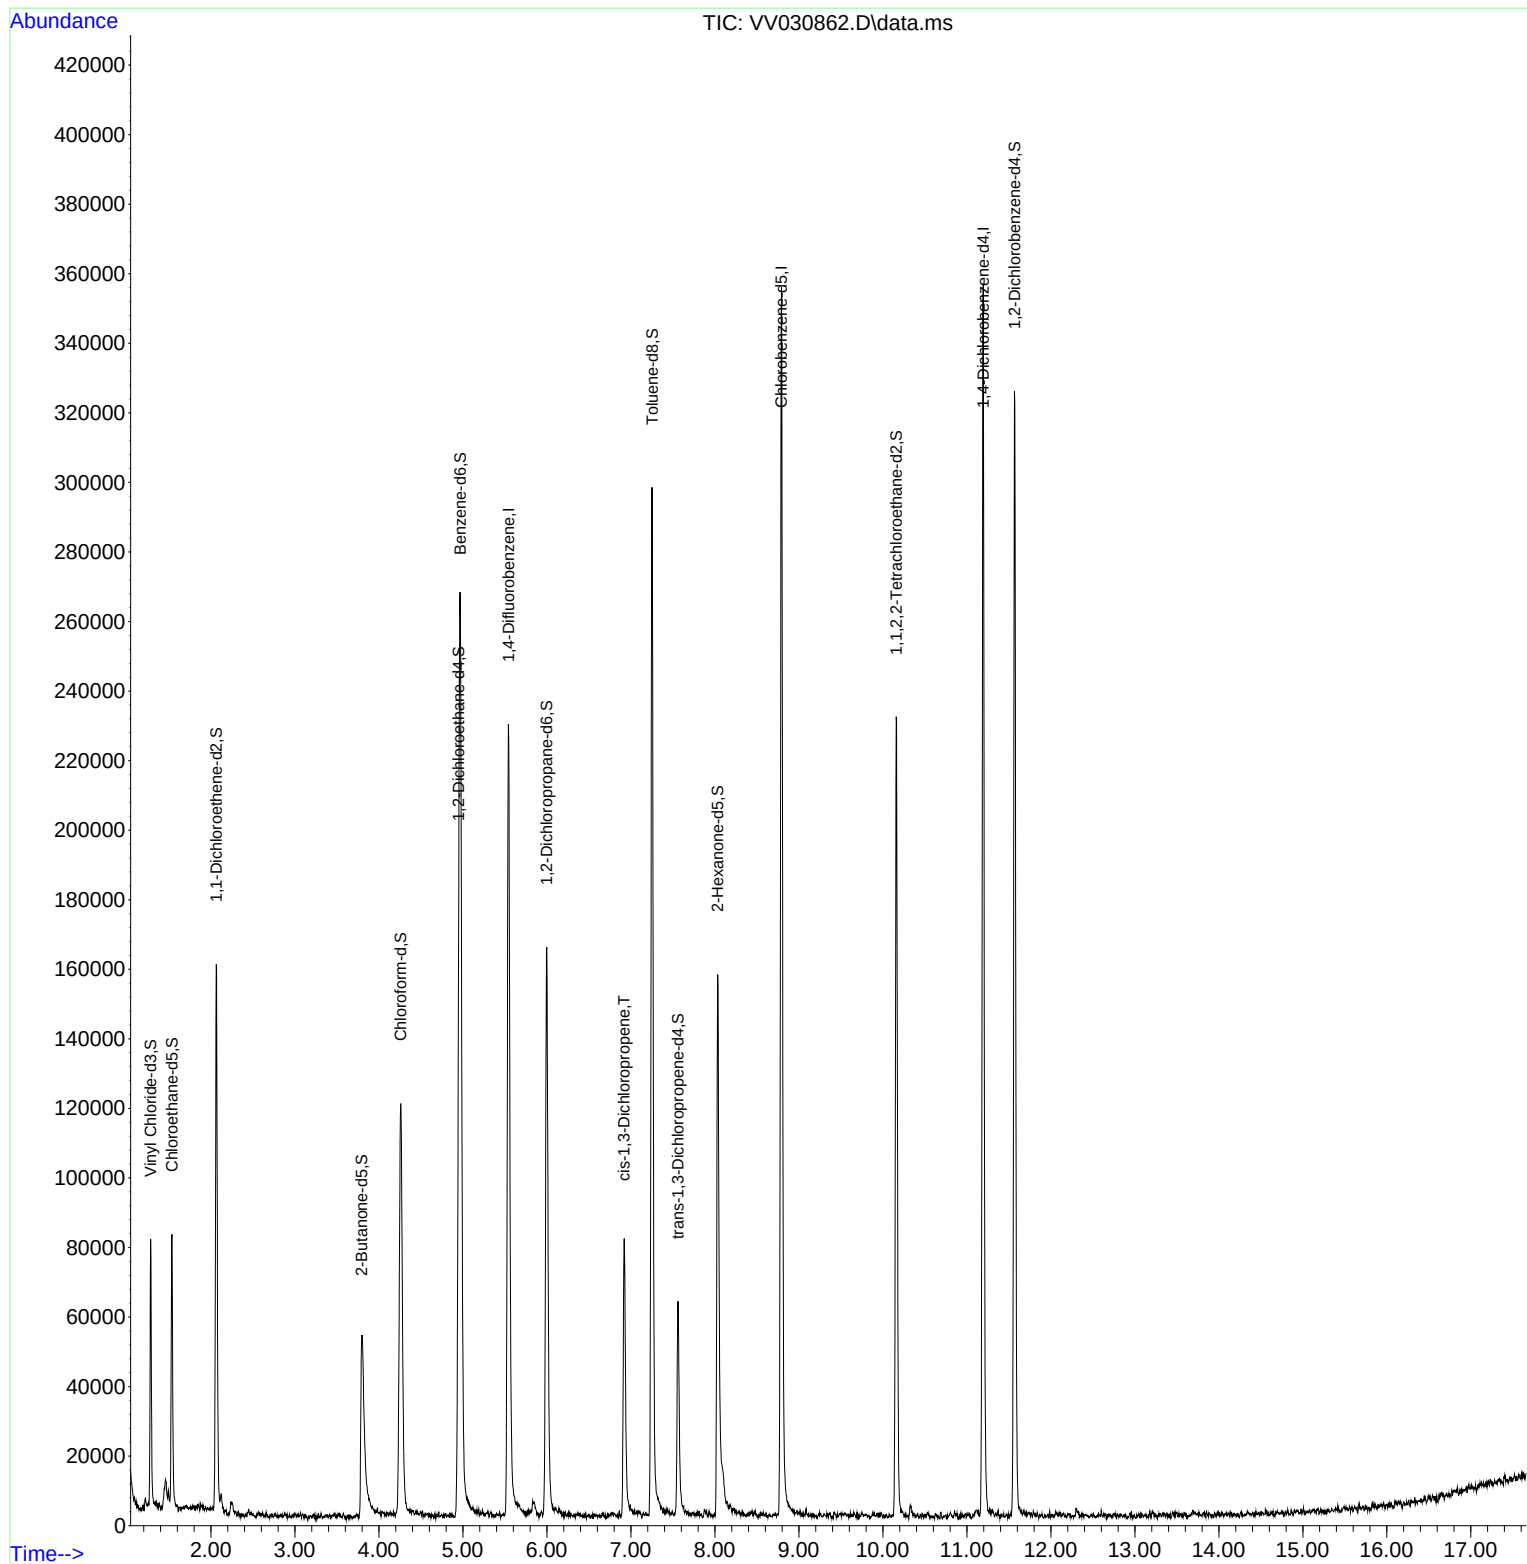

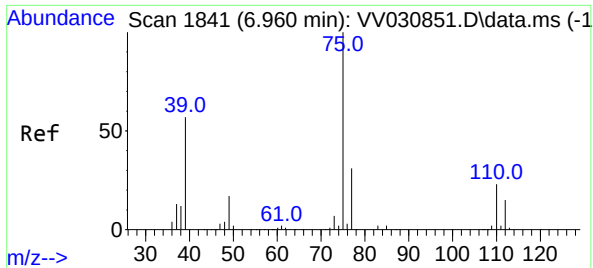

#39
 cis-1,3-Dichloropropene
 Concen: 1.140 ug/L
 RT: 6.918 min Scan# 11
 Delta R.T. -0.042 min
 Lab File: VV030862.D
 Acq: 26 Apr 2023 01:55

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AT5

Tgt Ion:	75	Resp:	2675
Ion	Ratio	Lower	Upper
75	100		
77	39.5	22.0	40.8

