

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
 Data File : VV030826.D
 Acq On : 25 Apr 2023 10:48
 Operator : SY/MD
 Sample : VV0425WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK334

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030826.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.285	69	76	89	rBV	105976	116545	13.68%	1.759%
2	1.535	148	154	166	rVB	96432	116105	13.63%	1.752%
3	2.063	309	318	331	rBV	206952	305624	35.88%	4.612%
4	2.494	451	452	454	rBV2	946	533	0.06%	0.008%
5	2.699	513	516	518	rBV4	1094	711	0.08%	0.011%
6	2.822	552	554	558	rBV5	1382	921	0.11%	0.014%
7	2.944	590	592	593	rBV2	1228	529	0.06%	0.008%
8	3.008	610	612	616	rVB4	1355	878	0.10%	0.013%
9	3.105	639	642	644	rBV4	1139	642	0.08%	0.010%
10	3.227	676	680	682	rBV5	1175	887	0.10%	0.013%
11	3.529	771	774	778	rBV6	556	543	0.06%	0.008%
12	3.606	795	798	800	rBV4	1407	748	0.09%	0.011%
13	3.732	835	837	841	rBV5	1118	998	0.12%	0.015%
14	3.799	847	858	884	rBV	52163	151516	17.79%	2.286%
15	4.256	988	1000	1027	rVB2	139380	349869	41.08%	5.279%
16	4.461	1059	1064	1068	rBV6	1969	1912	0.22%	0.029%
17	4.857	1183	1187	1190	rVB5	1542	982	0.12%	0.015%
18	4.963	1204	1220	1250	rBV2	313731	851691	100.00%	12.852%
19	5.307	1322	1327	1329	rBV5	1652	1642	0.19%	0.025%
20	5.355	1339	1342	1346	rBV6	1727	1365	0.16%	0.021%
21	5.384	1348	1351	1352	rBV3	955	514	0.06%	0.008%
22	5.542	1386	1400	1418	rBV	268340	560464	65.81%	8.457%
23	5.879	1504	1505	1508	rBV2	1402	780	0.09%	0.012%
24	5.995	1529	1541	1564	rBV	187228	382223	44.88%	5.768%
25	6.352	1650	1652	1655	rBV4	1310	872	0.10%	0.013%
26	6.493	1693	1696	1700	rBV6	840	519	0.06%	0.008%
27	6.757	1774	1778	1779	rBV3	619	479	0.06%	0.007%
28	6.767	1779	1781	1784	rVV4	1055	669	0.08%	0.010%
29	6.793	1786	1789	1792	rVV5	1355	879	0.10%	0.013%
30	6.847	1802	1806	1809	rBV5	1655	1307	0.15%	0.020%
31	6.918	1819	1828	1846	rBV	98813	184777	21.70%	2.788%
32	7.108	1885	1887	1891	rBV5	1381	768	0.09%	0.012%
33	7.172	1903	1907	1909	rBV4	1577	1125	0.13%	0.017%
34	7.249	1920	1931	1956	rBV	372871	664817	78.06%	10.032%
35	7.558	2019	2027	2047	rBV	70342	125386	14.72%	1.892%
36	7.883	2125	2128	2129	rBV2	997	511	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042523\
 Data File : VW030826.D
 Acq On : 25 Apr 2023 10:48
 Operator : SY/MD
 Sample : VW0425WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK334

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	8.034	2165	2175	2204	rBV	159174	328942	38.62%	4.964%
38	8.487	2314	2316	2317	rBV2	1622	790	0.09%	0.012%
39	8.564	2338	2340	2343	rBV4	1081	472	0.06%	0.007%
40	8.693	2376	2380	2381	rBV4	915	767	0.09%	0.012%
41	8.722	2386	2389	2393	rVB5	1114	795	0.09%	0.012%
42	8.754	2393	2399	2400	rBV5	1729	1561	0.18%	0.024%
43	8.792	2400	2411	2438	rVV	408637	691244	81.16%	10.431%
44	9.124	2511	2514	2515	rBV3	1380	681	0.08%	0.010%
45	9.165	2525	2527	2529	rBV3	1267	523	0.06%	0.008%
46	9.387	2593	2596	2597	rBV2	956	572	0.07%	0.009%
47	9.448	2611	2615	2617	rBV4	1181	836	0.10%	0.013%
48	9.468	2617	2621	2622	rBV4	1140	812	0.10%	0.012%
49	9.757	2709	2711	2714	rBV3	1022	498	0.06%	0.008%
50	9.776	2714	2717	2720	rBV5	1645	1007	0.12%	0.015%
51	9.821	2729	2731	2734	rVB2	1332	674	0.08%	0.010%
52	9.863	2739	2744	2746	rBV6	2161	2081	0.24%	0.031%
53	9.892	2750	2753	2755	rBV4	1740	812	0.10%	0.012%
54	10.159	2825	2836	2857	rVB	264879	405686	47.63%	6.122%
55	10.452	2925	2927	2930	rVB4	1102	678	0.08%	0.010%
56	10.577	2961	2966	2969	rBV5	1130	815	0.10%	0.012%
57	10.606	2973	2975	2979	rVB5	930	576	0.07%	0.009%
58	10.648	2986	2988	2992	rVB4	1132	695	0.08%	0.010%
59	10.709	3005	3007	3010	rVB3	1883	824	0.10%	0.012%
60	10.837	3045	3047	3049	rBV3	1237	562	0.07%	0.008%
61	10.918	3069	3072	3073	rBV2	1046	484	0.06%	0.007%
62	10.972	3086	3089	3091	rBV4	1416	890	0.10%	0.013%
63	11.014	3099	3102	3105	rBV5	1501	1047	0.12%	0.016%
64	11.053	3109	3114	3115	rBV3	1239	1030	0.12%	0.016%
65	11.095	3125	3127	3130	rBV3	841	599	0.07%	0.009%
66	11.191	3146	3157	3173	rBV	425423	675949	79.37%	10.200%
67	11.500	3249	3253	3256	rBV6	1269	1106	0.13%	0.017%
68	11.516	3256	3258	3261	rVB3	1384	692	0.08%	0.010%
69	11.567	3261	3274	3292	rBV	400831	643346	75.54%	9.708%
70	11.828	3352	3355	3358	rVB4	1324	745	0.09%	0.011%
71	11.953	3389	3394	3398	rVB7	1301	990	0.12%	0.015%
72	11.998	3405	3408	3412	rBV5	1384	1284	0.15%	0.019%
73	12.043	3417	3422	3424	rBV4	1210	1160	0.14%	0.018%
74	12.172	3461	3462	3468	rVB6	1480	1003	0.12%	0.015%
75	12.204	3468	3472	3475	rBV5	1438	1122	0.13%	0.017%
76	12.394	3527	3531	3533	rVB4	1051	627	0.07%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
 Data File : VV030826.D
 Acq On : 25 Apr 2023 10:48
 Operator : SY/MD
 Sample : VV0425WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK334

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	12.458	3548	3551	3553	rBV4	1073	737	0.09%	0.011%
78	12.522	3569	3571	3576	rBV6	1199	994	0.12%	0.015%
79	12.551	3579	3580	3583	rBV3	973	691	0.08%	0.010%
80	12.693	3618	3624	3627	rBV7	1134	1419	0.17%	0.021%
81	12.722	3630	3633	3635	rBV3	1411	774	0.09%	0.012%
82	12.805	3654	3659	3660	rBV4	1225	864	0.10%	0.013%
83	12.956	3704	3706	3712	rVB6	969	793	0.09%	0.012%
84	13.014	3720	3724	3727	rBV5	2275	1957	0.23%	0.030%
85	13.082	3741	3745	3746	rBV3	950	661	0.08%	0.010%
86	13.127	3757	3759	3764	rVB6	1260	1034	0.12%	0.016%
87	13.149	3764	3766	3769	rVB4	1309	480	0.06%	0.007%
88	13.165	3769	3771	3775	rBV3	771	607	0.07%	0.009%
89	13.307	3810	3815	3819	rBV8	1310	1465	0.17%	0.022%
90	13.352	3827	3829	3833	rVB5	1776	977	0.11%	0.015%
91	13.535	3883	3886	3888	rBV5	819	561	0.07%	0.008%
92	13.725	3943	3945	3948	rBV3	1193	625	0.07%	0.009%
93	13.908	3999	4002	4004	rBV4	2096	1349	0.16%	0.020%
94	14.178	4084	4086	4087	rBV2	1168	495	0.06%	0.007%
95	14.268	4112	4114	4116	rBV3	1233	484	0.06%	0.007%
96	14.329	4131	4133	4137	rBV5	1238	795	0.09%	0.012%
97	14.384	4148	4150	4155	rBV6	1084	820	0.10%	0.012%
98	14.406	4155	4157	4160	rBV3	1365	858	0.10%	0.013%
99	14.474	4176	4178	4181	rBV4	1765	1018	0.12%	0.015%
100	14.721	4252	4255	4256	rBV3	1675	903	0.11%	0.014%




Sum of corrected areas: 6627069

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
Data File : VV030826.D
Acq On : 25 Apr 2023 10:48
Operator : SY/MD
Sample : VV0425WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK334

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

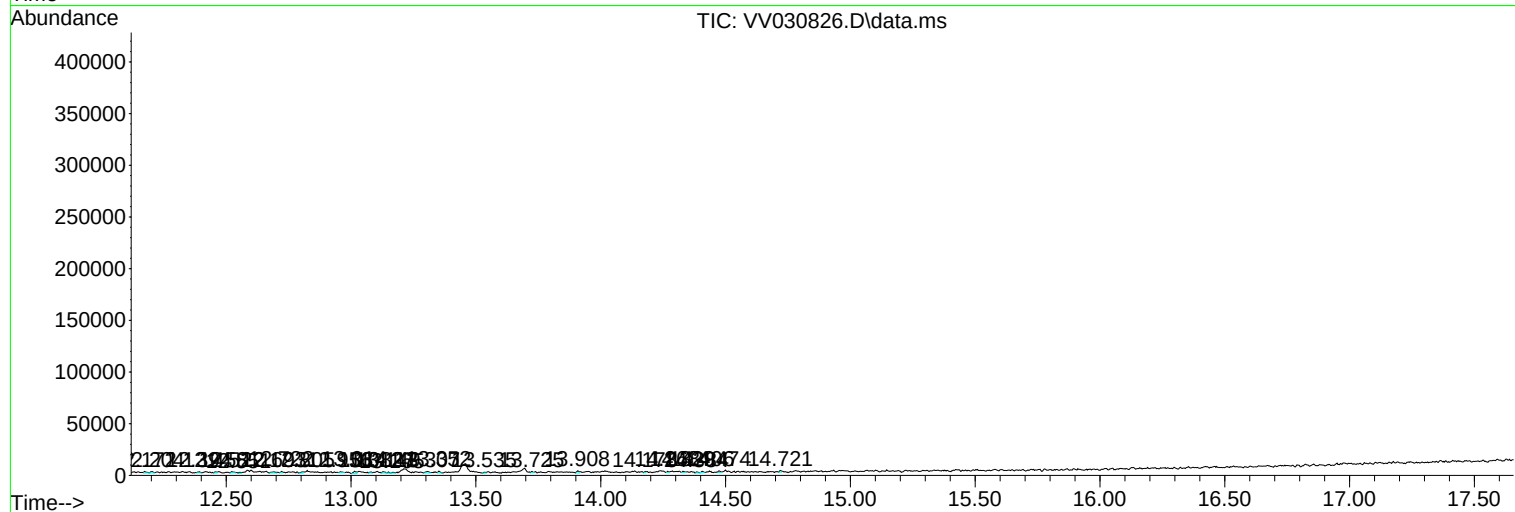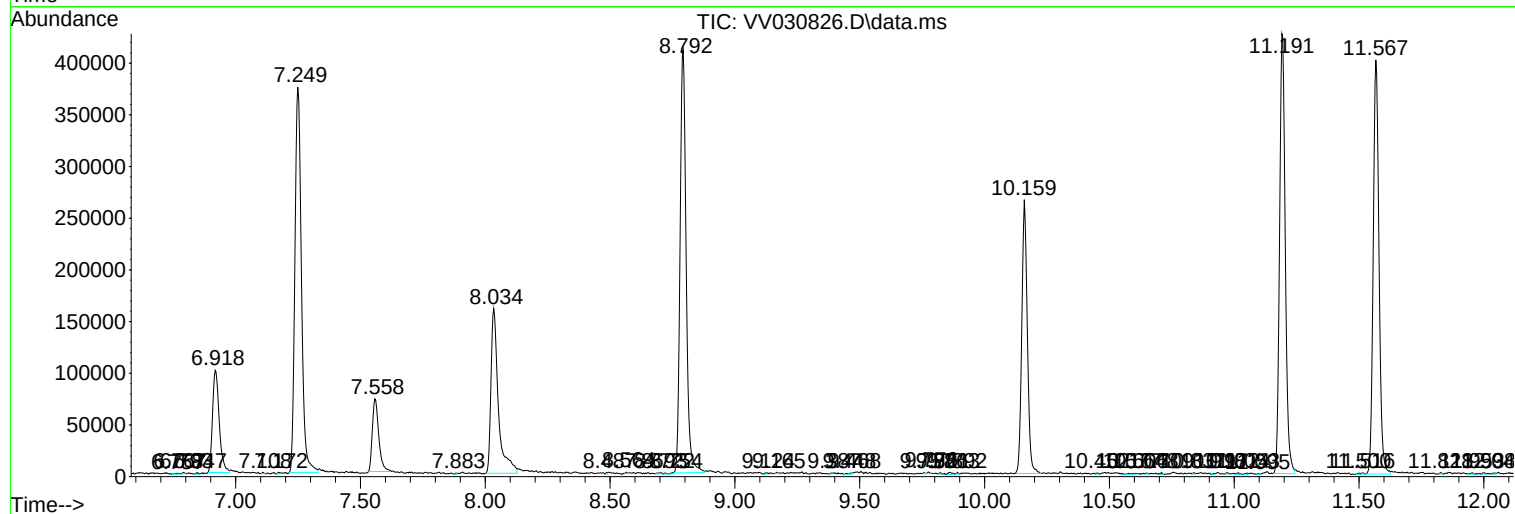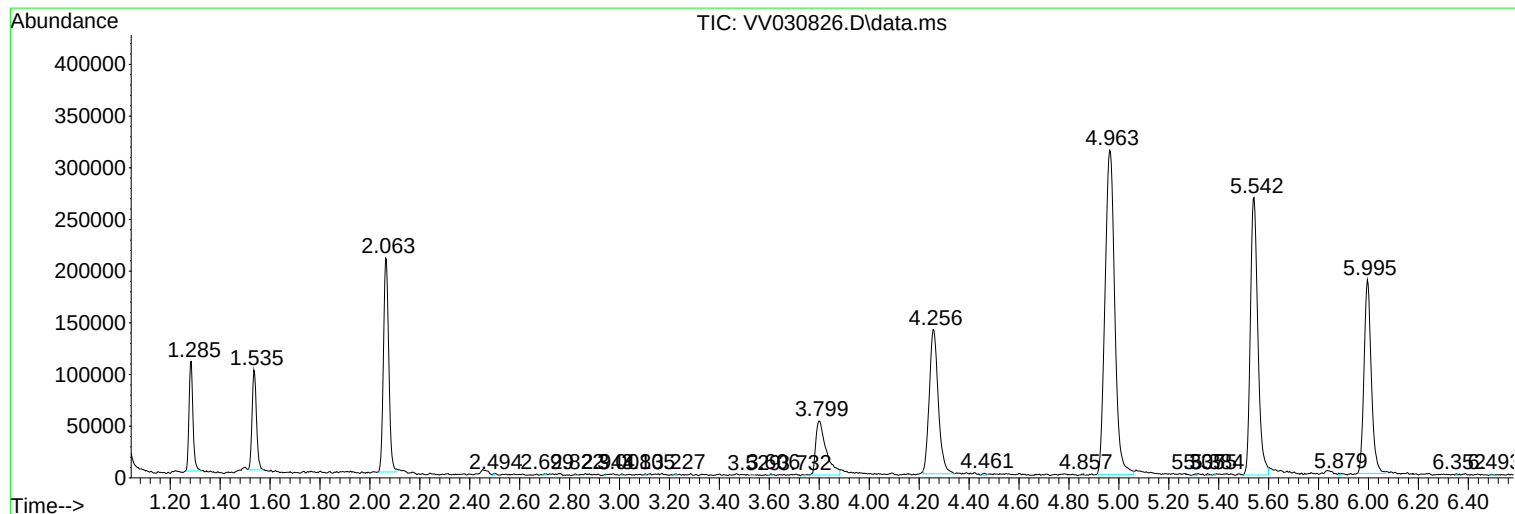

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
Data File : VV030826.D
Acq On : 25 Apr 2023 10:48
Operator : SY/MD
Sample : VV0425WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK334

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
Data File : VV030826.D
Acq On : 25 Apr 2023 10:48
Operator : SY/MD
Sample : VV0425WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK334

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------