

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
 Data File : VV030828.D
 Acq On : 25 Apr 2023 11:41
 Operator : SY/MD
 Sample : 02419-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M

Title : VOC Analysis

Signal : TIC: VV030828.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.285	69	76	84	rBV	98387	104463	12.80%	1.659%
2	1.535	148	154	168	rVB	91468	111278	13.63%	1.767%
3	2.066	310	319	334	rVB	187528	273320	33.49%	4.341%
4	2.259	376	379	385	rBV6	2027	1318	0.16%	0.021%
5	2.458	434	441	448	rBV6	4789	7152	0.88%	0.114%
6	2.510	455	457	462	rVB5	1131	841	0.10%	0.013%
7	2.532	462	464	466	rBV3	1141	608	0.07%	0.010%
8	2.597	482	484	487	rVB5	1252	652	0.08%	0.010%
9	2.622	489	492	495	rBV5	1045	1062	0.13%	0.017%
10	2.648	498	500	505	rVB6	1490	949	0.12%	0.015%
11	2.809	548	550	553	rBV4	1548	882	0.11%	0.014%
12	2.847	558	562	563	rBV3	1007	756	0.09%	0.012%
13	2.876	567	571	572	rVB3	1219	702	0.09%	0.011%
14	2.889	572	575	578	rBV4	1130	879	0.11%	0.014%
15	2.921	583	585	589	rBV5	1236	791	0.10%	0.013%
16	3.002	607	610	613	rBV4	1103	682	0.08%	0.011%
17	3.079	630	634	637	rBV4	1539	1404	0.17%	0.022%
18	3.259	687	690	693	rBV4	1008	676	0.08%	0.011%
19	3.349	715	718	719	rBV3	966	605	0.07%	0.010%
20	3.416	732	739	744	rVV10	1425	1902	0.23%	0.030%
21	3.471	754	756	759	rVB3	1145	592	0.07%	0.009%
22	3.606	795	798	804	rBV6	1249	1099	0.13%	0.017%
23	3.664	815	816	819	rBV3	969	587	0.07%	0.009%
24	3.757	842	845	847	rBV4	1011	599	0.07%	0.010%
25	3.799	848	858	878	rBV2	51206	137187	16.81%	2.179%
26	4.259	987	1001	1029	rVB	133327	334949	41.04%	5.320%
27	4.735	1145	1149	1152	rBV5	1024	878	0.11%	0.014%
28	4.966	1205	1221	1249	rBV2	306262	816165	100.00%	12.963%
29	5.542	1387	1400	1424	rBV	253959	535842	65.65%	8.510%
30	5.883	1504	1506	1508	rBV3	1420	752	0.09%	0.012%
31	5.998	1530	1542	1563	rBV	183446	373551	45.77%	5.933%
32	6.230	1611	1614	1616	rBV4	1382	999	0.12%	0.016%
33	6.284	1629	1631	1633	rBV2	1470	602	0.07%	0.010%
34	6.503	1697	1699	1702	rBV4	1454	993	0.12%	0.016%
35	6.690	1754	1757	1758	rBV2	1331	782	0.10%	0.012%
36	6.799	1788	1791	1795	rBV5	1625	1451	0.18%	0.023%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
 Data File : VV030828.D
 Acq On : 25 Apr 2023 11:41
 Operator : SY/MD
 Sample : 02419-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	6.857	1807	1809	1812	rBV3	1092	696	0.09%	0.011%
38	6.921	1819	1829	1848	rBV	97518	176744	21.66%	2.807%
39	7.120	1888	1891	1892	rBV3	1393	723	0.09%	0.011%
40	7.252	1920	1932	1953	rBV	345954	616512	75.54%	9.792%
41	7.561	2016	2028	2041	rBV	70641	127515	15.62%	2.025%
42	7.834	2109	2113	2114	rBV4	1063	670	0.08%	0.011%
43	7.902	2132	2134	2136	rBV3	1239	739	0.09%	0.012%
44	7.976	2154	2157	2158	rBV2	1416	763	0.09%	0.012%
45	8.034	2166	2175	2204	rBV	156755	309964	37.98%	4.923%
46	8.471	2308	2311	2314	rBV5	1260	937	0.11%	0.015%
47	8.590	2346	2348	2351	rVB4	1324	642	0.08%	0.010%
48	8.612	2351	2355	2358	rVB6	1368	1133	0.14%	0.018%
49	8.628	2358	2360	2362	rBV3	1507	744	0.09%	0.012%
50	8.657	2367	2369	2371	rVB3	1735	616	0.08%	0.010%
51	8.680	2373	2376	2379	rBV4	891	739	0.09%	0.012%
52	8.731	2390	2392	2396	rBV5	914	767	0.09%	0.012%
53	8.792	2399	2411	2434	rBV	390267	660954	80.98%	10.498%
54	9.140	2517	2519	2524	rVB6	1431	843	0.10%	0.013%
55	9.169	2524	2528	2531	rBV6	1488	1442	0.18%	0.023%
56	9.339	2578	2581	2583	rBV4	1394	690	0.08%	0.011%
57	9.407	2598	2602	2605	rBV6	962	583	0.07%	0.009%
58	9.686	2687	2689	2692	rBV4	1374	953	0.12%	0.015%
59	9.735	2699	2704	2706	rBV6	1353	856	0.10%	0.014%
60	10.056	2802	2804	2807	rVB4	1461	770	0.09%	0.012%
61	10.088	2809	2814	2817	rBV6	950	861	0.11%	0.014%
62	10.117	2821	2823	2825	rVV3	1586	710	0.09%	0.011%
63	10.159	2826	2836	2857	rVB	247647	402325	49.29%	6.390%
64	10.394	2906	2909	2912	rBV5	1040	845	0.10%	0.013%
65	10.564	2958	2962	2965	rBV6	1104	840	0.10%	0.013%
66	10.632	2979	2983	2986	rBV4	1442	1276	0.16%	0.020%
67	10.779	3026	3029	3032	rBV4	1119	936	0.11%	0.015%
68	10.841	3046	3048	3050	rVB3	1306	627	0.08%	0.010%
69	10.863	3050	3055	3057	rBV5	1941	1844	0.23%	0.029%
70	11.024	3101	3105	3106	rBV4	1103	642	0.08%	0.010%
71	11.082	3121	3123	3130	rVB6	1886	1257	0.15%	0.020%
72	11.127	3133	3137	3140	rBV6	1451	1137	0.14%	0.018%
73	11.191	3146	3157	3178	rBV	397454	633781	77.65%	10.066%
74	11.455	3236	3239	3240	rBV2	1169	661	0.08%	0.010%
75	11.525	3258	3261	3262	rBV2	1391	787	0.10%	0.012%
76	11.567	3263	3274	3294	rVV	371091	597964	73.27%	9.497%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
 Data File : VV030828.D
 Acq On : 25 Apr 2023 11:41
 Operator : SY/MD
 Sample : 02419-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	11.705	3315	3317	3321	rBV4	1309	970	0.12%	0.015%
78	11.947	3388	3392	3396	rBV5	935	857	0.11%	0.014%
79	12.017	3411	3414	3416	rBV3	1438	856	0.10%	0.014%
80	12.191	3464	3468	3470	rBV4	1120	738	0.09%	0.012%
81	12.246	3481	3485	3488	rBV6	1082	919	0.11%	0.015%
82	12.323	3506	3509	3510	rBV3	957	573	0.07%	0.009%
83	12.458	3546	3551	3553	rBV5	1818	1622	0.20%	0.026%
84	12.702	3619	3627	3629	rBV7	1640	2024	0.25%	0.032%
85	12.918	3692	3694	3696	rBV3	981	582	0.07%	0.009%
86	12.998	3713	3719	3722	rBV4	1303	1650	0.20%	0.026%
87	13.053	3734	3736	3739	rBV4	777	561	0.07%	0.009%
88	13.143	3762	3764	3769	rVB6	1320	897	0.11%	0.014%
89	13.204	3781	3783	3789	rVB6	1350	1106	0.14%	0.018%
90	13.294	3805	3811	3816	rBV8	1290	1653	0.20%	0.026%
91	13.345	3825	3827	3831	rBV4	1298	1029	0.13%	0.016%
92	13.384	3836	3839	3842	rBV4	1414	822	0.10%	0.013%
93	13.541	3883	3888	3891	rVV4	878	718	0.09%	0.011%
94	13.783	3961	3963	3965	rBV2	1092	582	0.07%	0.009%
95	13.873	3985	3991	3993	rBV7	1319	1351	0.17%	0.021%
96	13.972	4019	4022	4025	rVB3	1435	783	0.10%	0.012%
97	14.265	4109	4113	4114	rBV3	1717	1271	0.16%	0.020%
98	14.355	4139	4141	4143	rBV2	1643	721	0.09%	0.011%
99	14.667	4236	4238	4241	rBV3	1513	861	0.11%	0.014%
100	14.795	4275	4278	4281	rBV4	1912	1662	0.20%	0.026%




Sum of corrected areas: 6296246

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
Data File : VV030828.D
Acq On : 25 Apr 2023 11:41
Operator : SY/MD
Sample : 02419-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

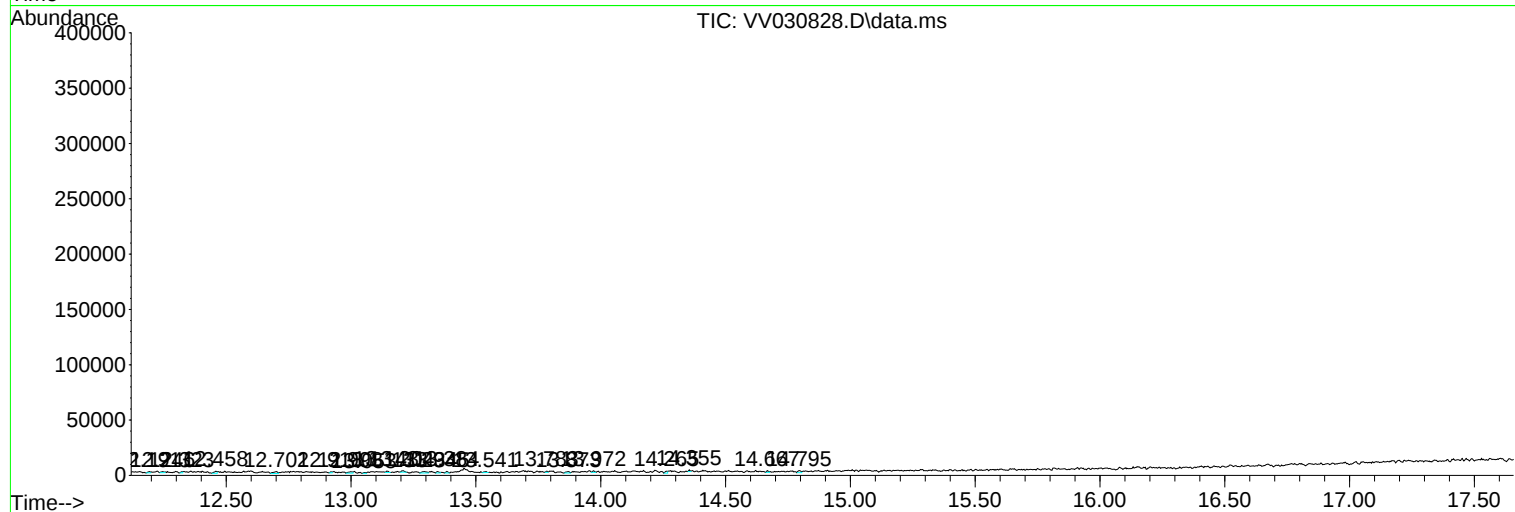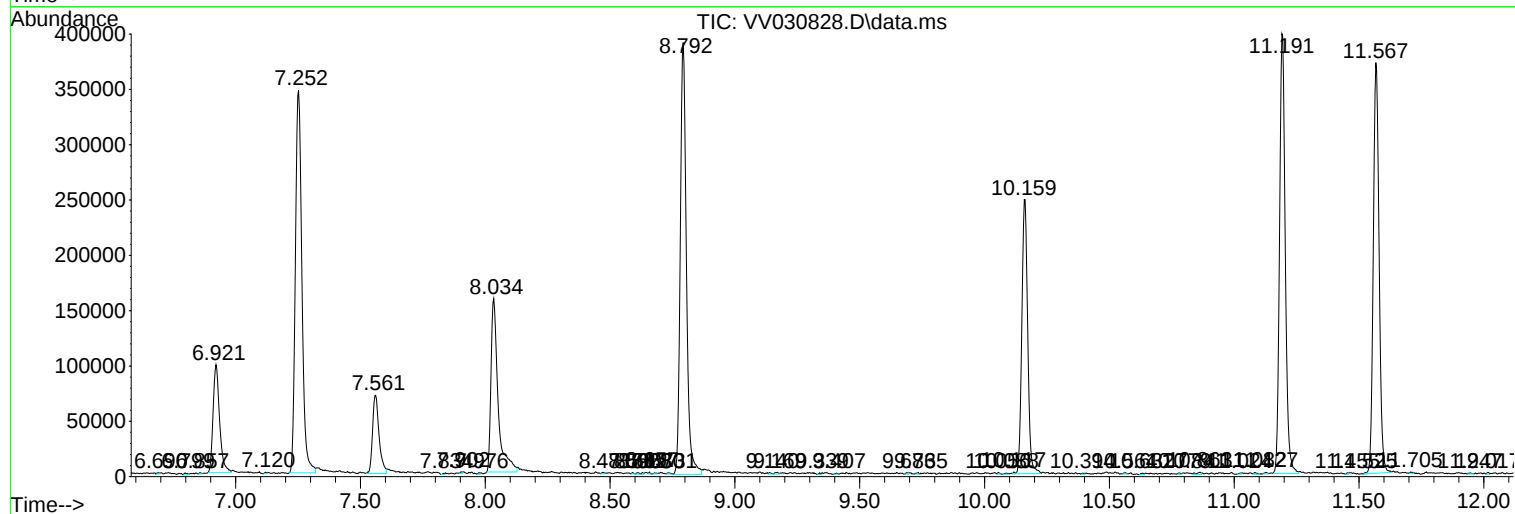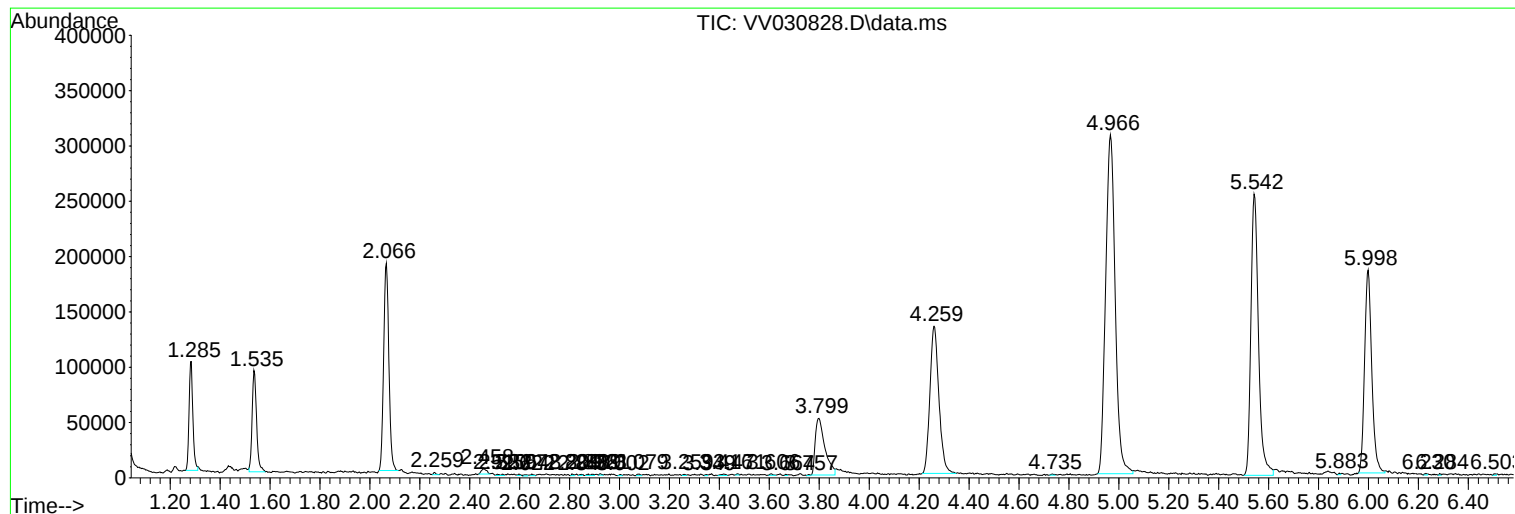

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
Data File : VV030828.D
Acq On : 25 Apr 2023 11:41
Operator : SY/MD
Sample : 02419-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
Data File : VV030828.D
Acq On : 25 Apr 2023 11:41
Operator : SY/MD
Sample : 02419-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc