

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
 Data File : VV030842.D
 Acq On : 25 Apr 2023 17:16
 Operator : SY/MD
 Sample : 02475-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AW9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030842.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.285	70	76	90	rVB	101297	109657	13.31%	1.714%
2	1.535	148	154	168	rVB	88020	113156	13.74%	1.768%
3	2.066	310	319	335	rBV	199071	288850	35.07%	4.514%
4	2.500	450	454	459	rBV7	1598	1476	0.18%	0.023%
5	2.564	472	474	476	rBV3	1256	776	0.09%	0.012%
6	2.645	496	499	501	rBV4	1771	1079	0.13%	0.017%
7	2.703	515	517	520	rBV4	1302	794	0.10%	0.012%
8	2.719	520	522	524	rBV3	1164	682	0.08%	0.011%
9	2.748	529	531	534	rBV4	981	797	0.10%	0.012%
10	2.796	539	546	547	rBV5	1608	1586	0.19%	0.025%
11	2.863	563	567	568	rBV3	1301	971	0.12%	0.015%
12	2.924	583	586	587	rBV3	1242	645	0.08%	0.010%
13	2.995	606	608	609	rBV2	889	487	0.06%	0.008%
14	3.053	624	626	627	rBV3	707	380	0.05%	0.006%
15	3.088	635	637	640	rBV4	956	489	0.06%	0.008%
16	3.185	663	667	669	rBV4	1073	942	0.11%	0.015%
17	3.288	695	699	700	rBV4	1174	886	0.11%	0.014%
18	3.506	764	767	769	rBV3	1345	925	0.11%	0.014%
19	3.519	769	771	774	rVB4	1129	593	0.07%	0.009%
20	3.548	774	780	782	rBV6	1215	1378	0.17%	0.022%
21	3.590	789	793	798	rBV7	1925	2446	0.30%	0.038%
22	3.661	812	815	818	rVB4	1436	818	0.10%	0.013%
23	3.680	818	821	823	rBV4	1153	540	0.07%	0.008%
24	3.741	837	840	842	rBV4	1750	1199	0.15%	0.019%
25	3.799	849	858	879	rBV	53070	146678	17.81%	2.292%
26	4.259	985	1001	1027	rBV2	134917	347905	42.24%	5.437%
27	4.619	1111	1113	1117	rVB4	1636	1056	0.13%	0.017%
28	4.654	1122	1124	1126	rBV3	958	493	0.06%	0.008%
29	4.966	1204	1221	1245	rBV2	307349	823703	100.00%	12.872%
30	5.249	1306	1309	1312	rBV4	1393	992	0.12%	0.016%
31	5.391	1349	1353	1356	rBV5	1452	980	0.12%	0.015%
32	5.436	1365	1367	1371	rVB3	1989	1041	0.13%	0.016%
33	5.542	1388	1400	1422	rBV	265009	548655	66.61%	8.574%
34	5.998	1530	1542	1562	rBV	183432	370369	44.96%	5.788%
35	6.259	1620	1623	1624	rBV3	1402	681	0.08%	0.011%
36	6.468	1685	1688	1690	rBV4	1314	927	0.11%	0.014%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042523\
 Data File : VW030842.D
 Acq On : 25 Apr 2023 17:16
 Operator : SY/MD
 Sample : 02475-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AW9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	6.542	1709	1711	1713	rBV2	985	484	0.06%	0.008%
38	6.674	1749	1752	1753	rBV2	1740	910	0.11%	0.014%
39	6.747	1772	1775	1776	rBV3	1186	675	0.08%	0.011%
40	6.921	1819	1829	1849	rBV	94120	177581	21.56%	2.775%
41	7.252	1920	1932	1954	rBV	351716	630989	76.60%	9.861%
42	7.490	2003	2006	2008	rBV4	1316	725	0.09%	0.011%
43	7.561	2019	2028	2045	rBV	70118	122256	14.84%	1.911%
44	7.821	2105	2109	2110	rBV4	2037	995	0.12%	0.016%
45	7.998	2161	2164	2165	rBV3	1144	576	0.07%	0.009%
46	8.034	2166	2175	2205	rVV	157063	318423	38.66%	4.976%
47	8.288	2252	2254	2256	rBV4	1406	705	0.09%	0.011%
48	8.471	2309	2311	2313	rBV3	1626	607	0.07%	0.009%
49	8.664	2369	2371	2375	rBV4	1074	427	0.05%	0.007%
50	8.715	2385	2387	2388	rBV2	909	395	0.05%	0.006%
51	8.792	2400	2411	2432	rBV	413663	677061	82.20%	10.581%
52	9.050	2488	2491	2494	rBV5	1709	755	0.09%	0.012%
53	9.239	2548	2550	2553	rBV4	1266	666	0.08%	0.010%
54	9.265	2556	2558	2560	rVB3	1552	719	0.09%	0.011%
55	9.284	2560	2564	2568	rBV6	1190	1058	0.13%	0.017%
56	9.323	2574	2576	2578	rBV3	892	513	0.06%	0.008%
57	9.339	2578	2581	2584	rBV5	1220	811	0.10%	0.013%
58	9.432	2607	2610	2611	rBV3	974	574	0.07%	0.009%
59	9.850	2735	2740	2743	rBV7	1277	1447	0.18%	0.023%
60	9.908	2755	2758	2762	rVB6	1740	1480	0.18%	0.023%
61	10.085	2809	2813	2814	rBV4	1130	726	0.09%	0.011%
62	10.162	2826	2837	2856	rVV	247018	397051	48.20%	6.205%
63	10.538	2951	2954	2957	rVB3	2164	1414	0.17%	0.022%
64	10.564	2957	2962	2964	rBV6	1243	868	0.11%	0.014%
65	10.577	2964	2966	2969	rBV3	1418	825	0.10%	0.013%
66	10.667	2991	2994	2996	rBV4	1005	671	0.08%	0.010%
67	10.686	2998	3000	3003	rVB3	1720	903	0.11%	0.014%
68	10.747	3018	3019	3024	rVB5	963	547	0.07%	0.009%
69	10.860	3051	3054	3055	rBV3	1162	537	0.07%	0.008%
70	10.924	3072	3074	3077	rBV4	733	399	0.05%	0.006%
71	10.940	3077	3079	3082	rBV3	1021	533	0.06%	0.008%
72	11.194	3145	3158	3176	rBV	413994	653860	79.38%	10.218%
73	11.394	3218	3220	3226	rVB6	1859	1244	0.15%	0.019%
74	11.471	3240	3244	3247	rBV6	1243	1145	0.14%	0.018%
75	11.570	3263	3275	3291	rBV	374588	605607	73.52%	9.464%
76	11.744	3326	3329	3331	rBV3	1036	481	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
 Data File : VV030842.D
 Acq On : 25 Apr 2023 17:16
 Operator : SY/MD
 Sample : 02475-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AW9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	11.760	3331	3334	3335	rBV2	991	601	0.07%	0.009%
78	11.911	3377	3381	3383	rBV4	1152	940	0.11%	0.015%
79	11.947	3390	3392	3395	rBV4	1246	716	0.09%	0.011%
80	11.963	3395	3397	3399	rBV3	971	377	0.05%	0.006%
81	12.059	3424	3427	3428	rBV3	1101	603	0.07%	0.009%
82	12.085	3433	3435	3440	rVV6	1156	1023	0.12%	0.016%
83	12.114	3440	3444	3447	rVB4	1220	1049	0.13%	0.016%
84	12.133	3447	3450	3453	rBV4	847	576	0.07%	0.009%
85	12.178	3463	3464	3466	rBV2	958	537	0.07%	0.008%
86	12.271	3490	3493	3494	rBV3	911	498	0.06%	0.008%
87	12.461	3549	3552	3555	rVV4	1202	755	0.09%	0.012%
88	12.490	3558	3561	3563	rBV3	922	619	0.08%	0.010%
89	12.577	3586	3588	3590	rBV3	927	540	0.07%	0.008%
90	12.648	3608	3610	3612	rBV3	1049	481	0.06%	0.008%
91	13.043	3729	3733	3734	rBV3	940	654	0.08%	0.010%
92	13.165	3768	3771	3773	rVB3	1231	663	0.08%	0.010%
93	13.213	3780	3786	3787	rBV6	1299	1289	0.16%	0.020%
94	13.432	3852	3854	3856	rBV2	1157	677	0.08%	0.011%
95	13.792	3963	3966	3970	rVB5	1380	642	0.08%	0.010%
96	13.963	4017	4019	4020	rBV	1154	440	0.05%	0.007%
97	14.046	4043	4045	4048	rVB4	1638	833	0.10%	0.013%
98	14.088	4056	4058	4062	rBV4	1236	774	0.09%	0.012%
99	14.107	4062	4064	4066	rBV3	1048	482	0.06%	0.008%
100	14.294	4120	4122	4125	rBV3	1099	501	0.06%	0.008%




Sum of corrected areas: 6398945

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
Data File : VV030842.D
Acq On : 25 Apr 2023 17:16
Operator : SY/MD
Sample : 02475-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AW9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

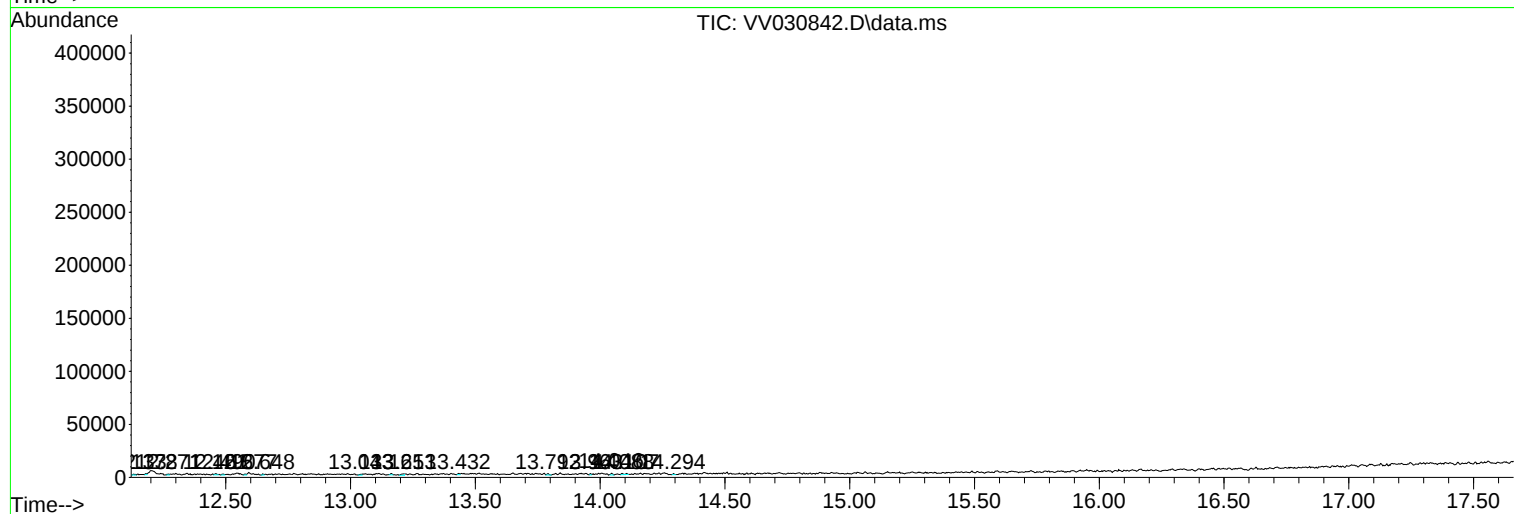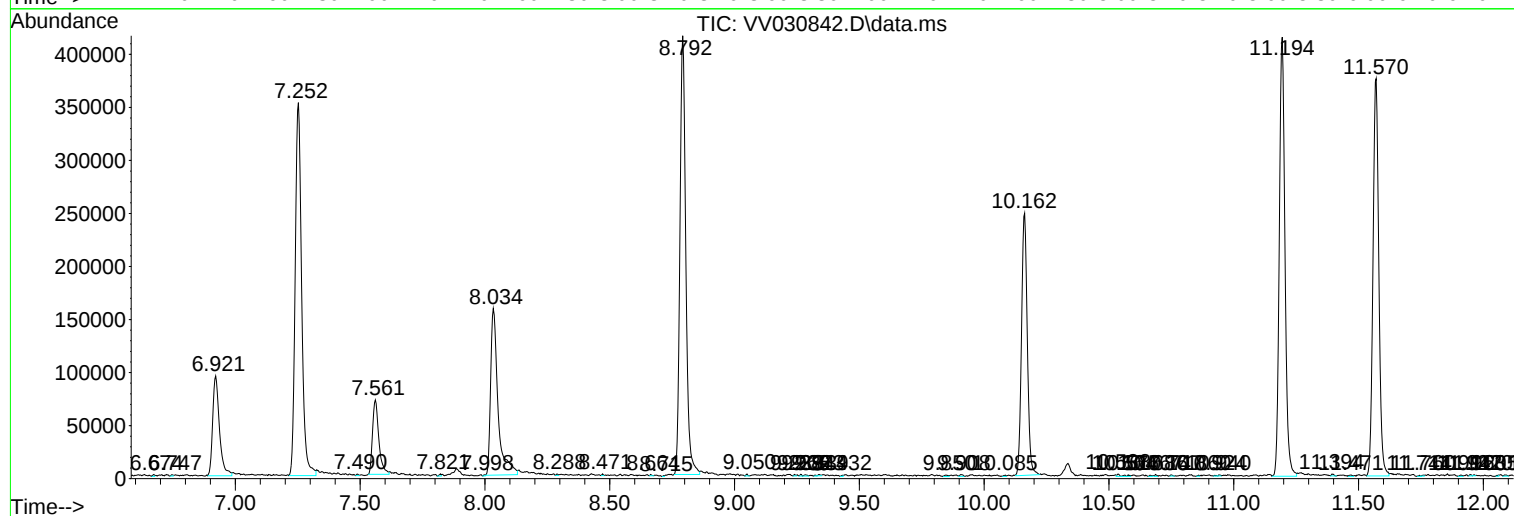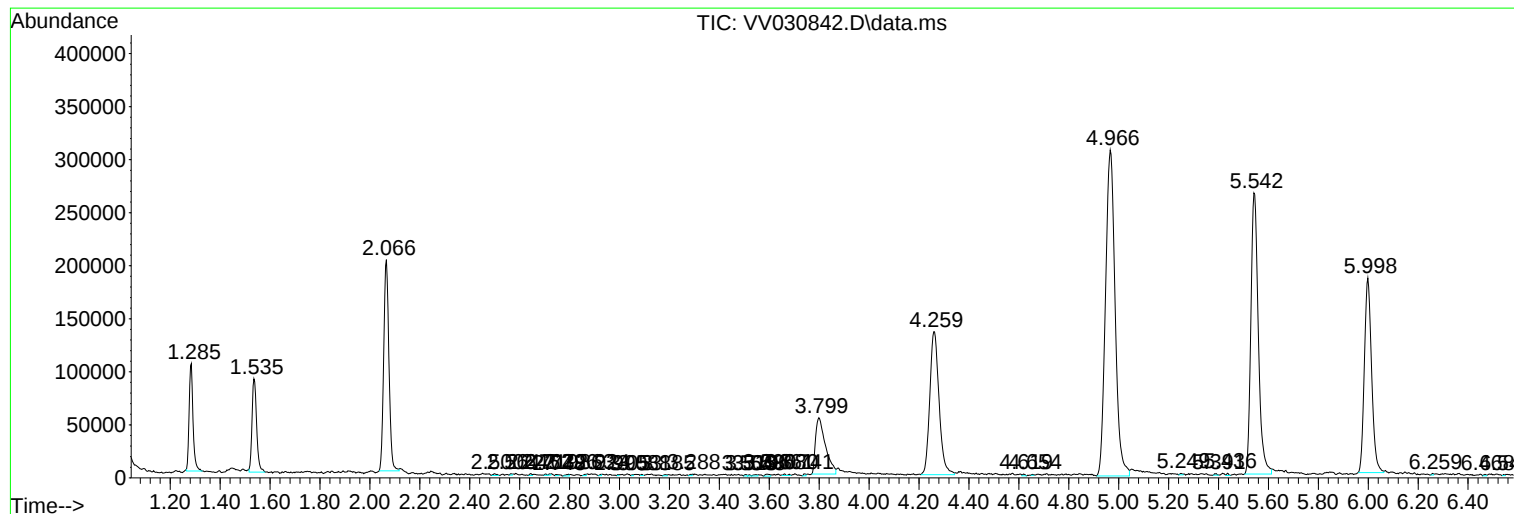

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
Data File : VV030842.D
Acq On : 25 Apr 2023 17:16
Operator : SY/MD
Sample : 02475-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AW9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
Data File : VV030842.D
Acq On : 25 Apr 2023 17:16
Operator : SY/MD
Sample : 02475-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AW9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------