

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
 Data File : VV030843.D
 Acq On : 25 Apr 2023 17:40
 Operator : SY/MD
 Sample : 02475-01 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AW3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030843.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.285	69	76	92	rVB	84849	95179	14.42%	1.800%
2	1.536	148	154	164	rVB	80076	92866	14.07%	1.756%
3	2.066	310	319	334	rBV	162634	236573	35.84%	4.475%
4	2.294	388	390	394	rVB3	1689	971	0.15%	0.018%
5	2.320	394	398	400	rBV5	1706	1408	0.21%	0.027%
6	2.352	406	408	411	rBV3	1149	668	0.10%	0.013%
7	2.429	428	432	433	rBV2	2154	1479	0.22%	0.028%
8	2.548	467	469	472	rBV4	1114	673	0.10%	0.013%
9	2.744	528	530	533	rVB3	1441	781	0.12%	0.015%
10	2.870	566	569	574	rBV7	1097	884	0.13%	0.017%
11	2.957	593	596	598	rBV4	1214	532	0.08%	0.010%
12	3.018	611	615	617	rBV5	1358	1152	0.17%	0.022%
13	3.044	622	623	625	rVV2	1462	699	0.11%	0.013%
14	3.072	629	632	635	rVV3	934	621	0.09%	0.012%
15	3.130	647	650	652	rBV4	1111	596	0.09%	0.011%
16	3.188	665	668	670	rBV4	1200	725	0.11%	0.014%
17	3.236	680	683	687	rVB5	1417	923	0.14%	0.017%
18	3.259	687	690	691	rBV3	982	656	0.10%	0.012%
19	3.317	705	708	709	rBV3	1395	597	0.09%	0.011%
20	3.359	719	721	723	rVB2	1038	461	0.07%	0.009%
21	3.433	742	744	747	rBV3	1719	905	0.14%	0.017%
22	3.458	751	752	757	rBV5	777	690	0.10%	0.013%
23	3.526	771	773	779	rVB6	1166	960	0.15%	0.018%
24	3.600	792	796	799	rBV5	860	574	0.09%	0.011%
25	3.806	848	860	880	rBV	40945	115276	17.46%	2.180%
26	4.063	938	940	945	rBV5	1365	821	0.12%	0.016%
27	4.259	988	1001	1020	rBV2	106495	268516	40.68%	5.079%
28	4.609	1108	1110	1112	rBV3	1861	1039	0.16%	0.020%
29	4.622	1112	1114	1117	rVV5	1179	740	0.11%	0.014%
30	4.905	1201	1202	1205	rBV3	797	485	0.07%	0.009%
31	4.966	1205	1221	1242	rBV2	247155	660143	100.00%	12.486%
32	5.307	1325	1327	1329	rBV2	1017	614	0.09%	0.012%
33	5.407	1353	1358	1360	rBV5	2334	1981	0.30%	0.037%
34	5.542	1389	1400	1423	rBV	229185	478361	72.46%	9.048%
35	5.944	1522	1525	1527	rBV4	1967	1435	0.22%	0.027%
36	5.998	1532	1542	1564	rVB2	146304	303079	45.91%	5.732%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042523\
 Data File : VW030843.D
 Acq On : 25 Apr 2023 17:40
 Operator : SY/MD
 Sample : 02475-01 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AW3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	6.124	1579	1581	1584	rBV4	1330	779	0.12%	0.015%
38	6.400	1665	1667	1670	rBV4	1275	782	0.12%	0.015%
39	6.445	1680	1681	1684	rVB3	1144	512	0.08%	0.010%
40	6.535	1707	1709	1713	rBV5	1171	732	0.11%	0.014%
41	6.731	1768	1770	1772	rBV3	1305	645	0.10%	0.012%
42	6.786	1785	1787	1790	rBV4	875	479	0.07%	0.009%
43	6.921	1815	1829	1842	rBV	76905	143965	21.81%	2.723%
44	7.056	1869	1871	1874	rVB3	1445	544	0.08%	0.010%
45	7.252	1920	1932	1948	rBV	276088	495723	75.09%	9.376%
46	7.561	2018	2028	2041	rBV	54478	100462	15.22%	1.900%
47	7.735	2079	2082	2084	rBV4	1876	1407	0.21%	0.027%
48	7.841	2111	2115	2117	rBV5	1247	736	0.11%	0.014%
49	8.034	2164	2175	2208	rBV	119305	260608	39.48%	4.929%
50	8.500	2317	2320	2322	rBV3	1058	684	0.10%	0.013%
51	8.793	2400	2411	2432	rBV	363756	604209	91.53%	11.428%
52	9.088	2499	2503	2505	rBV4	1623	1340	0.20%	0.025%
53	9.175	2528	2530	2533	rBV3	1458	723	0.11%	0.014%
54	9.210	2539	2541	2546	rVB4	1384	1025	0.16%	0.019%
55	9.490	2625	2628	2630	rBV3	1203	833	0.13%	0.016%
56	9.706	2692	2695	2698	rVB4	937	594	0.09%	0.011%
57	9.735	2702	2704	2705	rBV2	1108	508	0.08%	0.010%
58	9.828	2730	2733	2734	rBV3	1057	488	0.07%	0.009%
59	9.985	2780	2782	2785	rBV3	889	486	0.07%	0.009%
60	10.059	2802	2805	2808	rVB5	951	542	0.08%	0.010%
61	10.075	2808	2810	2812	rBV2	851	477	0.07%	0.009%
62	10.159	2825	2836	2851	rBV2	198458	317865	48.15%	6.012%
63	10.317	2883	2885	2889	rVB3	1112	566	0.09%	0.011%
64	10.477	2931	2935	2937	rBV4	1624	1138	0.17%	0.022%
65	10.522	2945	2949	2952	rBV6	921	645	0.10%	0.012%
66	10.735	3012	3015	3018	rVB5	1496	1077	0.16%	0.020%
67	10.754	3018	3021	3022	rBV3	1302	681	0.10%	0.013%
68	10.763	3022	3024	3028	rVV5	1056	833	0.13%	0.016%
69	10.812	3036	3039	3040	rBV3	665	479	0.07%	0.009%
70	10.834	3044	3046	3048	rBV2	925	520	0.08%	0.010%
71	10.876	3056	3059	3060	rBV3	1239	561	0.08%	0.011%
72	10.982	3086	3092	3093	rBV4	1800	1396	0.21%	0.026%
73	11.088	3123	3125	3128	rBV4	916	719	0.11%	0.014%
74	11.104	3128	3130	3132	rBV	930	472	0.07%	0.009%
75	11.194	3147	3158	3174	rBV	366327	565298	85.63%	10.692%
76	11.297	3187	3190	3194	rBV5	1862	1744	0.26%	0.033%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042523\
 Data File : VW030843.D
 Acq On : 25 Apr 2023 17:40
 Operator : SY/MD
 Sample : 02475-01 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AW3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M

Title : VOC Analysis

77	11.567	3264	3274	3290	rBV	298925	478027	72.41%	9.041%
78	11.699	3313	3315	3318	rBV4	1356	903	0.14%	0.017%
79	12.114	3441	3444	3446	rBV4	1363	891	0.13%	0.017%
80	12.181	3463	3465	3469	rVB4	1527	782	0.12%	0.015%
81	12.259	3486	3489	3492	rBV3	1439	1381	0.21%	0.026%
82	12.320	3503	3508	3510	rBV7	1674	1273	0.19%	0.024%
83	12.513	3565	3568	3571	rBV5	1546	1348	0.20%	0.025%
84	12.638	3604	3607	3610	rBV5	1325	915	0.14%	0.017%
85	12.728	3631	3635	3637	rVV5	894	682	0.10%	0.013%
86	12.940	3699	3701	3703	rBV3	1138	550	0.08%	0.010%
87	12.988	3714	3716	3718	rBV2	1349	775	0.12%	0.015%
88	13.075	3742	3743	3744	rBV2	1221	463	0.07%	0.009%
89	13.278	3803	3806	3809	rBV4	1702	1214	0.18%	0.023%
90	13.413	3846	3848	3851	rBV3	950	531	0.08%	0.010%
91	13.657	3922	3924	3927	rBV4	967	683	0.10%	0.013%
92	13.715	3939	3942	3944	rBV4	1254	904	0.14%	0.017%
93	13.815	3967	3973	3975	rBV7	1545	1860	0.28%	0.035%
94	13.828	3975	3977	3979	rVB2	1214	598	0.09%	0.011%
95	13.873	3986	3991	3993	rVB4	1308	903	0.14%	0.017%
96	13.886	3993	3995	3997	rBV2	1114	608	0.09%	0.011%
97	13.918	4002	4005	4008	rBV5	1892	1190	0.18%	0.023%
98	13.988	4023	4027	4029	rBV4	1575	1228	0.19%	0.023%
99	14.548	4198	4201	4204	rBV5	1660	1361	0.21%	0.026%
100	15.053	4356	4358	4360	rBV2	1160	634	0.10%	0.012%




Sum of corrected areas: 5287044

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
Data File : VV030843.D
Acq On : 25 Apr 2023 17:40
Operator : SY/MD
Sample : 02475-01 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AW3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

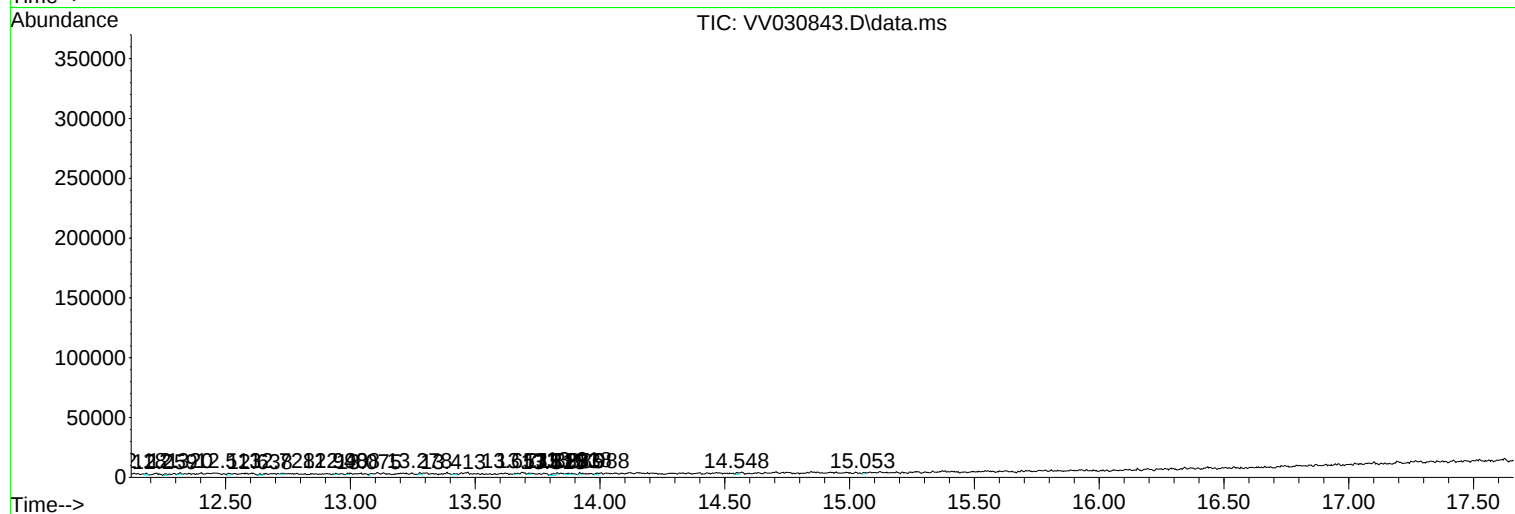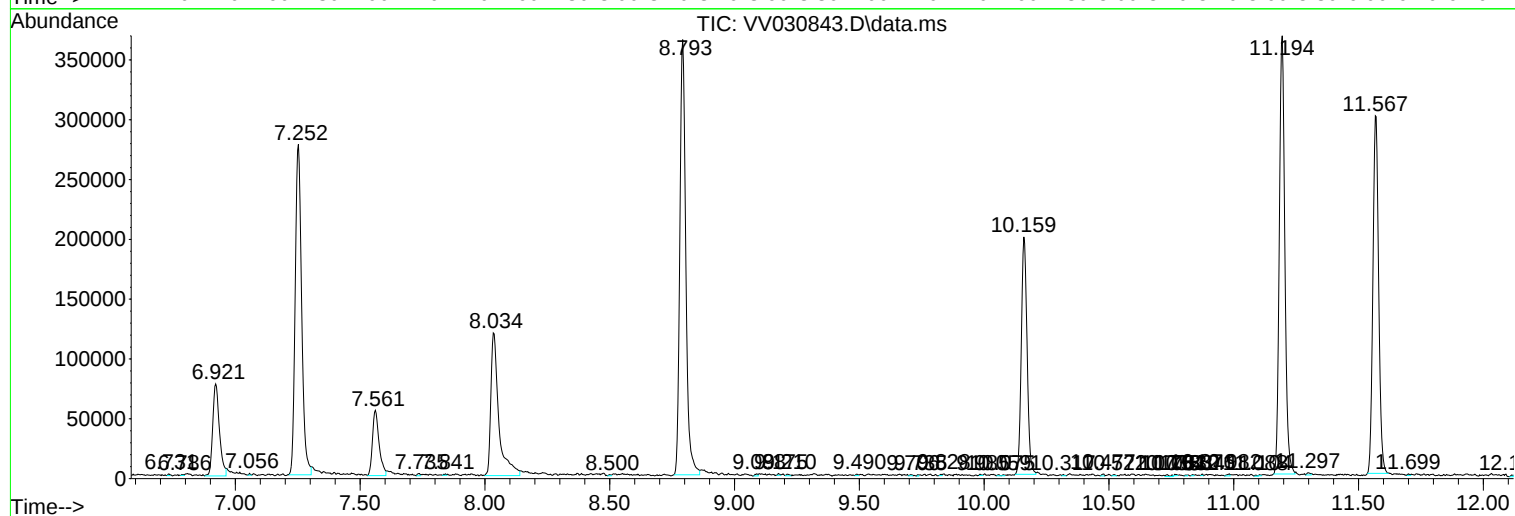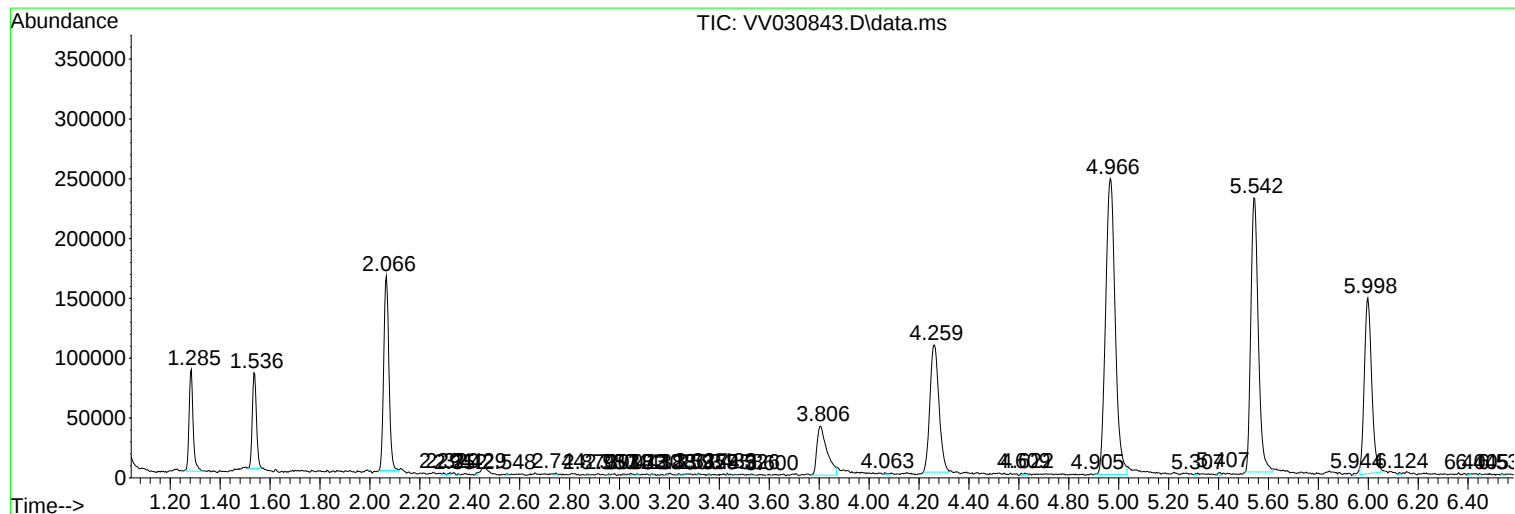

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
Data File : VV030843.D
Acq On : 25 Apr 2023 17:40
Operator : SY/MD
Sample : 02475-01 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AW3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
Data File : VV030843.D
Acq On : 25 Apr 2023 17:40
Operator : SY/MD
Sample : 02475-01 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AW3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------