

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
 Data File : VV030844.D
 Acq On : 25 Apr 2023 18:04
 Operator : SY/MD
 Sample : 02475-02 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AW4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M

Title : VOC Analysis

Signal : TIC: VV030844.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	69	75	90	rVB	102144	113440	13.47%	1.702%
2	1.536	148	154	173	rVB	94865	119119	14.15%	1.787%
3	2.066	310	319	333	rVB	204874	297668	35.36%	4.465%
4	2.404	421	424	428	rBV5	1940	1348	0.16%	0.020%
5	2.455	433	440	449	rVV5	6723	11697	1.39%	0.175%
6	2.626	489	493	498	rVB5	785	916	0.11%	0.014%
7	2.674	506	508	510	rBV3	1263	617	0.07%	0.009%
8	2.703	514	517	518	rBV3	1172	715	0.08%	0.011%
9	2.790	541	544	546	rBV3	1099	839	0.10%	0.013%
10	2.944	588	592	595	rBV6	1245	927	0.11%	0.014%
11	3.056	623	627	629	rBV4	1219	1085	0.13%	0.016%
12	3.124	645	648	650	rBV3	1419	751	0.09%	0.011%
13	3.159	658	659	663	rBV5	1035	662	0.08%	0.010%
14	3.445	743	748	751	rVB6	1105	1013	0.12%	0.015%
15	3.481	755	759	761	rBV5	1254	957	0.11%	0.014%
16	3.510	766	768	772	rVB5	1510	748	0.09%	0.011%
17	3.699	823	827	829	rBV5	1400	1191	0.14%	0.018%
18	3.799	847	858	892	rBV	53690	161770	19.22%	2.427%
19	4.143	963	965	969	rVB4	1387	731	0.09%	0.011%
20	4.259	985	1001	1023	rBV	135723	352664	41.89%	5.290%
21	4.844	1178	1183	1188	rVB8	1365	1600	0.19%	0.024%
22	4.873	1188	1192	1195	rBV6	1523	1516	0.18%	0.023%
23	4.966	1204	1221	1248	rBV3	312905	841858	100.00%	12.628%
24	5.442	1366	1369	1374	rBV7	1396	1024	0.12%	0.015%
25	5.542	1388	1400	1421	rBV	277649	570859	67.81%	8.563%
26	5.847	1484	1495	1510	rBV7	19523	44004	5.23%	0.660%
27	5.998	1529	1542	1561	rBV	186286	387916	46.08%	5.819%
28	6.198	1602	1604	1607	rBV3	1169	754	0.09%	0.011%
29	6.246	1616	1619	1621	rBV3	1093	641	0.08%	0.010%
30	6.362	1652	1655	1657	rBV3	1338	737	0.09%	0.011%
31	6.445	1676	1681	1686	rBV8	1550	1713	0.20%	0.026%
32	6.703	1756	1761	1767	rBV8	1960	2261	0.27%	0.034%
33	6.757	1776	1778	1786	rVB8	1297	929	0.11%	0.014%
34	6.844	1801	1805	1808	rBV6	1465	1002	0.12%	0.015%
35	6.921	1818	1829	1848	rBV	95712	180474	21.44%	2.707%
36	7.143	1896	1898	1902	rVB5	1235	696	0.08%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042523\
 Data File : VW030844.D
 Acq On : 25 Apr 2023 18:04
 Operator : SY/MD
 Sample : 02475-02 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AW4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	7.252	1920	1932	1948	rBV	362336	639332	75.94%	9.590%
38	7.561	2019	2028	2048	rVB	69047	122131	14.51%	1.832%
39	7.706	2071	2073	2075	rBV3	1399	706	0.08%	0.011%
40	7.735	2079	2082	2083	rBV3	1198	655	0.08%	0.010%
41	7.783	2095	2097	2100	rVB4	1964	1098	0.13%	0.016%
42	7.802	2100	2103	2106	rBV5	1781	1163	0.14%	0.017%
43	7.876	2124	2126	2133	rVB7	1694	1210	0.14%	0.018%
44	7.905	2133	2135	2137	rBV4	1182	780	0.09%	0.012%
45	7.957	2147	2151	2152	rBV4	818	643	0.08%	0.010%
46	7.985	2158	2160	2162	rVB3	1391	666	0.08%	0.010%
47	8.034	2165	2175	2206	rVV	165762	336910	40.02%	5.054%
48	8.265	2244	2247	2251	rVB6	1621	982	0.12%	0.015%
49	8.436	2295	2300	2301	rBV4	1331	1115	0.13%	0.017%
50	8.596	2346	2350	2351	rBV3	1567	1115	0.13%	0.017%
51	8.793	2400	2411	2434	rBV	418141	702202	83.41%	10.534%
52	9.124	2511	2514	2515	rBV3	1076	651	0.08%	0.010%
53	9.162	2523	2526	2527	rBV3	1327	831	0.10%	0.012%
54	9.220	2541	2544	2546	rVV4	1498	665	0.08%	0.010%
55	9.236	2546	2549	2551	rVB4	1465	756	0.09%	0.011%
56	9.439	2604	2612	2613	rBV5	1560	1600	0.19%	0.024%
57	9.465	2617	2620	2621	rBV3	1450	829	0.10%	0.012%
58	9.500	2628	2631	2634	rBV4	1934	1431	0.17%	0.021%
59	9.558	2646	2649	2651	rBV3	1393	858	0.10%	0.013%
60	9.696	2687	2692	2695	rBV7	1493	1582	0.19%	0.024%
61	9.915	2757	2760	2763	rBV5	1395	976	0.12%	0.015%
62	10.072	2805	2809	2813	rBV5	819	743	0.09%	0.011%
63	10.159	2823	2836	2856	rVV	256850	409127	48.60%	6.137%
64	10.362	2898	2899	2904	rVB3	1268	753	0.09%	0.011%
65	10.429	2917	2920	2923	rBV5	879	690	0.08%	0.010%
66	10.699	3001	3004	3009	rVB6	1485	1303	0.15%	0.020%
67	10.792	3029	3033	3035	rVV5	1423	1048	0.12%	0.016%
68	10.841	3045	3048	3053	rBV7	1010	734	0.09%	0.011%
69	11.127	3135	3137	3143	rVB5	1860	1299	0.15%	0.019%
70	11.194	3146	3158	3177	rVV	418625	674545	80.13%	10.119%
71	11.423	3226	3229	3231	rVB4	1151	617	0.07%	0.009%
72	11.442	3231	3235	3237	rBV4	1036	868	0.10%	0.013%
73	11.571	3261	3275	3293	rBV	375254	618793	73.50%	9.282%
74	11.844	3358	3360	3364	rBV5	1169	854	0.10%	0.013%
75	11.947	3389	3392	3395	rBV3	1224	1077	0.13%	0.016%
76	12.024	3410	3416	3418	rBV6	1212	1183	0.14%	0.018%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042523\
 Data File : VW030844.D
 Acq On : 25 Apr 2023 18:04
 Operator : SY/MD
 Sample : 02475-02 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AW4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	12.178	3459	3464	3465	rBV4	1103	930	0.11%	0.014%
78	12.252	3482	3487	3491	rVB5	1069	936	0.11%	0.014%
79	12.275	3491	3494	3500	rBV7	1653	1680	0.20%	0.025%
80	12.397	3530	3532	3538	rVB7	1581	1492	0.18%	0.022%
81	12.429	3538	3542	3544	rBV4	1336	916	0.11%	0.014%
82	12.648	3606	3610	3613	rBV5	1999	1600	0.19%	0.024%
83	12.725	3630	3634	3637	rVB6	1191	803	0.10%	0.012%
84	12.866	3675	3678	3680	rBV3	1360	874	0.10%	0.013%
85	12.902	3686	3689	3695	rBV6	930	1146	0.14%	0.017%
86	12.934	3696	3699	3704	rVB5	1348	1393	0.17%	0.021%
87	12.956	3704	3706	3710	rBV4	1235	705	0.08%	0.011%
88	13.069	3738	3741	3744	rBV5	1194	904	0.11%	0.014%
89	13.673	3925	3929	3932	rBV6	1239	892	0.11%	0.013%
90	13.754	3951	3954	3956	rBV4	1475	864	0.10%	0.013%
91	13.779	3959	3962	3964	rBV3	807	649	0.08%	0.010%
92	13.853	3982	3985	3988	rBV3	1067	702	0.08%	0.011%
93	13.934	4007	4010	4012	rBV4	967	705	0.08%	0.011%
94	14.017	4032	4036	4038	rBV4	873	642	0.08%	0.010%
95	14.165	4080	4082	4087	rVB5	1324	1013	0.12%	0.015%
96	14.214	4093	4097	4100	rBV4	1607	1262	0.15%	0.019%
97	14.435	4164	4166	4170	rBV4	1179	997	0.12%	0.015%
98	14.776	4270	4272	4275	rBV4	1131	912	0.11%	0.014%
99	15.114	4375	4377	4382	rVB6	1794	1575	0.19%	0.024%
100	15.143	4383	4386	4389	rBV4	1570	1387	0.16%	0.021%




Sum of corrected areas: 6666342

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
Data File : VV030844.D
Acq On : 25 Apr 2023 18:04
Operator : SY/MD
Sample : 02475-02 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AW4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

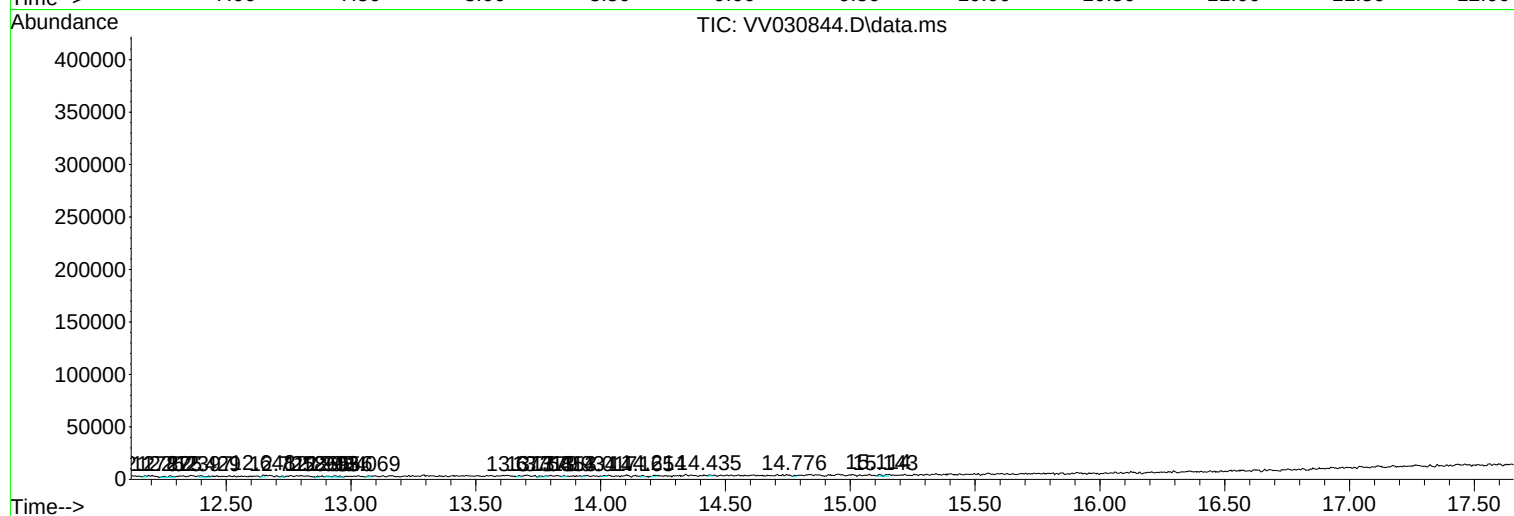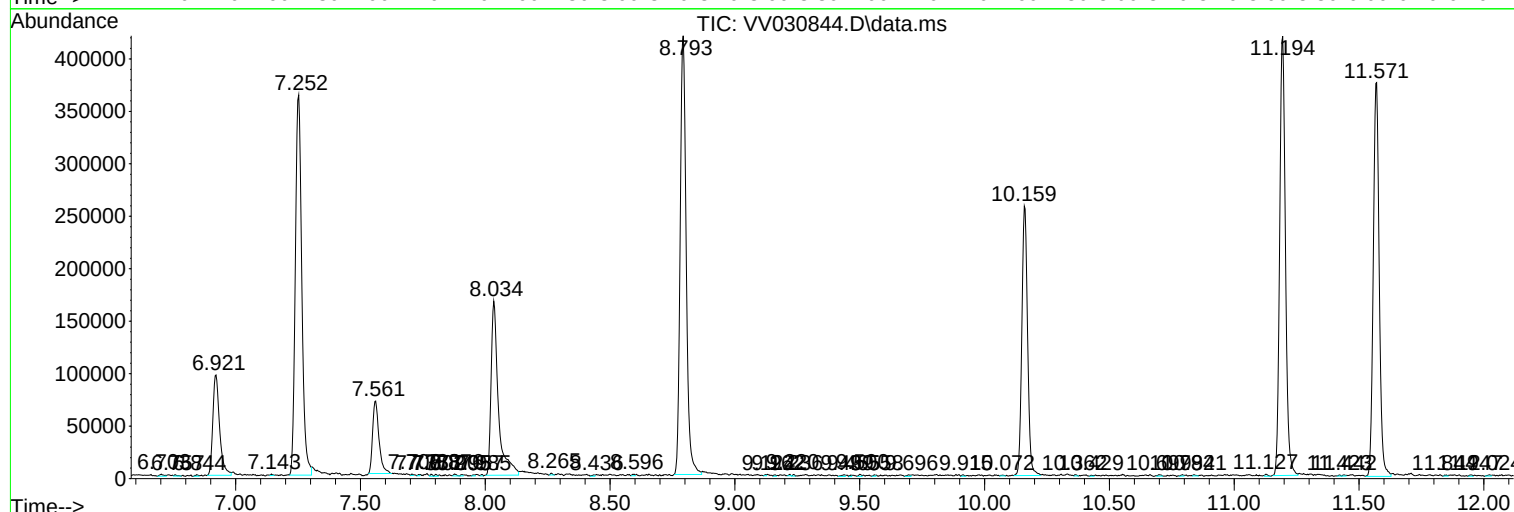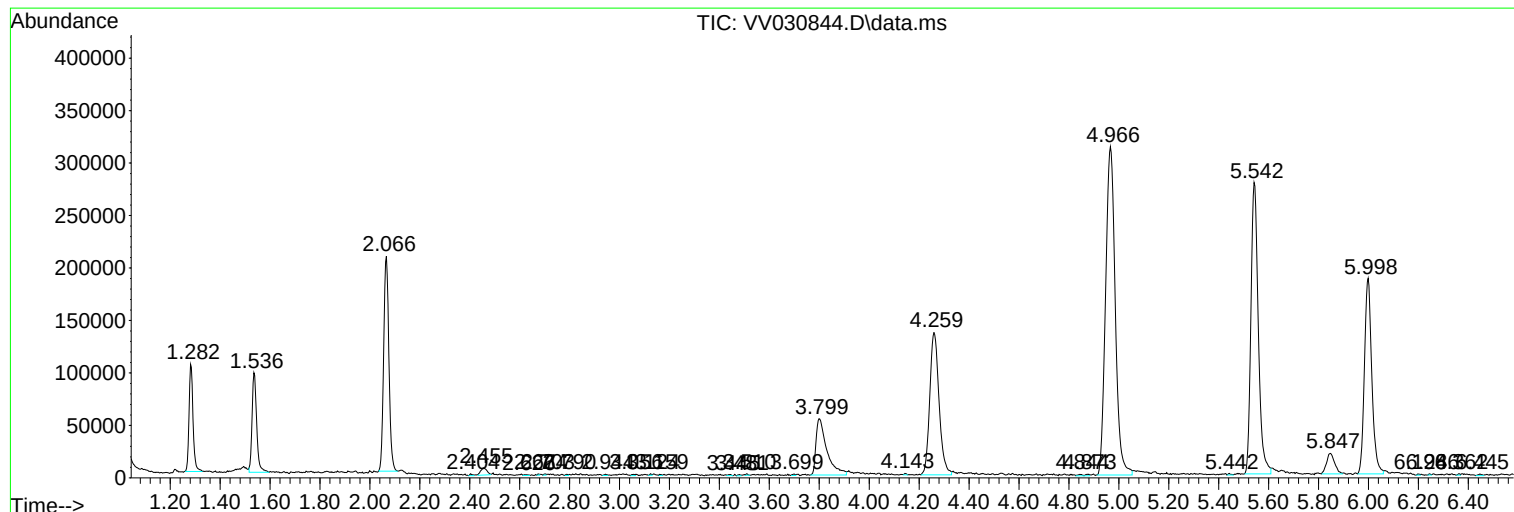

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
Data File : VV030844.D
Acq On : 25 Apr 2023 18:04
Operator : SY/MD
Sample : 02475-02 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AW4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
Data File : VV030844.D
Acq On : 25 Apr 2023 18:04
Operator : SY/MD
Sample : 02475-02 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AW4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------