

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042523\
 Data File : VW030845.D
 Acq On : 25 Apr 2023 18:28
 Operator : SY/MD
 Sample : 02475-03 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AW5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VW030845.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.285	70	76	91	rVB	98468	110782	13.29%	1.711%
2	1.535	148	154	165	rVB	92148	109961	13.19%	1.698%
3	2.066	310	319	332	rBV	201066	289566	34.73%	4.473%
4	2.156	345	347	349	rBV3	1300	551	0.07%	0.009%
5	2.227	365	369	372	rBV6	2101	1573	0.19%	0.024%
6	2.285	385	387	388	rBV	1346	710	0.09%	0.011%
7	2.323	397	399	403	rBV5	1723	902	0.11%	0.014%
8	2.400	420	423	425	rBV4	1294	766	0.09%	0.012%
9	2.674	506	508	511	rBV3	1022	569	0.07%	0.009%
10	2.783	539	542	544	rBV3	1093	812	0.10%	0.013%
11	2.799	546	547	551	rVB4	1323	701	0.08%	0.011%
12	2.863	565	567	569	rBV3	1105	622	0.07%	0.010%
13	3.053	623	626	629	rBV4	1214	1004	0.12%	0.016%
14	3.169	655	662	666	rBV7	1244	1495	0.18%	0.023%
15	3.230	675	681	683	rBV5	1834	1333	0.16%	0.021%
16	3.246	684	686	688	rBV3	1360	618	0.07%	0.010%
17	3.375	724	726	729	rVB4	1213	571	0.07%	0.009%
18	3.497	762	764	767	rVB2	1327	714	0.09%	0.011%
19	3.796	848	857	880	rBV	52334	145135	17.41%	2.242%
20	4.169	969	973	975	rBV4	1388	888	0.11%	0.014%
21	4.259	988	1001	1024	rVB	133871	330310	39.62%	5.102%
22	4.587	1100	1103	1106	rBV5	1440	1147	0.14%	0.018%
23	4.638	1115	1119	1122	rBV4	1415	976	0.12%	0.015%
24	4.828	1176	1178	1180	rBV3	956	518	0.06%	0.008%
25	4.966	1204	1221	1245	rBV3	309680	833721	100.00%	12.878%
26	5.403	1354	1357	1359	rBV4	1858	1040	0.12%	0.016%
27	5.490	1381	1384	1386	rBV4	1202	614	0.07%	0.009%
28	5.542	1388	1400	1428	rVV	271105	567309	68.05%	8.763%
29	5.998	1527	1542	1568	rBV2	184527	389056	46.67%	6.009%
30	6.420	1671	1673	1677	rVB5	1387	850	0.10%	0.013%
31	6.439	1677	1679	1680	rBV2	1202	664	0.08%	0.010%
32	6.484	1690	1693	1698	rBV7	1395	1243	0.15%	0.019%
33	6.555	1713	1715	1718	rVB4	2126	962	0.12%	0.015%
34	6.815	1794	1796	1798	rBV2	1061	560	0.07%	0.009%
35	6.873	1811	1814	1815	rBV3	1034	678	0.08%	0.010%
36	6.921	1817	1829	1847	rBV	93962	179048	21.48%	2.766%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042523\
 Data File : VW030845.D
 Acq On : 25 Apr 2023 18:28
 Operator : SY/MD
 Sample : 02475-03 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AW5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	7.252	1920	1932	1957	rBV	351947	638988	76.64%	9.870%
38	7.561	2019	2028	2044	rBV	69426	123528	14.82%	1.908%
39	7.696	2068	2070	2076	rBV6	1635	1411	0.17%	0.022%
40	7.812	2103	2106	2109	rVV5	1628	1027	0.12%	0.016%
41	7.886	2127	2129	2134	rVB5	1593	791	0.09%	0.012%
42	7.908	2134	2136	2144	rVB8	1790	1624	0.19%	0.025%
43	7.979	2154	2158	2161	rVV5	966	855	0.10%	0.013%
44	8.034	2166	2175	2205	rVV	162286	325991	39.10%	5.035%
45	8.474	2310	2312	2314	rBV3	1430	661	0.08%	0.010%
46	8.690	2375	2379	2382	rBV7	1389	1320	0.16%	0.020%
47	8.792	2400	2411	2431	rBV	414367	688107	82.53%	10.628%
48	9.117	2509	2512	2513	rBV3	1056	548	0.07%	0.008%
49	9.223	2543	2545	2547	rBV2	1486	673	0.08%	0.010%
50	9.461	2617	2619	2623	rVB3	1230	571	0.07%	0.009%
51	9.484	2623	2626	2628	rBV4	1618	971	0.12%	0.015%
52	9.532	2639	2641	2646	rVV5	1517	809	0.10%	0.012%
53	9.564	2649	2651	2654	rBV4	1294	660	0.08%	0.010%
54	9.654	2675	2679	2680	rBV4	947	611	0.07%	0.009%
55	9.786	2717	2720	2723	rBV5	1574	1065	0.13%	0.016%
56	9.879	2747	2749	2753	rBV5	1260	949	0.11%	0.015%
57	10.066	2804	2807	2809	rVB4	1382	857	0.10%	0.013%
58	10.082	2809	2812	2820	rVB7	2322	2789	0.33%	0.043%
59	10.120	2820	2824	2825	rBV4	1657	1170	0.14%	0.018%
60	10.159	2825	2836	2854	rBV	253175	407210	48.84%	6.290%
61	10.384	2904	2906	2912	rBV7	1001	820	0.10%	0.013%
62	10.452	2924	2927	2931	rVB5	1874	1232	0.15%	0.019%
63	10.509	2944	2945	2948	rVB2	1526	534	0.06%	0.008%
64	10.603	2971	2974	2975	rBV4	890	541	0.06%	0.008%
65	10.661	2987	2992	2996	rVB7	1559	1568	0.19%	0.024%
66	10.789	3028	3032	3034	rBV5	1873	1241	0.15%	0.019%
67	10.828	3042	3044	3047	rBV4	867	569	0.07%	0.009%
68	10.857	3050	3053	3054	rBV3	1307	828	0.10%	0.013%
69	10.950	3079	3082	3088	rBV6	2029	1574	0.19%	0.024%
70	10.982	3088	3092	3096	rBV5	1261	1107	0.13%	0.017%
71	11.194	3147	3158	3175	rBV	413464	656185	78.71%	10.135%
72	11.567	3263	3274	3292	rBV	378934	601826	72.19%	9.296%
73	11.773	3336	3338	3342	rBV5	1452	1119	0.13%	0.017%
74	11.937	3387	3389	3391	rBV3	1179	575	0.07%	0.009%
75	12.085	3431	3435	3439	rVB6	1049	884	0.11%	0.014%
76	12.220	3473	3477	3480	rBV4	1081	950	0.11%	0.015%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042523\
 Data File : VW030845.D
 Acq On : 25 Apr 2023 18:28
 Operator : SY/MD
 Sample : 02475-03 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AW5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	12.390	3528	3530	3532	rVB3	1638	636	0.08%	0.010%
78	12.406	3532	3535	3536	rBV3	1070	668	0.08%	0.010%
79	12.496	3561	3563	3565	rBV4	1252	592	0.07%	0.009%
80	12.580	3583	3589	3591	rBV7	1172	1003	0.12%	0.015%
81	13.024	3724	3727	3728	rBV2	1520	717	0.09%	0.011%
82	13.143	3762	3764	3766	rBV4	1275	785	0.09%	0.012%
83	13.175	3770	3774	3775	rBV4	1173	743	0.09%	0.011%
84	13.252	3796	3798	3803	rVB5	1589	1021	0.12%	0.016%
85	13.304	3810	3814	3816	rVB5	1448	1050	0.13%	0.016%
86	13.329	3816	3822	3824	rBV7	882	656	0.08%	0.010%
87	13.448	3857	3859	3861	rBV3	1286	688	0.08%	0.011%
88	13.509	3874	3878	3880	rBV4	1086	918	0.11%	0.014%
89	13.731	3944	3947	3948	rBV2	1494	566	0.07%	0.009%
90	13.770	3955	3959	3963	rBV6	1602	1899	0.23%	0.029%
91	13.844	3980	3982	3986	rVB4	1479	820	0.10%	0.013%
92	13.930	4006	4009	4012	rVB5	1259	830	0.10%	0.013%
93	13.947	4012	4014	4015	rBV2	1130	537	0.06%	0.008%
94	14.156	4074	4079	4081	rBV4	1273	1409	0.17%	0.022%
95	14.355	4139	4141	4145	rBV4	1557	1303	0.16%	0.020%
96	14.525	4190	4194	4197	rBV5	1377	1268	0.15%	0.020%
97	14.641	4228	4230	4232	rBV3	1099	529	0.06%	0.008%
98	14.744	4260	4262	4265	rBV4	1389	1015	0.12%	0.016%
99	15.033	4350	4352	4354	rBV3	1993	905	0.11%	0.014%
100	15.165	4391	4393	4396	rBV4	1631	953	0.11%	0.015%




Sum of corrected areas: 6474219

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
Data File : VV030845.D
Acq On : 25 Apr 2023 18:28
Operator : SY/MD
Sample : 02475-03 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AW5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

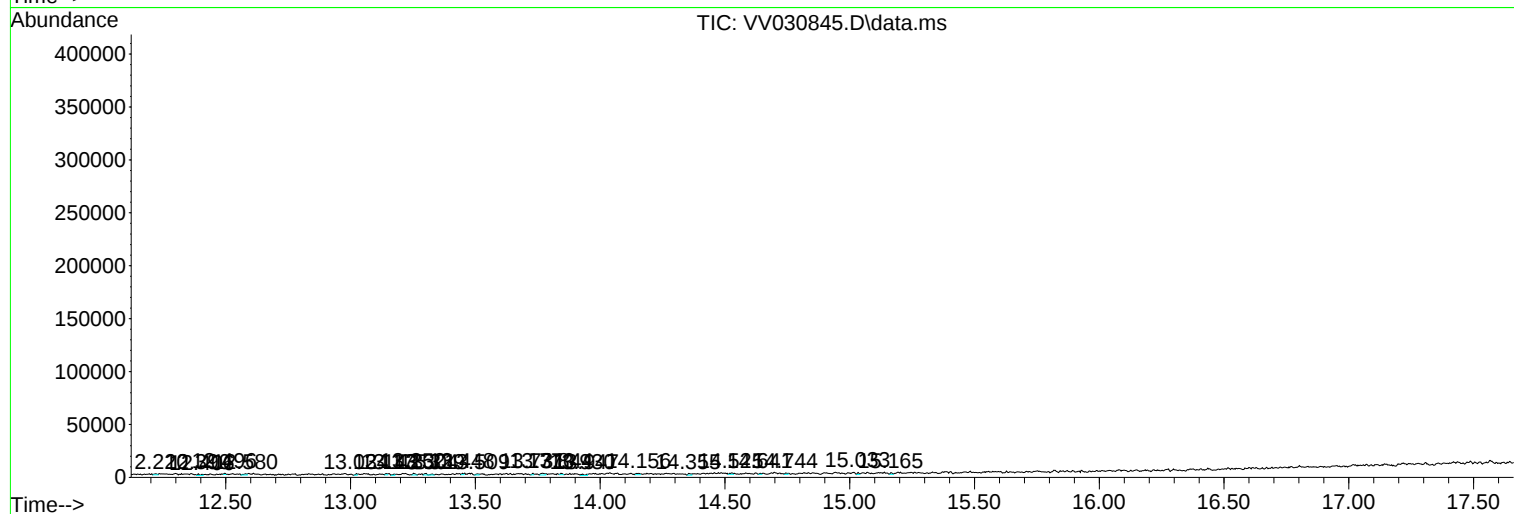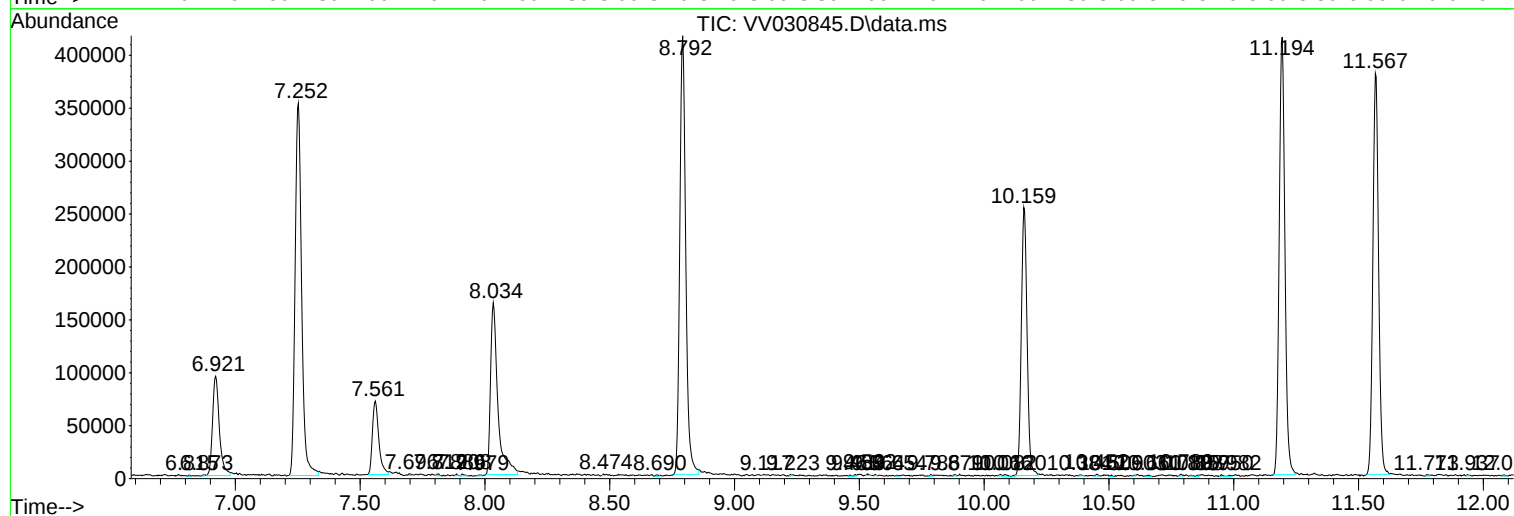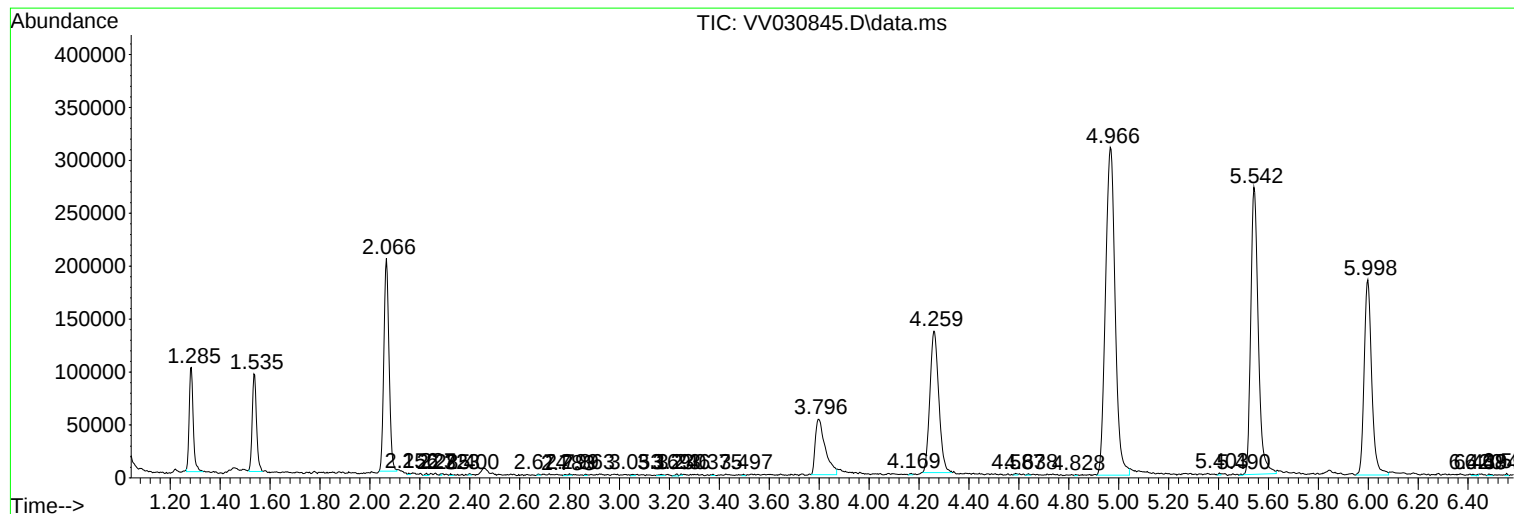

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
Data File : VV030845.D
Acq On : 25 Apr 2023 18:28
Operator : SY/MD
Sample : 02475-03 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AW5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
Data File : VV030845.D
Acq On : 25 Apr 2023 18:28
Operator : SY/MD
Sample : 02475-03 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AW5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc