

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
 Data File : VV030847.D
 Acq On : 25 Apr 2023 19:16
 Operator : SY/MD
 Sample : 02475-05 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AW7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030847.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.285	70	76	88	rVB	95687	103220	12.82%	1.614%
2	1.539	148	155	167	rVB	93636	110732	13.76%	1.732%
3	2.066	309	319	335	rBV	198823	295040	36.65%	4.614%
4	2.211	362	364	367	rBV4	2130	1284	0.16%	0.020%
5	2.249	370	376	378	rBV6	1801	1636	0.20%	0.026%
6	2.323	395	399	401	rBV3	1295	936	0.12%	0.015%
7	2.365	410	412	415	rVB4	1171	547	0.07%	0.009%
8	2.391	418	420	425	rVB6	1767	974	0.12%	0.015%
9	2.420	425	429	431	rBV4	1516	1156	0.14%	0.018%
10	2.603	484	486	490	rVB4	1049	568	0.07%	0.009%
11	2.661	502	504	505	rBV2	1051	474	0.06%	0.007%
12	2.957	594	596	598	rBV2	784	471	0.06%	0.007%
13	2.992	603	607	609	rBV4	1596	1254	0.16%	0.020%
14	3.066	627	630	631	rBV3	974	525	0.07%	0.008%
15	3.249	685	687	692	rVB5	629	470	0.06%	0.007%
16	3.288	696	699	700	rBV3	1429	739	0.09%	0.012%
17	3.365	720	723	726	rBV4	1182	675	0.08%	0.011%
18	3.535	773	776	779	rVB4	1256	744	0.09%	0.012%
19	3.648	809	811	816	rVB5	1294	1053	0.13%	0.016%
20	3.674	816	819	821	rBV4	1194	895	0.11%	0.014%
21	3.799	849	858	882	rBV2	52104	148047	18.39%	2.315%
22	4.162	969	971	973	rBV3	1041	546	0.07%	0.009%
23	4.259	988	1001	1023	rBV	128887	327316	40.66%	5.118%
24	4.584	1099	1102	1106	rBV6	1103	933	0.12%	0.015%
25	4.735	1146	1149	1153	rBV5	978	738	0.09%	0.012%
26	4.889	1194	1197	1198	rBV3	943	601	0.07%	0.009%
27	4.966	1205	1221	1246	rBV2	301399	804929	100.00%	12.587%
28	5.542	1388	1400	1428	rBV	270979	568554	70.63%	8.891%
29	5.998	1529	1542	1559	rBV	179864	374498	46.53%	5.856%
30	6.249	1618	1620	1624	rVB5	1537	785	0.10%	0.012%
31	6.333	1642	1646	1648	rBV3	1518	1269	0.16%	0.020%
32	6.381	1658	1661	1663	rBV3	1419	899	0.11%	0.014%
33	6.609	1726	1732	1736	rBV	4002	3747	0.47%	0.059%
34	6.731	1768	1770	1774	rVB5	1579	797	0.10%	0.012%
35	6.921	1815	1829	1846	rBV	91943	177102	22.00%	2.769%
36	7.252	1921	1932	1951	rBV	348364	610466	75.84%	9.546%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042523\
 Data File : VW030847.D
 Acq On : 25 Apr 2023 19:16
 Operator : SY/MD
 Sample : 02475-05 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AW7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	7.561	2019	2028	2043	rBV	68024	117137	14.55%	1.832%
38	7.863	2118	2122	2124	rBV5	935	662	0.08%	0.010%
39	8.034	2166	2175	2215	rBV	159207	332001	41.25%	5.192%
40	8.342	2268	2271	2273	rBV3	1412	926	0.12%	0.014%
41	8.403	2287	2290	2293	rBV6	1107	868	0.11%	0.014%
42	8.667	2368	2372	2375	rVB6	1610	1039	0.13%	0.016%
43	8.725	2386	2390	2391	rBV3	1062	640	0.08%	0.010%
44	8.792	2399	2411	2430	rBV	418285	696381	86.51%	10.890%
45	9.323	2572	2576	2578	rBV5	1279	1013	0.13%	0.016%
46	9.339	2578	2581	2584	rVV4	1445	1012	0.13%	0.016%
47	9.432	2608	2610	2614	rVV4	959	508	0.06%	0.008%
48	9.452	2614	2616	2620	rVB4	1035	582	0.07%	0.009%
49	9.519	2633	2637	2638	rBV4	1042	777	0.10%	0.012%
50	9.542	2643	2644	2648	rVV4	1142	629	0.08%	0.010%
51	9.567	2650	2652	2657	rVB5	1320	758	0.09%	0.012%
52	9.609	2661	2665	2667	rBV5	996	803	0.10%	0.013%
53	9.638	2672	2674	2677	rBV3	1490	848	0.11%	0.013%
54	9.850	2737	2740	2743	rBV4	1238	775	0.10%	0.012%
55	9.979	2776	2780	2782	rBV4	864	550	0.07%	0.009%
56	10.075	2807	2810	2811	rBV3	1310	686	0.09%	0.011%
57	10.159	2826	2836	2853	rBV	252598	400196	49.72%	6.258%
58	10.297	2877	2879	2882	rVB4	1387	622	0.08%	0.010%
59	10.416	2911	2916	2918	rBV4	1361	1186	0.15%	0.019%
60	10.461	2928	2930	2934	rBV5	707	556	0.07%	0.009%
61	10.480	2934	2936	2939	rVV4	895	557	0.07%	0.009%
62	10.577	2962	2966	2969	rBV3	1332	981	0.12%	0.015%
63	10.593	2969	2971	2973	rBV3	901	498	0.06%	0.008%
64	10.651	2985	2989	2991	rBV6	940	587	0.07%	0.009%
65	10.718	3003	3010	3012	rBV6	2286	2543	0.32%	0.040%
66	10.934	3075	3077	3081	rVB5	1456	1081	0.13%	0.017%
67	10.998	3094	3097	3098	rBV2	1160	512	0.06%	0.008%
68	11.053	3112	3114	3117	rVB3	1336	827	0.10%	0.013%
69	11.091	3122	3126	3128	rBV5	1064	930	0.12%	0.015%
70	11.194	3146	3158	3175	rBV	415059	655547	81.44%	10.251%
71	11.567	3257	3274	3291	rVV	374398	598812	74.39%	9.364%
72	11.808	3347	3349	3352	rBV4	1114	659	0.08%	0.010%
73	11.950	3389	3393	3397	rBV5	1294	1424	0.18%	0.022%
74	12.062	3424	3428	3432	rBV4	849	941	0.12%	0.015%
75	12.082	3432	3434	3436	rBV2	905	496	0.06%	0.008%
76	12.111	3441	3443	3446	rBV3	1117	741	0.09%	0.012%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
 Data File : VV030847.D
 Acq On : 25 Apr 2023 19:16
 Operator : SY/MD
 Sample : 02475-05 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AW7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	12.197	3466	3470	3472	rBV4	1534	985	0.12%	0.015%
78	12.313	3500	3506	3508	rBV6	1587	1738	0.22%	0.027%
79	12.442	3543	3546	3549	rBV5	1332	1015	0.13%	0.016%
80	12.557	3578	3582	3584	rBV4	1454	962	0.12%	0.015%
81	12.676	3614	3619	3621	rVB6	1520	1348	0.17%	0.021%
82	12.689	3621	3623	3626	rBV4	1185	804	0.10%	0.013%
83	12.795	3653	3656	3660	rBV6	1038	778	0.10%	0.012%
84	12.821	3660	3664	3667	rVB6	970	746	0.09%	0.012%
85	13.027	3722	3728	3731	rBV6	1518	1480	0.18%	0.023%
86	13.046	3731	3734	3736	rBV4	1202	647	0.08%	0.010%
87	13.271	3802	3804	3805	rBV	1254	537	0.07%	0.008%
88	13.320	3815	3819	3822	rVB5	1194	860	0.11%	0.013%
89	13.339	3822	3825	3826	rBV3	1362	866	0.11%	0.014%
90	13.393	3841	3842	3847	rBV4	756	567	0.07%	0.009%
91	13.448	3851	3859	3860	rBV8	1554	1562	0.19%	0.024%
92	13.522	3880	3882	3887	rVB4	1039	659	0.08%	0.010%
93	13.828	3973	3977	3983	rBV8	1145	1003	0.12%	0.016%
94	13.892	3995	3997	4000	rBV4	976	659	0.08%	0.010%
95	13.972	4019	4022	4023	rBV2	1426	775	0.10%	0.012%
96	14.345	4136	4138	4140	rBV3	1049	483	0.06%	0.008%
97	14.390	4150	4152	4156	rVB5	1437	861	0.11%	0.013%
98	14.464	4172	4175	4179	rBV6	1186	926	0.12%	0.014%
99	14.927	4317	4319	4322	rBV4	1501	941	0.12%	0.015%
100	15.123	4378	4380	4383	rBV4	1371	713	0.09%	0.011%


Sum of corrected areas: 6394826

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
Data File : VV030847.D
Acq On : 25 Apr 2023 19:16
Operator : SY/MD
Sample : 02475-05 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AW7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

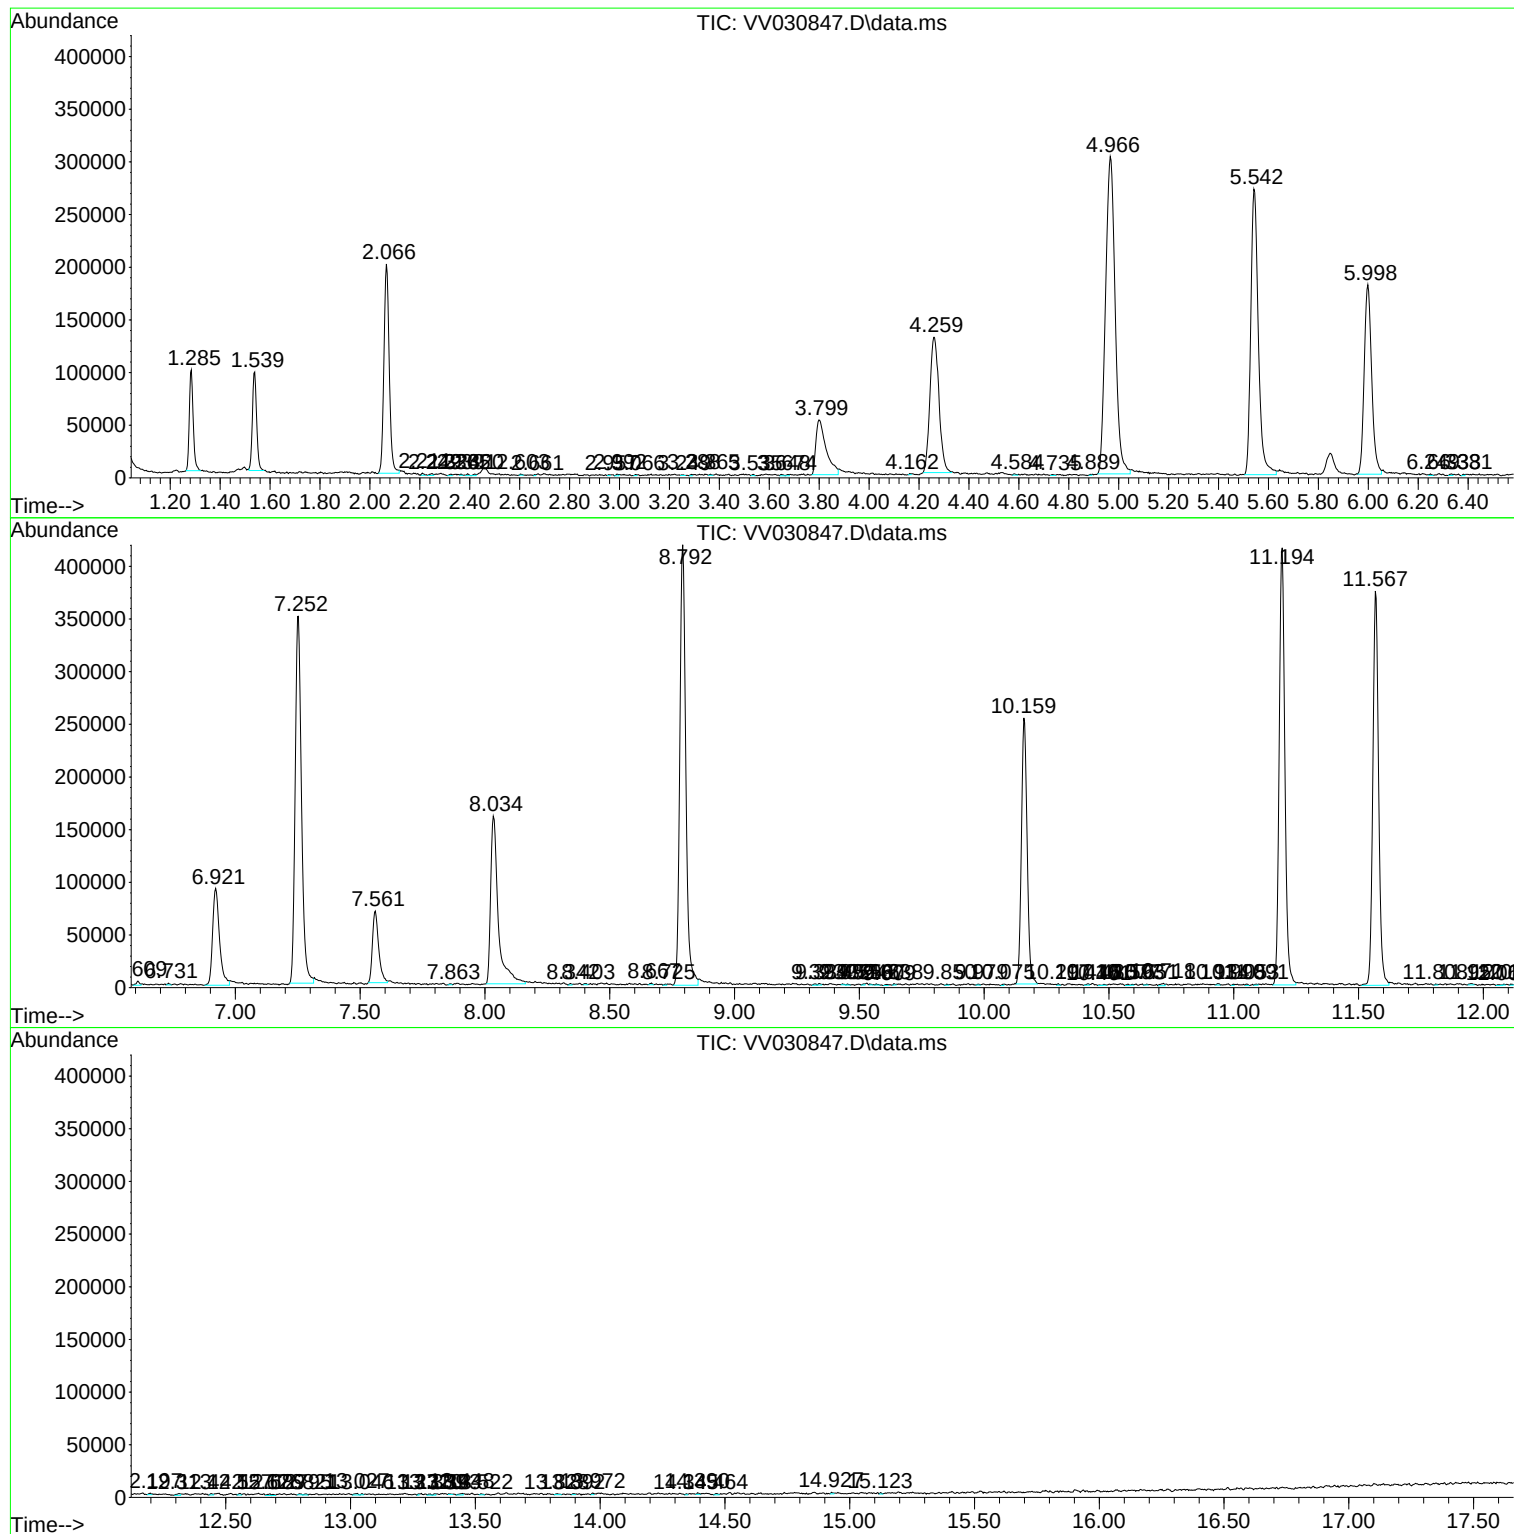

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
Data File : VV030847.D
Acq On : 25 Apr 2023 19:16
Operator : SY/MD
Sample : 02475-05 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AW7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
Data File : VV030847.D
Acq On : 25 Apr 2023 19:16
Operator : SY/MD
Sample : 02475-05 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AW7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc