

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
 Data File : VV030848.D
 Acq On : 25 Apr 2023 19:40
 Operator : SY/MD
 Sample : 02475-06 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AW8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030848.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.285	69	76	89	rVB	104935	113436	13.63%	1.715%
2	1.536	148	154	170	rVB	94427	115540	13.88%	1.747%
3	2.066	310	319	333	rVB	201986	293258	35.24%	4.435%
4	2.224	366	368	372	rBV5	1833	1715	0.21%	0.026%
5	2.458	431	441	449	rBV3	7392	11638	1.40%	0.176%
6	2.513	454	458	461	rVB6	1425	1207	0.15%	0.018%
7	2.536	461	465	468	rBV5	1046	877	0.11%	0.013%
8	2.610	483	488	489	rBV4	1216	1101	0.13%	0.017%
9	2.831	552	557	560	rBV7	1147	1048	0.13%	0.016%
10	2.921	581	585	588	rBV5	1139	857	0.10%	0.013%
11	3.044	621	623	628	rVB7	2190	1276	0.15%	0.019%
12	3.073	628	632	633	rBV4	1450	812	0.10%	0.012%
13	3.191	666	669	673	rVB5	1476	1141	0.14%	0.017%
14	3.426	739	742	745	rBV5	1117	998	0.12%	0.015%
15	3.481	758	759	765	rVB5	1488	879	0.11%	0.013%
16	3.536	772	776	780	rBV5	1000	982	0.12%	0.015%
17	3.609	797	799	802	rBV4	1470	1068	0.13%	0.016%
18	3.632	802	806	809	rBV5	1476	1351	0.16%	0.020%
19	3.677	815	820	821	rBV5	1033	886	0.11%	0.013%
20	3.754	842	844	849	rVB5	1031	833	0.10%	0.013%
21	3.799	849	858	878	rBV	53766	149818	18.00%	2.266%
22	4.079	943	945	947	rBV3	1555	640	0.08%	0.010%
23	4.262	988	1002	1028	rVB	137154	343828	41.32%	5.200%
24	4.564	1094	1096	1100	rBV6	1355	889	0.11%	0.013%
25	4.680	1126	1132	1138	rBV8	1198	1539	0.18%	0.023%
26	4.773	1158	1161	1162	rBV3	949	554	0.07%	0.008%
27	4.822	1172	1176	1177	rBV4	1253	864	0.10%	0.013%
28	4.876	1189	1193	1199	rBV5	1982	1830	0.22%	0.028%
29	4.905	1199	1202	1204	rBV4	1307	843	0.10%	0.013%
30	4.966	1204	1221	1244	rBV2	310770	832144	100.00%	12.584%
31	5.278	1316	1318	1321	rBV3	1346	762	0.09%	0.012%
32	5.349	1336	1340	1343	rBV6	1385	1037	0.12%	0.016%
33	5.400	1355	1356	1358	rBV2	1197	606	0.07%	0.009%
34	5.542	1388	1400	1425	rVV	269106	566835	68.12%	8.572%
35	5.847	1486	1495	1510	rVB6	19279	42487	5.11%	0.643%
36	5.998	1530	1542	1562	rBV	184360	377797	45.40%	5.713%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042523\
 Data File : VW030848.D
 Acq On : 25 Apr 2023 19:40
 Operator : SY/MD
 Sample : 02475-06 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AW8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	6.359	1650	1654	1657	rBV5	873	721	0.09%	0.011%
38	6.420	1671	1673	1675	rBV3	1337	787	0.09%	0.012%
39	6.699	1756	1760	1761	rBV4	1482	889	0.11%	0.013%
40	6.818	1793	1797	1798	rBV3	1048	758	0.09%	0.011%
41	6.857	1807	1809	1814	rVV5	1328	1000	0.12%	0.015%
42	6.921	1820	1829	1845	rBV	92306	170917	20.54%	2.585%
43	7.162	1901	1904	1905	rBV3	1224	655	0.08%	0.010%
44	7.198	1913	1915	1917	rBV2	876	556	0.07%	0.008%
45	7.252	1921	1932	1957	rVV	363445	647369	77.80%	9.790%
46	7.561	2015	2028	2041	rBV	72372	130301	15.66%	1.970%
47	7.912	2135	2137	2145	rBV7	1137	1271	0.15%	0.019%
48	8.034	2165	2175	2206	rBV	169106	345924	41.57%	5.231%
49	8.793	2400	2411	2431	rBV	419218	696698	83.72%	10.536%
50	9.075	2497	2499	2501	rVB3	1441	552	0.07%	0.008%
51	9.182	2529	2532	2536	rBV6	1305	1238	0.15%	0.019%
52	9.233	2545	2548	2552	rVB4	1076	695	0.08%	0.011%
53	9.259	2552	2556	2557	rBV4	878	745	0.09%	0.011%
54	9.320	2572	2575	2576	rBV3	1063	611	0.07%	0.009%
55	9.452	2613	2616	2618	rBV3	1032	650	0.08%	0.010%
56	9.580	2654	2656	2660	rBV3	1620	1339	0.16%	0.020%
57	9.770	2713	2715	2717	rVB3	1532	671	0.08%	0.010%
58	9.786	2717	2720	2727	rVB7	1139	1337	0.16%	0.020%
59	9.831	2727	2734	2735	rBV6	1089	1150	0.14%	0.017%
60	10.092	2811	2815	2816	rBV3	1025	679	0.08%	0.010%
61	10.159	2825	2836	2857	rVB	254402	407526	48.97%	6.163%
62	10.503	2941	2943	2946	rBV3	967	562	0.07%	0.008%
63	10.664	2991	2993	2997	rBV4	811	676	0.08%	0.010%
64	10.751	3014	3020	3023	rBV7	1612	1691	0.20%	0.026%
65	10.870	3054	3057	3063	rVB8	1880	1567	0.19%	0.024%
66	10.905	3063	3068	3071	rBV7	771	901	0.11%	0.014%
67	10.995	3095	3096	3099	rVB3	1191	593	0.07%	0.009%
68	11.104	3125	3130	3133	rBV7	2379	2585	0.31%	0.039%
69	11.191	3146	3157	3175	rBV	417197	663394	79.72%	10.032%
70	11.407	3222	3224	3227	rVB4	1319	794	0.10%	0.012%
71	11.490	3247	3250	3252	rBV4	1847	1105	0.13%	0.017%
72	11.567	3255	3274	3291	rBV	389884	623048	74.87%	9.422%
73	12.034	3417	3419	3422	rVV4	1080	597	0.07%	0.009%
74	12.098	3436	3439	3443	rBV6	1427	1230	0.15%	0.019%
75	12.175	3460	3463	3467	rVB6	1322	1012	0.12%	0.015%
76	12.358	3518	3520	3524	rBV5	1358	1022	0.12%	0.015%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042523\
 Data File : VW030848.D
 Acq On : 25 Apr 2023 19:40
 Operator : SY/MD
 Sample : 02475-06 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AW8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	12.419	3537	3539	3544	rVB5	1184	619	0.07%	0.009%
78	12.603	3591	3596	3599	rBV6	1179	992	0.12%	0.015%
79	12.641	3606	3608	3611	rBV5	978	690	0.08%	0.010%
80	12.718	3630	3632	3635	rVB3	1589	915	0.11%	0.014%
81	12.741	3635	3639	3640	rBV3	1160	579	0.07%	0.009%
82	12.757	3641	3644	3646	rBV3	1246	702	0.08%	0.011%
83	12.825	3661	3665	3669	rBV7	1412	1269	0.15%	0.019%
84	12.950	3701	3704	3706	rBV3	1371	879	0.11%	0.013%
85	13.027	3726	3728	3736	rVB9	1947	1567	0.19%	0.024%
86	13.066	3736	3740	3745	rBV8	1843	2096	0.25%	0.032%
87	13.152	3764	3767	3769	rBV4	1622	903	0.11%	0.014%
88	13.349	3825	3828	3834	rVB6	1515	1525	0.18%	0.023%
89	13.532	3883	3885	3888	rVB3	1780	815	0.10%	0.012%
90	13.632	3913	3916	3920	rBV6	836	758	0.09%	0.011%
91	13.661	3922	3925	3929	rVB4	1704	1173	0.14%	0.018%
92	13.693	3932	3935	3936	rBV3	1230	709	0.09%	0.011%
93	13.757	3952	3955	3958	rBV4	1468	1066	0.13%	0.016%
94	13.905	3998	4001	4004	rBV5	1946	1569	0.19%	0.024%
95	13.956	4013	4017	4019	rBV5	1211	950	0.11%	0.014%
96	14.307	4124	4126	4129	rBV4	1070	590	0.07%	0.009%
97	14.355	4137	4141	4143	rBV5	1379	1175	0.14%	0.018%
98	14.390	4150	4152	4153	rBV2	1359	555	0.07%	0.008%
99	14.889	4305	4307	4309	rBV3	1362	636	0.08%	0.010%
100	15.336	4444	4446	4447	rBV2	1499	667	0.08%	0.010%




Sum of corrected areas: 6612591

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
Data File : VV030848.D
Acq On : 25 Apr 2023 19:40
Operator : SY/MD
Sample : 02475-06 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AW8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

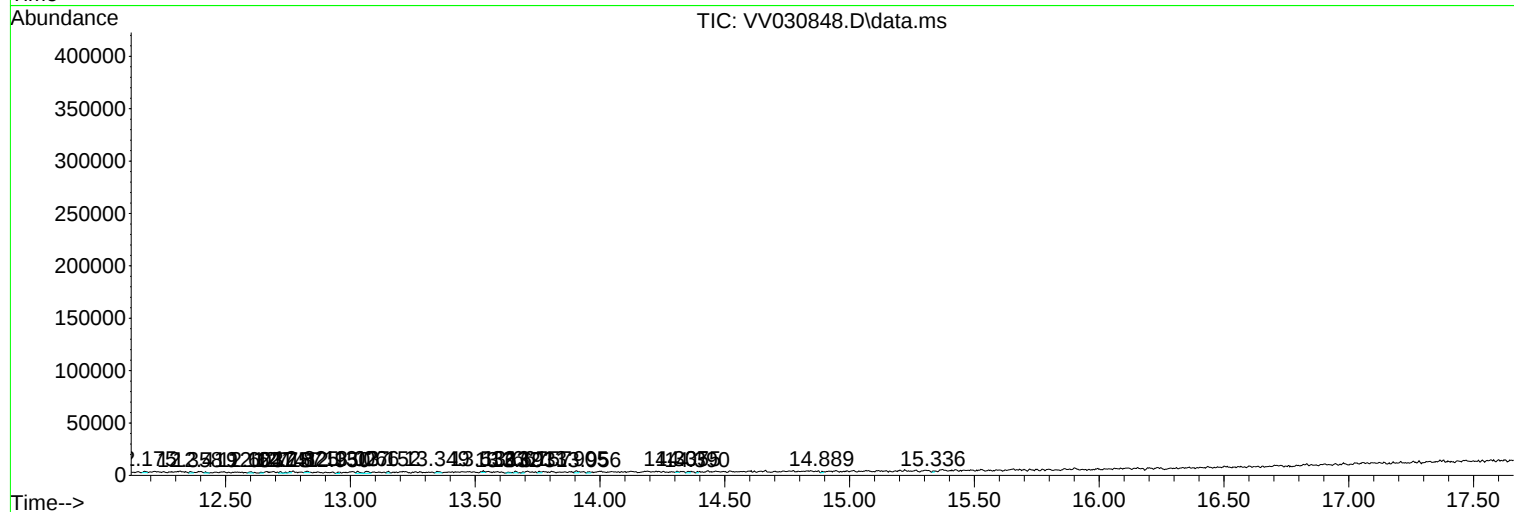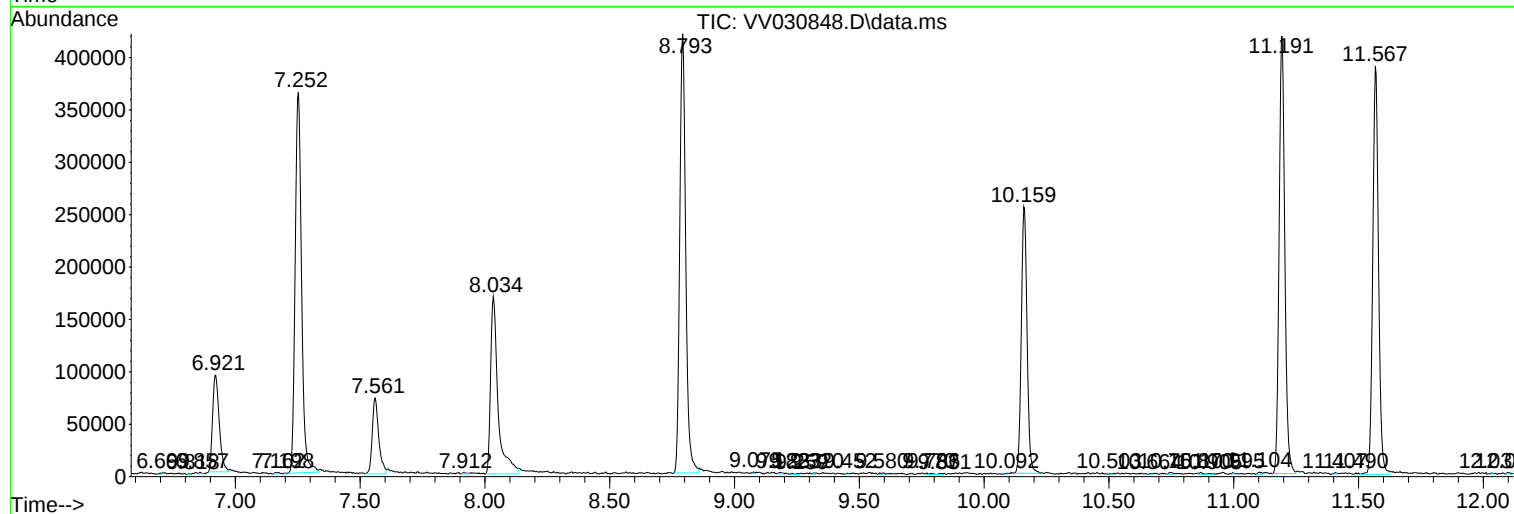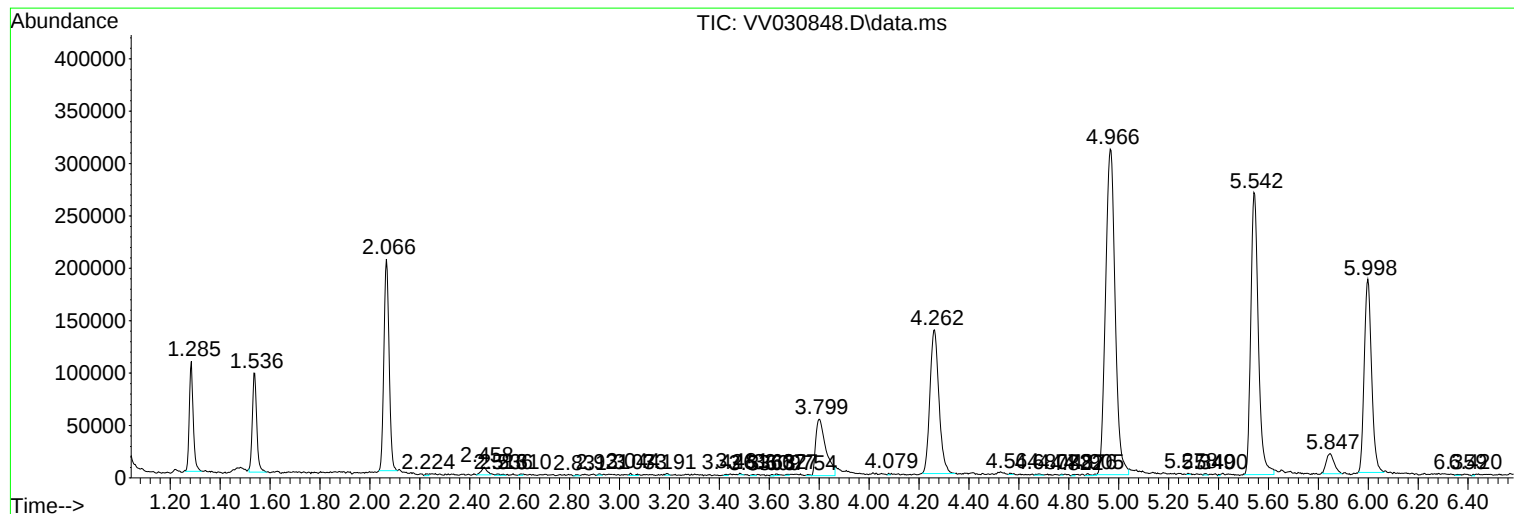

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
Data File : VV030848.D
Acq On : 25 Apr 2023 19:40
Operator : SY/MD
Sample : 02475-06 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AW8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
Data File : VV030848.D
Acq On : 25 Apr 2023 19:40
Operator : SY/MD
Sample : 02475-06 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AW8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------