

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
 Data File : VV030852.D
 Acq On : 25 Apr 2023 21:39
 Operator : SY/MD
 Sample : VV0425WBL02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK335

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M

Title : VOC Analysis

Signal : TIC: VV030852.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	69	75	88	rVB	104333	112767	13.41%	1.715%
2	1.536	148	154	167	rVB	90450	107601	12.80%	1.636%
3	2.063	309	318	333	rBV	203917	301531	35.87%	4.585%
4	2.362	408	411	414	rBV4	1460	1239	0.15%	0.019%
5	2.564	472	474	479	rVB5	1328	979	0.12%	0.015%
6	2.590	479	482	483	rBV3	937	630	0.07%	0.010%
7	2.651	497	501	504	rBV6	1043	908	0.11%	0.014%
8	2.683	508	511	512	rBV2	1484	786	0.09%	0.012%
9	2.786	535	543	545	rBV7	1138	1203	0.14%	0.018%
10	2.918	581	584	586	rBV4	1303	826	0.10%	0.013%
11	3.060	624	628	633	rVV6	1310	1234	0.15%	0.019%
12	3.111	641	644	646	rBV5	1277	845	0.10%	0.013%
13	3.198	668	671	673	rBV4	1537	784	0.09%	0.012%
14	3.278	694	696	699	rBV4	1278	583	0.07%	0.009%
15	3.378	721	727	732	rVB10	1170	1175	0.14%	0.018%
16	3.420	736	740	742	rVB3	964	639	0.08%	0.010%
17	3.507	763	767	769	rBV4	1473	1232	0.15%	0.019%
18	3.658	812	814	820	rVB6	899	678	0.08%	0.010%
19	3.706	826	829	831	rBV4	1451	847	0.10%	0.013%
20	3.796	848	857	884	rBV2	53518	152417	18.13%	2.318%
21	4.162	969	971	974	rBV3	1628	1001	0.12%	0.015%
22	4.259	986	1001	1022	rBV2	134539	341987	40.68%	5.201%
23	4.799	1166	1169	1172	rBV4	1058	717	0.09%	0.011%
24	4.966	1203	1221	1247	rBV2	315952	840680	100.00%	12.784%
25	5.227	1298	1302	1303	rBV4	1390	907	0.11%	0.014%
26	5.336	1334	1336	1339	rVB4	1661	951	0.11%	0.014%
27	5.387	1349	1352	1353	rBV3	1344	689	0.08%	0.010%
28	5.542	1386	1400	1422	rBV	268465	560533	66.68%	8.524%
29	5.998	1529	1542	1564	rBV	180689	382381	45.48%	5.815%
30	6.227	1611	1613	1615	rBV2	1638	682	0.08%	0.010%
31	6.304	1635	1637	1639	rVB3	1765	646	0.08%	0.010%
32	6.323	1639	1643	1645	rVB5	1245	831	0.10%	0.013%
33	6.342	1645	1649	1652	rBV4	2001	1257	0.15%	0.019%
34	6.365	1653	1656	1659	rBV4	1675	1008	0.12%	0.015%
35	6.413	1670	1671	1673	rBV2	1201	583	0.07%	0.009%
36	6.555	1711	1715	1719	rBV7	1922	1628	0.19%	0.025%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
 Data File : VV030852.D
 Acq On : 25 Apr 2023 21:39
 Operator : SY/MD
 Sample : VV0425WBL02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK335

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	6.619	1732	1735	1737	rBV4	1337	839	0.10%	0.013%
38	6.680	1752	1754	1761	rVB6	1746	1720	0.20%	0.026%
39	6.873	1812	1814	1817	rBV4	1212	865	0.10%	0.013%
40	6.921	1817	1829	1851	rBV	96412	180717	21.50%	2.748%
41	7.149	1898	1900	1903	rBV3	1280	898	0.11%	0.014%
42	7.252	1921	1932	1950	rBV	350458	627127	74.60%	9.537%
43	7.506	2009	2011	2016	rVB6	937	603	0.07%	0.009%
44	7.561	2017	2028	2048	rBV	70369	132106	15.71%	2.009%
45	7.915	2130	2138	2144	rBV8	2830	4545	0.54%	0.069%
46	8.034	2165	2175	2202	rBV	164566	332700	39.58%	5.059%
47	8.448	2302	2304	2308	rBV5	1236	682	0.08%	0.010%
48	8.593	2345	2349	2353	rVB6	1535	1156	0.14%	0.018%
49	8.719	2384	2388	2392	rBV8	1545	1871	0.22%	0.028%
50	8.792	2400	2411	2431	rBV	414033	686482	81.66%	10.439%
51	9.143	2518	2520	2523	rBV4	1416	805	0.10%	0.012%
52	9.436	2609	2611	2615	rBV4	992	766	0.09%	0.012%
53	9.603	2661	2663	2666	rVV4	1689	1077	0.13%	0.016%
54	9.677	2681	2686	2692	rVB9	1968	2170	0.26%	0.033%
55	9.738	2698	2705	2708	rBV8	1584	1982	0.24%	0.030%
56	9.789	2714	2721	2724	rBV6	1758	2425	0.29%	0.037%
57	9.928	2762	2764	2770	rVB7	2082	1306	0.16%	0.020%
58	9.982	2777	2781	2785	rBV5	1164	767	0.09%	0.012%
59	10.018	2789	2792	2795	rBV5	966	708	0.08%	0.011%
60	10.095	2814	2816	2817	rBV2	1271	589	0.07%	0.009%
61	10.104	2817	2819	2822	rVV4	1290	682	0.08%	0.010%
62	10.162	2824	2837	2856	rVV	249584	406075	48.30%	6.175%
63	10.355	2890	2897	2898	rBV6	1145	912	0.11%	0.014%
64	10.834	3042	3046	3049	rBV6	1710	1383	0.16%	0.021%
65	10.860	3050	3054	3061	rVB8	2663	4061	0.48%	0.062%
66	11.082	3121	3123	3125	rVB3	1252	586	0.07%	0.009%
67	11.098	3125	3128	3129	rBV3	1558	928	0.11%	0.014%
68	11.194	3146	3158	3177	rBV	420232	670039	79.70%	10.189%
69	11.323	3196	3198	3201	rVB4	1438	796	0.09%	0.012%
70	11.432	3229	3232	3235	rVB4	1172	753	0.09%	0.011%
71	11.571	3263	3275	3291	rBV	370685	611584	72.75%	9.300%
72	11.693	3311	3313	3317	rVB4	1910	1296	0.15%	0.020%
73	11.792	3340	3344	3348	rBV6	1433	1595	0.19%	0.024%
74	12.034	3414	3419	3420	rBV5	1027	822	0.10%	0.013%
75	12.111	3440	3443	3444	rBV3	1411	691	0.08%	0.011%
76	12.140	3449	3452	3454	rVB3	1234	665	0.08%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
 Data File : VV030852.D
 Acq On : 25 Apr 2023 21:39
 Operator : SY/MD
 Sample : VV0425WBL02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK335

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	12.156	3454	3457	3459	rBV3	1370	738	0.09%	0.011%
78	12.201	3467	3471	3474	rBV5	943	769	0.09%	0.012%
79	12.226	3477	3479	3483	rVV4	1027	647	0.08%	0.010%
80	12.355	3517	3519	3523	rBV4	1453	880	0.10%	0.013%
81	12.538	3572	3576	3577	rBV3	1450	751	0.09%	0.011%
82	12.706	3624	3628	3630	rBV4	1194	711	0.08%	0.011%
83	12.747	3637	3641	3642	rBV3	1116	673	0.08%	0.010%
84	12.802	3654	3658	3661	rBV4	1282	1106	0.13%	0.017%
85	12.828	3664	3666	3670	rVV4	1015	683	0.08%	0.010%
86	13.062	3735	3739	3740	rBV3	1123	865	0.10%	0.013%
87	13.214	3778	3786	3793	rVB3	5060	8823	1.05%	0.134%
88	13.316	3816	3818	3822	rVV3	924	679	0.08%	0.010%
89	13.413	3844	3848	3849	rVV4	1322	745	0.09%	0.011%
90	13.448	3849	3859	3871	rBV	13731	25630	3.05%	0.390%
91	13.574	3894	3898	3900	rBV5	937	694	0.08%	0.011%
92	13.693	3928	3935	3944	rVB5	5946	9045	1.08%	0.138%
93	13.750	3951	3953	3957	rVB4	1170	679	0.08%	0.010%
94	13.799	3965	3968	3970	rBV4	1697	1182	0.14%	0.018%
95	13.969	4017	4021	4023	rVV6	2291	1823	0.22%	0.028%
96	14.014	4033	4035	4039	rVB5	1248	820	0.10%	0.012%
97	14.114	4061	4066	4068	rBV6	1467	1005	0.12%	0.015%
98	14.284	4116	4119	4122	rBV5	1179	1030	0.12%	0.016%
99	14.509	4187	4189	4192	rVB4	1371	615	0.07%	0.009%
100	14.850	4289	4295	4297	rBV6	2147	2194	0.26%	0.033%




Sum of corrected areas: 6575946

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
Data File : VV030852.D
Acq On : 25 Apr 2023 21:39
Operator : SY/MD
Sample : VV0425WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK335

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

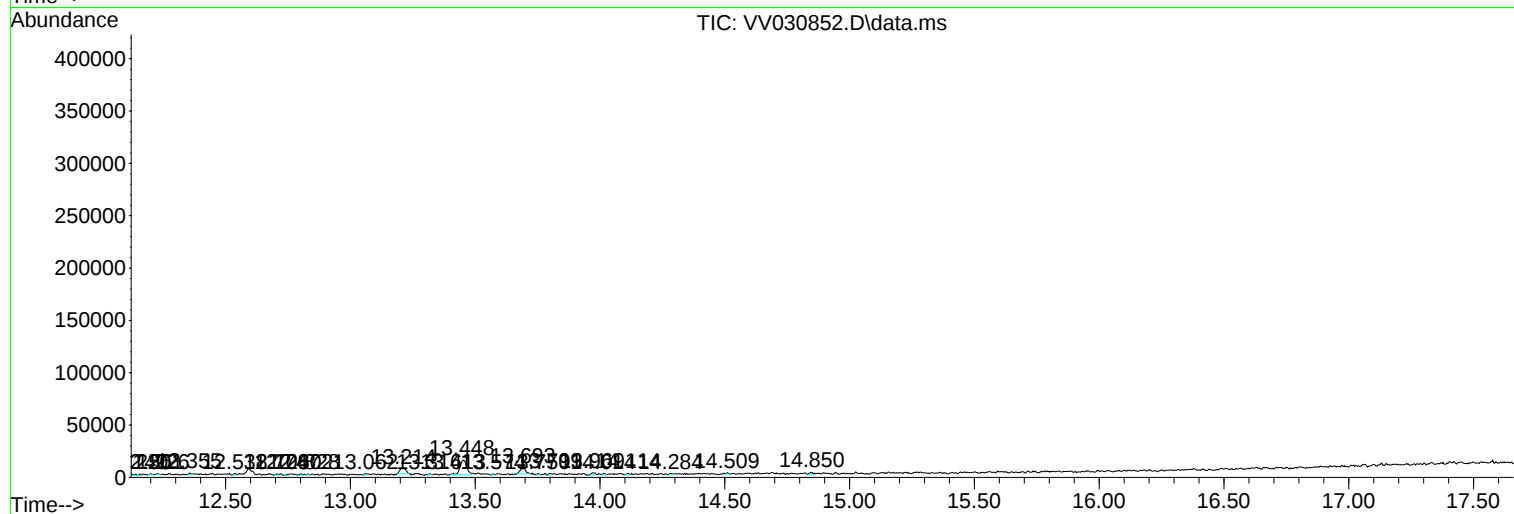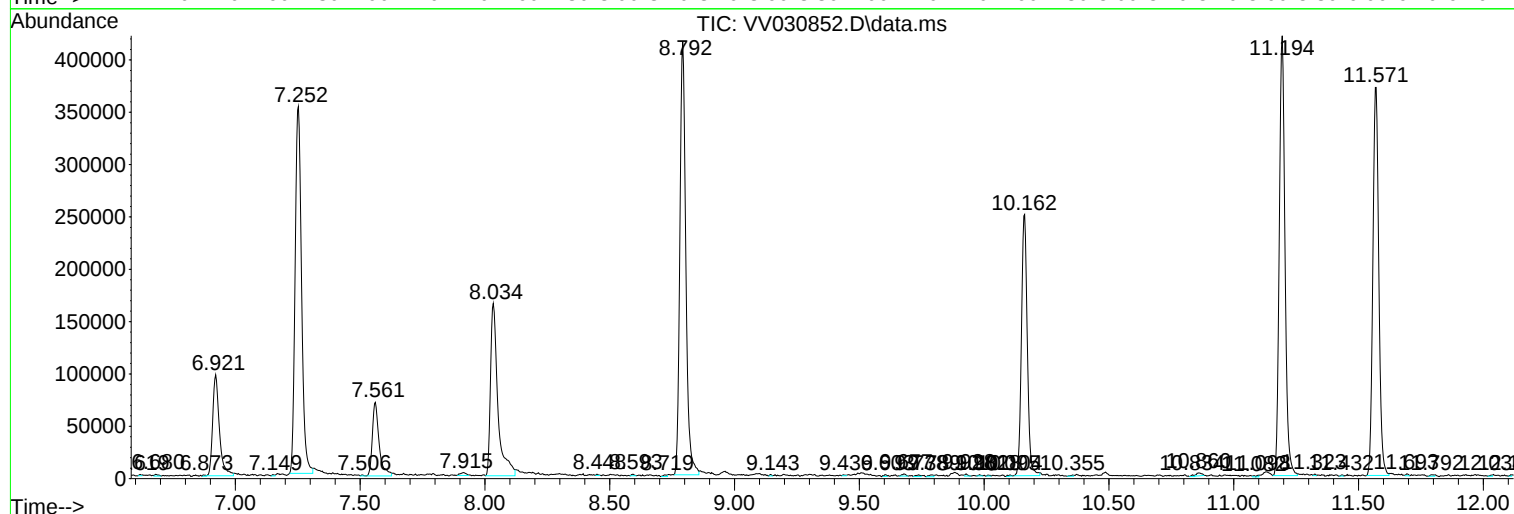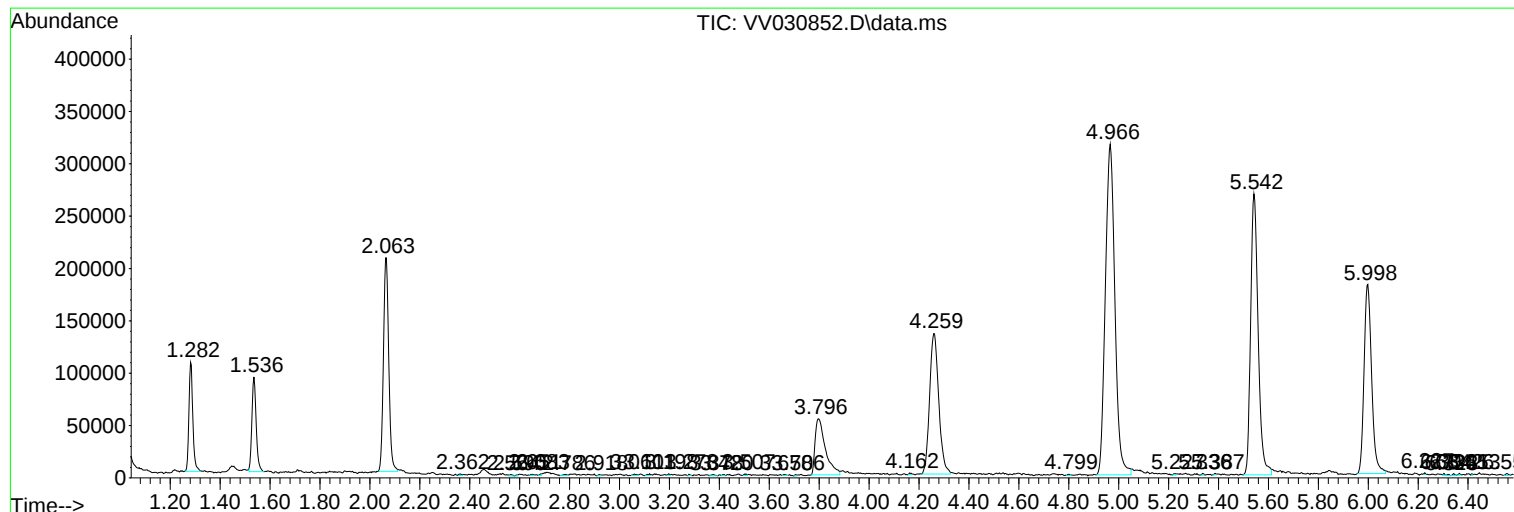

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
Data File : VV030852.D
Acq On : 25 Apr 2023 21:39
Operator : SY/MD
Sample : VV0425WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK335

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
Data File : VV030852.D
Acq On : 25 Apr 2023 21:39
Operator : SY/MD
Sample : VV0425WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK335

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------