

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
 Data File : VV030853.D
 Acq On : 25 Apr 2023 22:19
 Operator : SY/MD
 Sample : 02474-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AS3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030853.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	69	75	90	rVB	89125	99880	12.79%	1.623%
2	1.536	148	154	163	rVB	86058	98229	12.58%	1.596%
3	2.063	309	318	332	rBV	177022	256730	32.87%	4.172%
4	2.359	407	410	412	rBV4	1482	755	0.10%	0.012%
5	2.687	510	512	513	rBV2	1434	655	0.08%	0.011%
6	2.764	533	536	542	rVB7	1389	1067	0.14%	0.017%
7	2.950	591	594	599	rBV6	1485	1067	0.14%	0.017%
8	3.108	640	643	644	rBV2	1284	690	0.09%	0.011%
9	3.288	694	699	700	rBV5	876	910	0.12%	0.015%
10	3.323	707	710	712	rBV4	672	560	0.07%	0.009%
11	3.359	719	721	724	rBV4	1633	968	0.12%	0.016%
12	3.584	785	791	793	rBV4	2157	1447	0.19%	0.024%
13	3.642	806	809	811	rBV2	1389	779	0.10%	0.013%
14	3.664	811	816	819	rVB6	1485	1312	0.17%	0.021%
15	3.683	819	822	824	rBV3	1294	824	0.11%	0.013%
16	3.696	824	826	828	rBV3	1038	548	0.07%	0.009%
17	3.799	847	858	881	rBV	51691	150518	19.27%	2.446%
18	4.098	949	951	955	rBV5	1184	889	0.11%	0.014%
19	4.256	986	1000	1023	rBV	124727	319934	40.96%	5.200%
20	4.818	1173	1175	1178	rBV3	1019	583	0.07%	0.009%
21	4.870	1189	1191	1195	rBV4	853	629	0.08%	0.010%
22	4.963	1203	1220	1245	rBV2	291338	781043	100.00%	12.693%
23	5.288	1319	1321	1326	rVV6	1132	993	0.13%	0.016%
24	5.387	1349	1352	1354	rBV3	1468	781	0.10%	0.013%
25	5.539	1388	1399	1423	rVV	254022	524930	67.21%	8.531%
26	5.995	1525	1541	1566	rBV	174348	370397	47.42%	6.020%
27	6.204	1603	1606	1608	rBV4	1236	711	0.09%	0.012%
28	6.233	1613	1615	1621	rVB7	1756	1340	0.17%	0.022%
29	6.394	1663	1665	1668	rVB4	1996	968	0.12%	0.016%
30	6.423	1668	1674	1675	rBV5	1522	1088	0.14%	0.018%
31	6.510	1699	1701	1706	rVB6	1256	711	0.09%	0.012%
32	6.532	1706	1708	1714	rBV7	1082	1080	0.14%	0.018%
33	6.555	1714	1715	1719	rVB3	1169	578	0.07%	0.009%
34	6.574	1719	1721	1725	rBV4	1362	1105	0.14%	0.018%
35	6.645	1742	1743	1748	rVB5	1402	751	0.10%	0.012%
36	6.699	1758	1760	1763	rBV4	1460	742	0.10%	0.012%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042523\
 Data File : VW030853.D
 Acq On : 25 Apr 2023 22:19
 Operator : SY/MD
 Sample : 02474-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AS3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	6.719	1763	1766	1769	rVB5	867	655	0.08%	0.011%
38	6.918	1817	1828	1848	rBV2	88338	173256	22.18%	2.816%
39	7.140	1895	1897	1899	rBV3	1030	572	0.07%	0.009%
40	7.249	1920	1931	1950	rBV	329962	583968	74.77%	9.491%
41	7.461	1994	1997	2001	rBV6	1602	1044	0.13%	0.017%
42	7.506	2009	2011	2013	rBV3	1239	549	0.07%	0.009%
43	7.558	2019	2027	2051	rBV2	63843	117732	15.07%	1.913%
44	8.034	2164	2175	2191	rBV	154908	288503	36.94%	4.689%
45	8.461	2305	2308	2310	rBV4	1297	596	0.08%	0.010%
46	8.593	2346	2349	2356	rVB9	2056	1835	0.23%	0.030%
47	8.635	2361	2362	2371	rVB7	1092	815	0.10%	0.013%
48	8.789	2399	2410	2431	rBV	385582	658424	84.30%	10.701%
49	9.085	2496	2502	2510	rVB	3300	4815	0.62%	0.078%
50	9.339	2574	2581	2584	rBV9	1250	1306	0.17%	0.021%
51	9.828	2730	2733	2737	rBV5	1260	835	0.11%	0.014%
52	10.159	2825	2836	2856	rVV	236456	385769	49.39%	6.269%
53	10.281	2870	2874	2878	rBV5	1044	1164	0.15%	0.019%
54	10.336	2881	2891	2899	rVV3	10511	16832	2.16%	0.274%
55	10.387	2904	2907	2910	rBV5	1388	954	0.12%	0.016%
56	10.407	2910	2913	2915	rBV3	1101	686	0.09%	0.011%
57	10.448	2923	2926	2928	rBV3	1315	838	0.11%	0.014%
58	10.583	2965	2968	2971	rBV5	1329	906	0.12%	0.015%
59	10.741	3015	3017	3022	rVB5	1297	811	0.10%	0.013%
60	10.773	3025	3027	3030	rBV3	835	589	0.08%	0.010%
61	10.841	3044	3048	3049	rBV4	1750	1041	0.13%	0.017%
62	11.133	3125	3139	3146	rBV4	4297	9458	1.21%	0.154%
63	11.191	3146	3157	3176	rBV	399675	637955	81.68%	10.368%
64	11.384	3215	3217	3219	rBV4	990	661	0.08%	0.011%
65	11.458	3238	3240	3242	rBV3	1449	565	0.07%	0.009%
66	11.506	3245	3255	3262	rVV10	6023	12030	1.54%	0.196%
67	11.567	3264	3274	3292	rVB	364514	576028	73.75%	9.362%
68	11.802	3344	3347	3349	rBV3	939	626	0.08%	0.010%
69	11.905	3376	3379	3382	rVB4	1320	805	0.10%	0.013%
70	12.159	3454	3458	3461	rVB4	1519	1230	0.16%	0.020%
71	12.288	3496	3498	3500	rBV2	1735	1005	0.13%	0.016%
72	12.371	3519	3524	3527	rBV6	1664	1615	0.21%	0.026%
73	12.416	3532	3538	3540	rBV6	1255	989	0.13%	0.016%
74	12.458	3548	3551	3554	rBV5	720	596	0.08%	0.010%
75	12.503	3563	3565	3569	rVB5	1067	557	0.07%	0.009%
76	12.583	3586	3590	3591	rBV4	3599	1904	0.24%	0.031%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
 Data File : VV030853.D
 Acq On : 25 Apr 2023 22:19
 Operator : SY/MD
 Sample : 02474-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AS3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	12.632	3603	3605	3610	rVV5	1406	832	0.11%	0.014%
78	12.657	3610	3613	3615	rVB4	1200	749	0.10%	0.012%
79	12.670	3615	3617	3621	rVB5	918	580	0.07%	0.009%
80	12.693	3621	3624	3626	rVB4	1237	654	0.08%	0.011%
81	12.712	3627	3630	3634	rVB5	1195	809	0.10%	0.013%
82	12.731	3634	3636	3638	rBV3	854	599	0.08%	0.010%
83	12.776	3647	3650	3652	rBV4	1480	762	0.10%	0.012%
84	12.927	3694	3697	3700	rVB5	1075	714	0.09%	0.012%
85	12.995	3716	3718	3723	rBV5	1561	1253	0.16%	0.020%
86	13.130	3759	3760	3762	rVV2	1351	562	0.07%	0.009%
87	13.146	3763	3765	3768	rVV3	1767	1113	0.14%	0.018%
88	13.181	3771	3776	3778	rBV6	2069	1605	0.21%	0.026%
89	13.214	3778	3786	3798	rVB6	5536	9991	1.28%	0.162%
90	13.519	3878	3881	3884	rBV5	1171	920	0.12%	0.015%
91	13.538	3884	3887	3890	rVB4	1537	891	0.11%	0.014%
92	13.693	3926	3935	3938	rBV9	5131	7058	0.90%	0.115%
93	13.808	3968	3971	3973	rBV4	799	591	0.08%	0.010%
94	14.027	4035	4039	4041	rBV4	1508	998	0.13%	0.016%
95	14.345	4136	4138	4140	rBV2	1514	620	0.08%	0.010%
96	14.406	4155	4157	4159	rVB3	1362	643	0.08%	0.010%
97	14.429	4160	4164	4166	rBV4	1306	1001	0.13%	0.016%
98	14.660	4233	4236	4238	rBV4	1577	1057	0.14%	0.017%
99	15.172	4393	4395	4399	rBV4	1391	879	0.11%	0.014%
100	15.326	4440	4443	4446	rBV5	2240	1536	0.20%	0.025%




Sum of corrected areas: 6153128

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
Data File : VV030853.D
Acq On : 25 Apr 2023 22:19
Operator : SY/MD
Sample : 02474-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AS3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

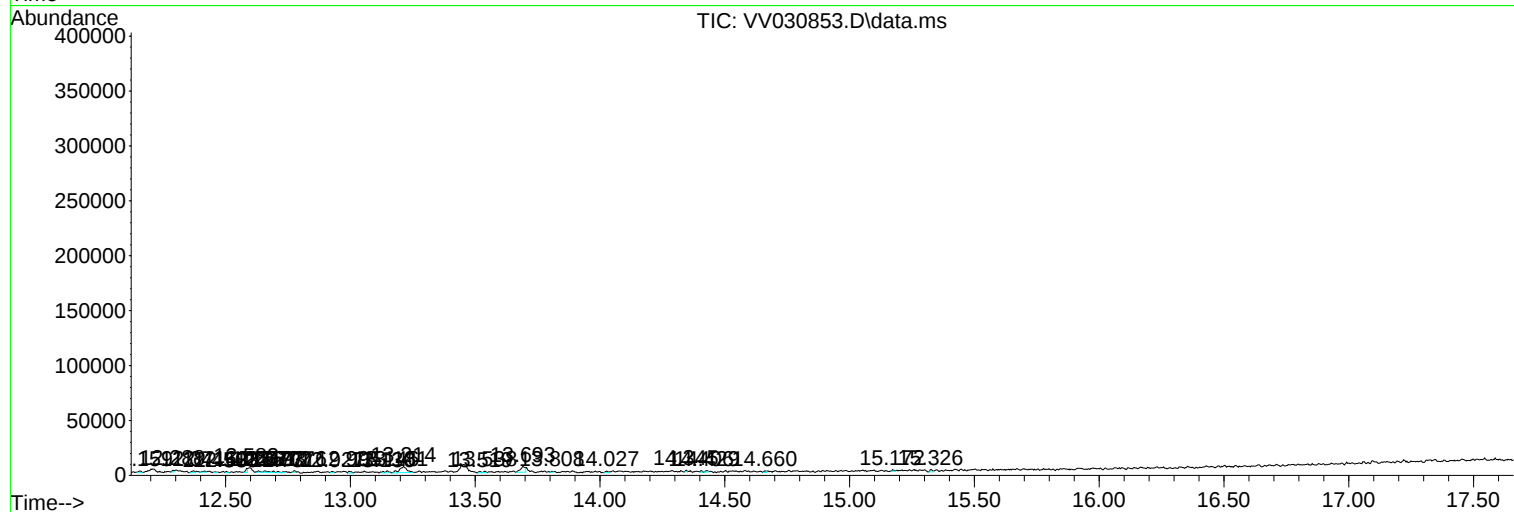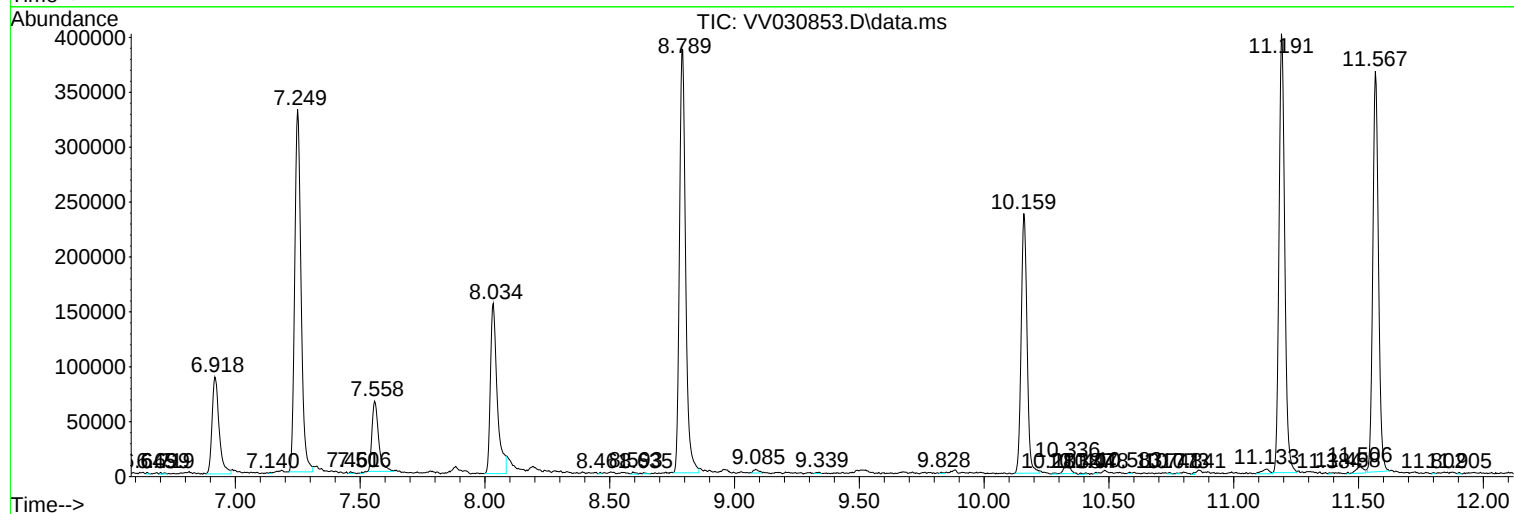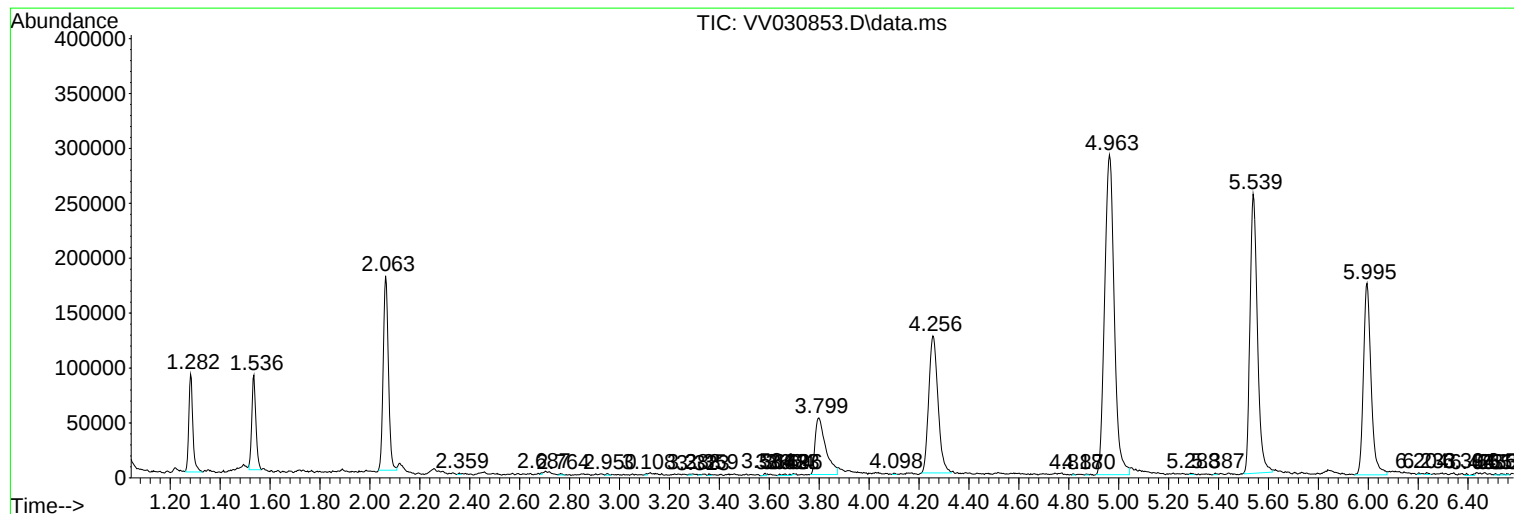

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
Data File : VV030853.D
Acq On : 25 Apr 2023 22:19
Operator : SY/MD
Sample : 02474-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AS3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
Data File : VV030853.D
Acq On : 25 Apr 2023 22:19
Operator : SY/MD
Sample : 02474-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AS3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc