

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
 Data File : VV030854.D
 Acq On : 25 Apr 2023 22:43
 Operator : SY/MD
 Sample : 02474-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AS4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030854.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	87	rBV	101657	111242	13.34%	1.696%
2	1.535	148	154	167	rVB	87251	106192	12.74%	1.619%
3	2.066	310	319	332	rBV	205105	299526	35.93%	4.566%
4	2.223	364	368	369	rBV4	1889	977	0.12%	0.015%
5	2.317	395	397	401	rBV4	1100	641	0.08%	0.010%
6	2.561	469	473	476	rBV6	1460	1270	0.15%	0.019%
7	2.629	491	494	496	rBV3	1548	819	0.10%	0.012%
8	2.757	530	534	536	rBV5	1429	899	0.11%	0.014%
9	2.789	542	544	547	rBV4	1900	1120	0.13%	0.017%
10	2.985	602	605	607	rBV4	1404	796	0.10%	0.012%
11	3.024	613	617	621	rBV7	1198	959	0.12%	0.015%
12	3.059	624	628	632	rBV6	2119	1586	0.19%	0.024%
13	3.095	634	639	641	rBV6	1312	1007	0.12%	0.015%
14	3.127	645	649	652	rBV4	1688	1165	0.14%	0.018%
15	3.156	656	658	663	rBV5	1231	1057	0.13%	0.016%
16	3.194	667	670	671	rBV2	1349	655	0.08%	0.010%
17	3.365	721	723	726	rBV4	1516	837	0.10%	0.013%
18	3.445	744	748	751	rBV4	1314	1109	0.13%	0.017%
19	3.519	766	771	774	rVB7	1476	1131	0.14%	0.017%
20	3.612	798	800	804	rBV5	1203	704	0.08%	0.011%
21	3.796	848	857	884	rBV	56014	158791	19.05%	2.420%
22	4.185	974	978	979	rBV4	1116	698	0.08%	0.011%
23	4.259	989	1001	1022	rVB	135315	331495	39.77%	5.053%
24	4.815	1170	1174	1176	rBV4	1207	841	0.10%	0.013%
25	4.966	1204	1221	1243	rBV2	316411	833628	100.00%	12.707%
26	5.278	1311	1318	1322	rBV8	1857	2186	0.26%	0.033%
27	5.442	1367	1369	1372	rBV3	889	747	0.09%	0.011%
28	5.542	1388	1400	1419	rVV	276870	564250	67.69%	8.601%
29	5.998	1525	1542	1560	rBV	186730	389424	46.71%	5.936%
30	6.246	1615	1619	1620	rBV4	1038	842	0.10%	0.013%
31	6.474	1685	1690	1692	rBV6	1391	1210	0.15%	0.018%
32	6.513	1697	1702	1705	rVB6	1737	1374	0.16%	0.021%
33	6.529	1705	1707	1710	rBV3	1249	904	0.11%	0.014%
34	6.645	1741	1743	1745	rVB3	1809	743	0.09%	0.011%
35	6.825	1796	1799	1803	rVB5	1037	913	0.11%	0.014%
36	6.847	1803	1806	1808	rBV2	1600	1189	0.14%	0.018%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042523\
 Data File : VW030854.D
 Acq On : 25 Apr 2023 22:43
 Operator : SY/MD
 Sample : 02474-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AS4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	6.921	1818	1829	1847	rBV	94242	180174	21.61%	2.746%
38	7.214	1918	1920	1921	rVV2	1284	680	0.08%	0.010%
39	7.249	1921	1931	1952	rVV	352414	632716	75.90%	9.645%
40	7.561	2019	2028	2045	rBV	71371	125823	15.09%	1.918%
41	7.857	2118	2120	2121	rBV2	1664	634	0.08%	0.010%
42	8.034	2165	2175	2205	rBV	171479	349429	41.92%	5.326%
43	8.361	2273	2277	2282	rVB8	1363	1073	0.13%	0.016%
44	8.792	2398	2411	2430	rBV	425224	707558	84.88%	10.786%
45	9.062	2493	2495	2499	rBV5	1562	1016	0.12%	0.015%
46	9.101	2502	2507	2509	rBV4	1537	1244	0.15%	0.019%
47	9.236	2544	2549	2557	rVB10	1197	1505	0.18%	0.023%
48	9.361	2583	2588	2591	rBV7	1306	1367	0.16%	0.021%
49	9.419	2599	2606	2608	rBV6	1556	1556	0.19%	0.024%
50	9.615	2663	2667	2668	rBV4	1374	839	0.10%	0.013%
51	9.770	2711	2715	2717	rBV4	1287	730	0.09%	0.011%
52	9.805	2724	2726	2728	rBV3	1197	756	0.09%	0.012%
53	9.898	2753	2755	2761	rVB6	1156	860	0.10%	0.013%
54	9.931	2761	2765	2768	rBV6	1153	814	0.10%	0.012%
55	10.017	2790	2792	2798	rVB7	1475	1002	0.12%	0.015%
56	10.159	2825	2836	2861	rVB	253415	410780	49.28%	6.262%
57	10.435	2918	2922	2924	rVB5	1084	818	0.10%	0.012%
58	10.477	2931	2935	2937	rBV4	1358	1006	0.12%	0.015%
59	10.554	2956	2959	2960	rBV3	1333	656	0.08%	0.010%
60	10.657	2988	2991	2995	rBV6	813	641	0.08%	0.010%
61	10.789	3029	3032	3035	rVV5	1769	1111	0.13%	0.017%
62	10.985	3089	3093	3099	rBV7	1209	1166	0.14%	0.018%
63	11.127	3134	3137	3140	rBV4	1244	1093	0.13%	0.017%
64	11.194	3147	3158	3175	rBV	408546	659252	79.08%	10.049%
65	11.512	3253	3257	3258	rBV3	1878	1343	0.16%	0.020%
66	11.567	3264	3274	3297	rVB	376061	610933	73.29%	9.313%
67	11.776	3336	3339	3343	rVB5	1833	1607	0.19%	0.024%
68	11.815	3347	3351	3352	rBV4	1094	697	0.08%	0.011%
69	11.873	3367	3369	3373	rVB4	1781	1114	0.13%	0.017%
70	11.895	3373	3376	3381	rBV7	1222	970	0.12%	0.015%
71	11.982	3398	3403	3406	rBV5	1687	1481	0.18%	0.023%
72	12.014	3411	3413	3415	rBV3	1364	661	0.08%	0.010%
73	12.207	3469	3473	3474	rBV3	1828	1018	0.12%	0.016%
74	12.303	3498	3503	3505	rBV5	1930	1287	0.15%	0.020%
75	12.342	3512	3515	3518	rBV5	1753	984	0.12%	0.015%
76	12.496	3561	3563	3567	rVB5	1149	866	0.10%	0.013%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
 Data File : VV030854.D
 Acq On : 25 Apr 2023 22:43
 Operator : SY/MD
 Sample : 02474-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AS4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	12.561	3579	3583	3585	rVB5	1352	955	0.11%	0.015%
78	12.664	3611	3615	3617	rBV3	1131	792	0.10%	0.012%
79	13.014	3722	3724	3728	rBV5	1060	701	0.08%	0.011%
80	13.114	3752	3755	3760	rBV7	1174	994	0.12%	0.015%
81	13.136	3760	3762	3763	rBV2	1354	607	0.07%	0.009%
82	13.165	3769	3771	3774	rVB4	1227	654	0.08%	0.010%
83	13.207	3774	3784	3790	rBV4	4416	7226	0.87%	0.110%
84	13.255	3797	3799	3802	rBV5	1095	696	0.08%	0.011%
85	13.374	3834	3836	3839	rVV4	1004	631	0.08%	0.010%
86	13.557	3890	3893	3895	rBV4	1006	696	0.08%	0.011%
87	13.795	3966	3967	3971	rBV4	1240	687	0.08%	0.010%
88	13.885	3993	3995	3998	rBV4	1346	671	0.08%	0.010%
89	13.969	4019	4021	4025	rVB4	1551	1109	0.13%	0.017%
90	14.162	4078	4081	4087	rBV7	956	784	0.09%	0.012%
91	14.188	4087	4089	4090	rBV2	1183	629	0.08%	0.010%
92	14.242	4104	4106	4112	rVB7	1137	947	0.11%	0.014%
93	14.274	4112	4116	4120	rBV6	1019	963	0.12%	0.015%
94	14.303	4122	4125	4128	rBV5	1498	972	0.12%	0.015%
95	14.339	4134	4136	4139	rBV4	1243	661	0.08%	0.010%
96	14.358	4139	4142	4148	rVB6	1997	1652	0.20%	0.025%
97	14.390	4150	4152	4154	rBV3	1149	681	0.08%	0.010%
98	14.786	4271	4275	4277	rBV4	1180	945	0.11%	0.014%
99	14.898	4306	4310	4315	rBV7	1605	1696	0.20%	0.026%
100	15.139	4381	4385	4388	rBV5	1695	1725	0.21%	0.026%




Sum of corrected areas: 6560261

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
Data File : VV030854.D
Acq On : 25 Apr 2023 22:43
Operator : SY/MD
Sample : 02474-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AS4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

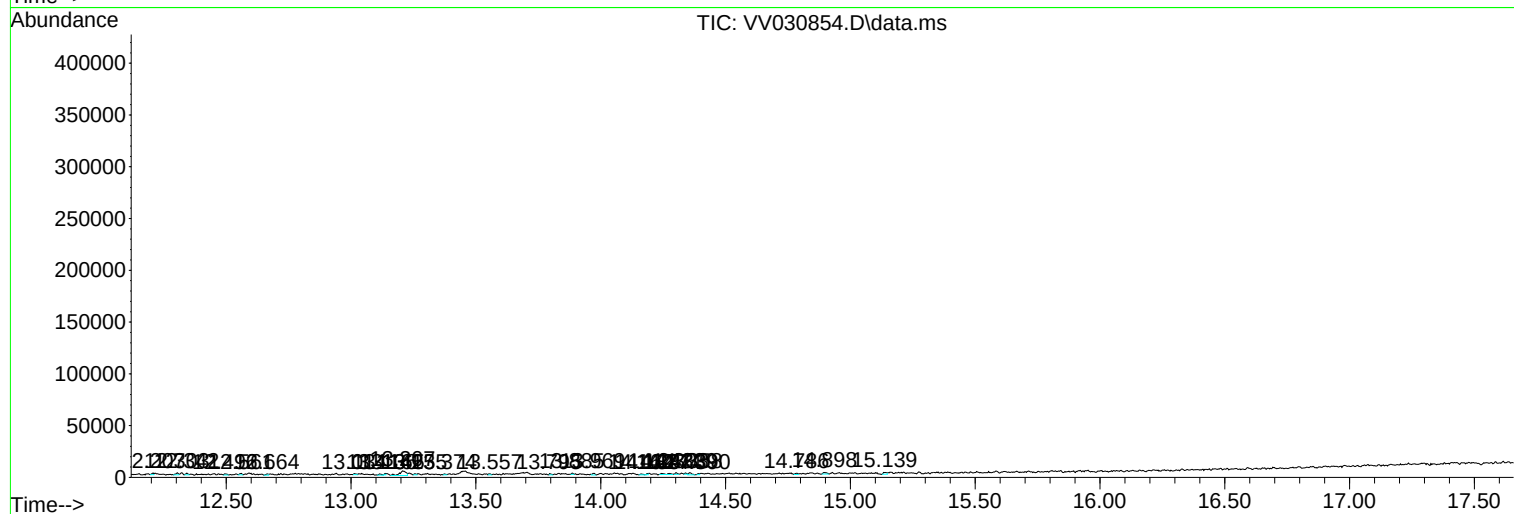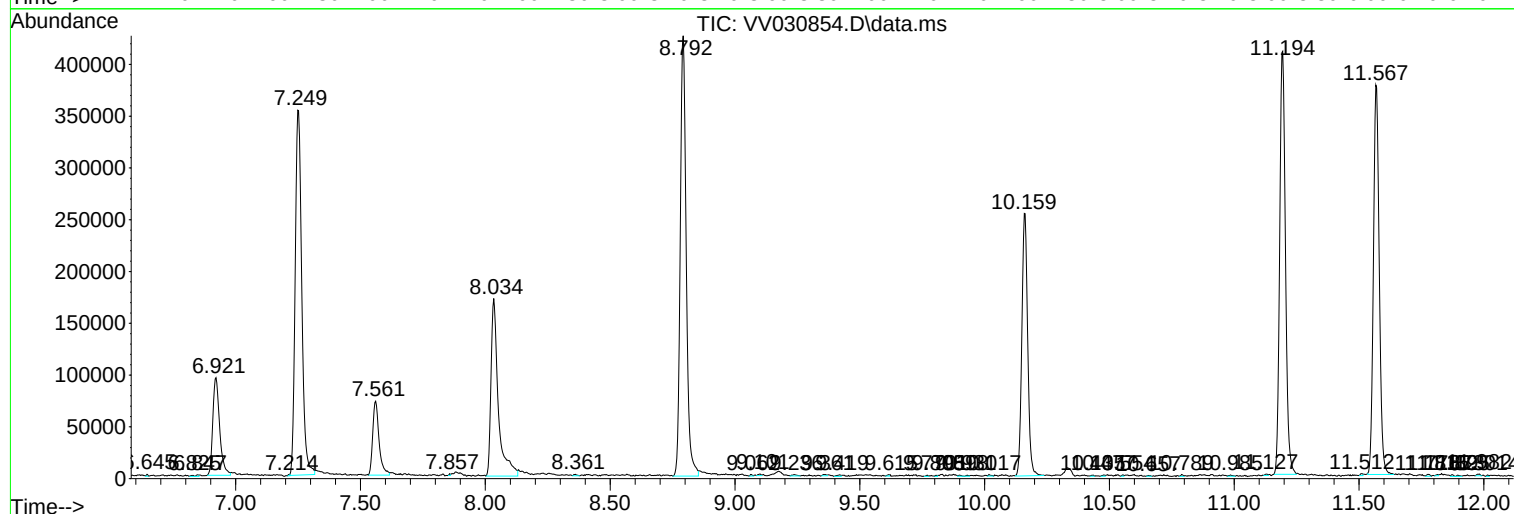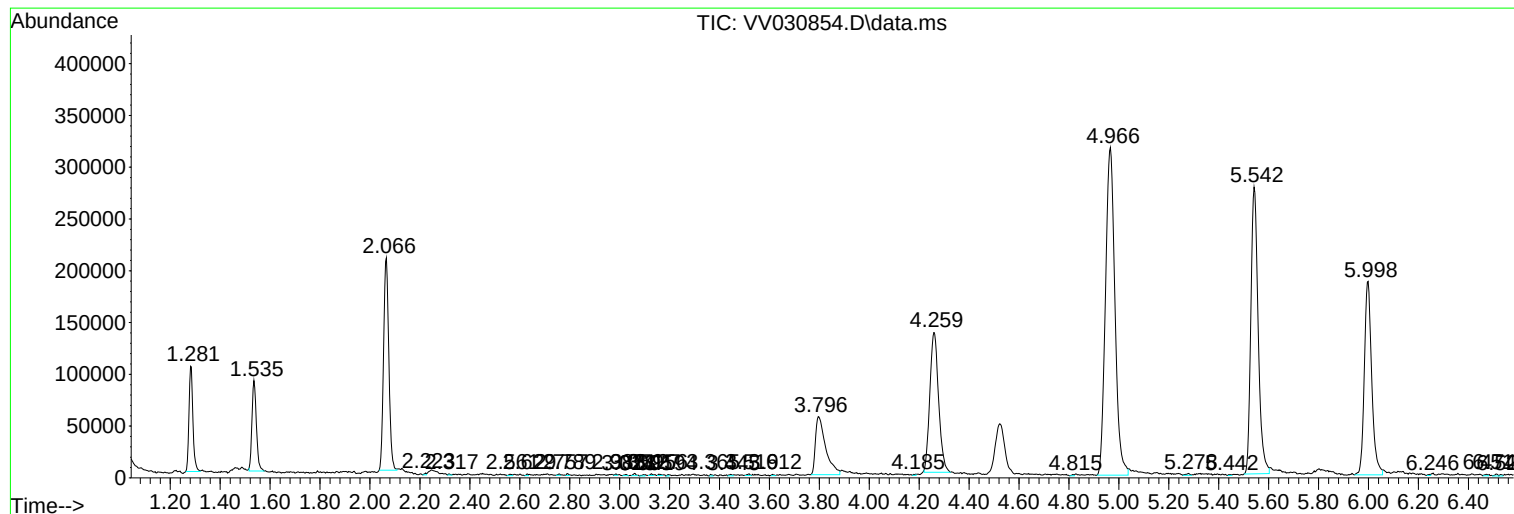

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
Data File : VV030854.D
Acq On : 25 Apr 2023 22:43
Operator : SY/MD
Sample : 02474-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AS4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
Data File : VV030854.D
Acq On : 25 Apr 2023 22:43
Operator : SY/MD
Sample : 02474-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AS4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------