

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
 Data File : VV030855.D
 Acq On : 25 Apr 2023 23:07
 Operator : SY/MD
 Sample : 02474-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AS5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030855.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	88	rVB	93077	100737	12.68%	1.610%
2	1.535	148	154	168	rVB	91306	105972	13.33%	1.693%
3	2.066	310	319	331	rBV	190865	276753	34.82%	4.423%
4	2.301	390	392	396	rVB3	2034	1382	0.17%	0.022%
5	2.381	414	417	419	rBV3	1308	1006	0.13%	0.016%
6	2.542	464	467	469	rVB3	974	569	0.07%	0.009%
7	2.558	469	472	474	rBV3	953	522	0.07%	0.008%
8	2.574	474	477	479	rBV4	1143	715	0.09%	0.011%
9	2.773	537	539	542	rVB4	1286	523	0.07%	0.008%
10	2.924	582	586	589	rBV5	1074	972	0.12%	0.016%
11	2.969	597	600	604	rBV3	1286	766	0.10%	0.012%
12	3.403	731	735	737	rBV5	888	807	0.10%	0.013%
13	3.413	737	738	742	rVV4	1387	591	0.07%	0.009%
14	3.439	742	746	748	rVB3	1329	960	0.12%	0.015%
15	3.455	748	751	756	rBV5	1185	1070	0.13%	0.017%
16	3.567	784	786	791	rBV6	1528	1155	0.15%	0.018%
17	3.606	796	798	802	rVB5	1209	799	0.10%	0.013%
18	3.632	802	806	807	rBV3	1070	818	0.10%	0.013%
19	3.796	847	857	885	rBV	54011	156868	19.74%	2.507%
20	4.198	980	982	984	rBV4	1108	532	0.07%	0.009%
21	4.259	989	1001	1022	rVB	130147	320684	40.35%	5.125%
22	4.387	1038	1041	1045	rVB6	2307	1603	0.20%	0.026%
23	4.445	1056	1059	1061	rVB3	1308	666	0.08%	0.011%
24	4.500	1074	1076	1078	rBV2	1379	742	0.09%	0.012%
25	4.680	1130	1132	1135	rBV3	752	482	0.06%	0.008%
26	4.722	1143	1145	1148	rBV5	989	592	0.07%	0.009%
27	4.966	1203	1221	1247	rBV2	296834	794744	100.00%	12.700%
28	5.542	1388	1400	1425	rBV	268735	554113	69.72%	8.855%
29	5.998	1528	1542	1558	rBV	180283	369295	46.47%	5.902%
30	6.307	1635	1638	1641	rBV5	1165	869	0.11%	0.014%
31	6.407	1666	1669	1671	rVB3	1160	637	0.08%	0.010%
32	6.538	1707	1710	1712	rBV4	1467	1034	0.13%	0.017%
33	6.757	1775	1778	1779	rBV3	1198	562	0.07%	0.009%
34	6.921	1815	1829	1846	rBV	91956	173530	21.83%	2.773%
35	7.153	1899	1901	1904	rBV4	1263	895	0.11%	0.014%
36	7.188	1909	1912	1913	rBV2	1209	694	0.09%	0.011%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042523\
 Data File : VW030855.D
 Acq On : 25 Apr 2023 23:07
 Operator : SY/MD
 Sample : 02474-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AS5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	7.252	1921	1932	1951	rBV	333118	593493	74.68%	9.484%
38	7.477	2000	2002	2003	rBV2	959	533	0.07%	0.009%
39	7.561	2018	2028	2043	rBV2	66314	119739	15.07%	1.914%
40	7.876	2123	2126	2127	rBV3	1669	1045	0.13%	0.017%
41	8.034	2165	2175	2205	rBV	161043	331164	41.67%	5.292%
42	8.712	2384	2386	2387	rBV2	1138	494	0.06%	0.008%
43	8.792	2401	2411	2443	rVB	408457	673239	84.71%	10.759%
44	9.062	2492	2495	2501	rBV7	1553	1578	0.20%	0.025%
45	9.136	2515	2518	2520	rBV5	1333	731	0.09%	0.012%
46	9.197	2533	2537	2539	rBV4	1242	1077	0.14%	0.017%
47	9.297	2563	2568	2570	rBV6	989	846	0.11%	0.014%
48	9.329	2575	2578	2579	rBV3	932	509	0.06%	0.008%
49	9.982	2776	2781	2785	rBV8	1565	1545	0.19%	0.025%
50	10.027	2791	2795	2796	rBV2	931	523	0.07%	0.008%
51	10.120	2822	2824	2826	rBV4	1203	490	0.06%	0.008%
52	10.162	2826	2837	2859	rVV	244742	393571	49.52%	6.290%
53	10.381	2902	2905	2907	rBV4	1151	809	0.10%	0.013%
54	10.509	2939	2945	2948	rVB7	1381	1419	0.18%	0.023%
55	10.538	2951	2954	2959	rVB6	1273	1251	0.16%	0.020%
56	10.564	2959	2962	2963	rBV3	1419	800	0.10%	0.013%
57	10.619	2976	2979	2981	rBV3	746	537	0.07%	0.009%
58	10.686	2996	3000	3003	rBV6	1346	1140	0.14%	0.018%
59	10.760	3020	3023	3026	rBV4	1067	643	0.08%	0.010%
60	10.776	3026	3028	3031	rVV3	1222	520	0.07%	0.008%
61	10.821	3040	3042	3046	rBV4	1091	798	0.10%	0.013%
62	10.844	3046	3049	3051	rBV3	1235	853	0.11%	0.014%
63	10.892	3062	3064	3066	rBV3	1361	578	0.07%	0.009%
64	10.927	3072	3075	3078	rBV3	881	789	0.10%	0.013%
65	11.049	3111	3113	3116	rVB3	1448	748	0.09%	0.012%
66	11.066	3116	3118	3121	rBV4	943	629	0.08%	0.010%
67	11.194	3144	3158	3174	rBV	405391	645380	81.21%	10.314%
68	11.358	3207	3209	3211	rBV2	960	537	0.07%	0.009%
69	11.570	3264	3275	3290	rBV	361516	574391	72.27%	9.179%
70	11.744	3326	3329	3331	rBV4	1678	1222	0.15%	0.020%
71	11.783	3336	3341	3342	rBV3	895	527	0.07%	0.008%
72	11.812	3346	3350	3353	rBV5	1110	1203	0.15%	0.019%
73	11.905	3377	3379	3380	rBV2	1030	514	0.06%	0.008%
74	11.956	3391	3395	3397	rBV4	1150	960	0.12%	0.015%
75	11.979	3399	3402	3404	rBV3	1288	866	0.11%	0.014%
76	12.024	3413	3416	3419	rBV5	1196	1103	0.14%	0.018%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
 Data File : VV030855.D
 Acq On : 25 Apr 2023 23:07
 Operator : SY/MD
 Sample : 02474-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AS5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	12.303	3499	3503	3504	rBV3	1468	1087	0.14%	0.017%
78	12.368	3521	3523	3524	rBV3	1094	574	0.07%	0.009%
79	12.615	3598	3600	3603	rBV3	1218	752	0.09%	0.012%
80	12.741	3635	3639	3643	rBV6	1827	1542	0.19%	0.025%
81	12.808	3657	3660	3661	rBV2	1456	722	0.09%	0.012%
82	12.966	3707	3709	3712	rVB5	1631	805	0.10%	0.013%
83	13.053	3733	3736	3738	rBV4	1026	608	0.08%	0.010%
84	13.094	3747	3749	3752	rBV3	1377	926	0.12%	0.015%
85	13.127	3757	3759	3763	rBV3	1530	1197	0.15%	0.019%
86	13.172	3769	3773	3777	rBV6	1350	1003	0.13%	0.016%
87	13.194	3777	3780	3781	rBV3	1469	873	0.11%	0.014%
88	13.255	3797	3799	3801	rBV3	1125	589	0.07%	0.009%
89	13.316	3816	3818	3820	rBV3	1253	776	0.10%	0.012%
90	13.406	3844	3846	3851	rBV5	1299	943	0.12%	0.015%
91	13.557	3890	3893	3894	rBV3	1363	654	0.08%	0.010%
92	13.654	3919	3923	3927	rVB7	1268	849	0.11%	0.014%
93	13.689	3928	3934	3938	rBV9	2080	3043	0.38%	0.049%
94	13.734	3944	3948	3951	rVB5	1282	927	0.12%	0.015%
95	13.831	3972	3978	3981	rVB8	2148	1852	0.23%	0.030%
96	13.863	3986	3988	3991	rBV2	1149	902	0.11%	0.014%
97	13.937	4008	4011	4015	rBV6	1137	1041	0.13%	0.017%
98	13.985	4023	4026	4028	rBV4	1332	778	0.10%	0.012%
99	14.065	4049	4051	4053	rBV3	1369	626	0.08%	0.010%
100	15.213	4404	4408	4409	rBV3	1447	1066	0.13%	0.017%




Sum of corrected areas: 6257588

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
Data File : VV030855.D
Acq On : 25 Apr 2023 23:07
Operator : SY/MD
Sample : 02474-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AS5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

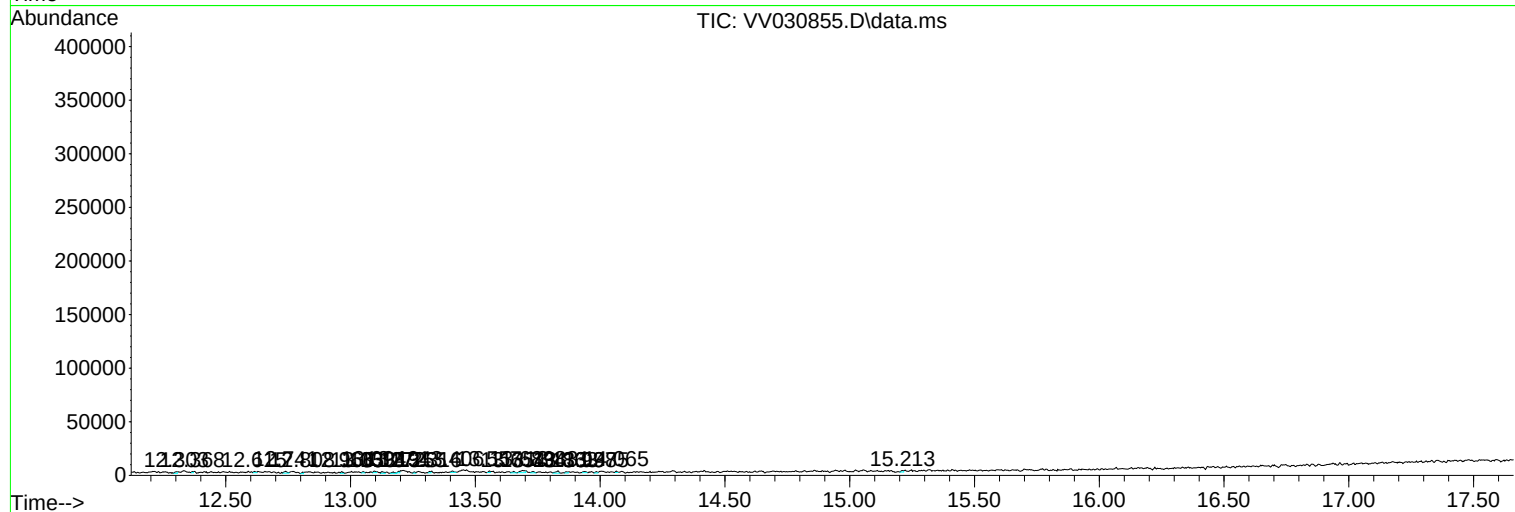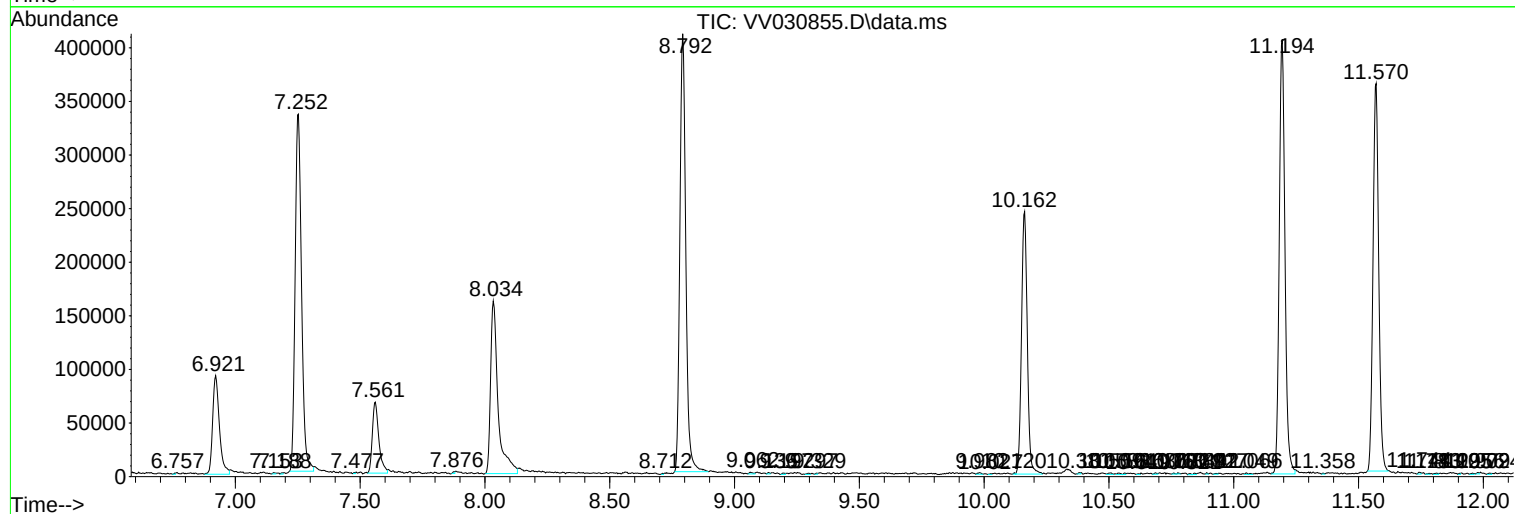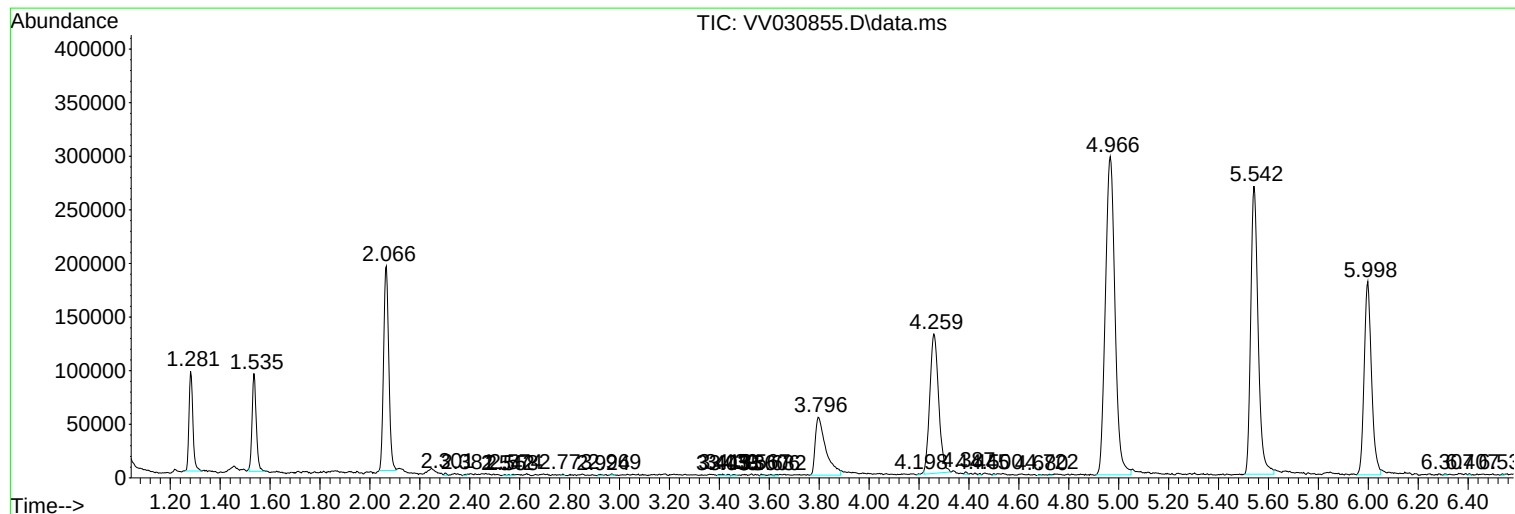

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
Data File : VV030855.D
Acq On : 25 Apr 2023 23:07
Operator : SY/MD
Sample : 02474-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AS5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042523\
Data File : VV030855.D
Acq On : 25 Apr 2023 23:07
Operator : SY/MD
Sample : 02474-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AS5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc